

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072418\
 Data File : BF107637.D
 Acq On : 24 Jul 2018 23:28
 Operator : JU/SJ
 Sample : J4031-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PLANTER-DOC-7

Quant Time: Jul 25 04:39:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	264562	20.00	ng	-0.01
21) Naphthalene-d8	8.25	136	1000874	20.00	ng	-0.01
38) Acenaphthene-d10	10.01	164	413606	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	725584	20.00	ng	0.00
75) Chrysene-d12	14.15	240	528535	20.00	ng	-0.01
86) Perylene-d12	15.69	264	460182	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	1575507	95.75	ng	0.00
7) Phenol-d6	6.61	99	1932180	97.79	ng	0.00
23) Nitrobenzene-d5	7.54	82	1174825	79.22	ng	-0.01
41) 2,4,6-Tribromophenol	10.81	330	448729	95.41	ng	-0.01
44) 2-Fluorobiphenyl	9.32	172	1984996	81.19	ng	-0.01
78) Terphenyl-d14	13.09	244	1666041	80.70	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.72	163	423457	13.585	ng	98
74) Fluoranthene	12.72	202	100826	2.657	ng	95
77) Pyrene	12.95	202	96042	2.657	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072418\
Data File : BF107637.D
Acq On : 24 Jul 2018 23:28
Operator : JU/SJ
Sample : J4031-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PLANTER-DOC-7

Quant Time: Jul 25 04:39:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

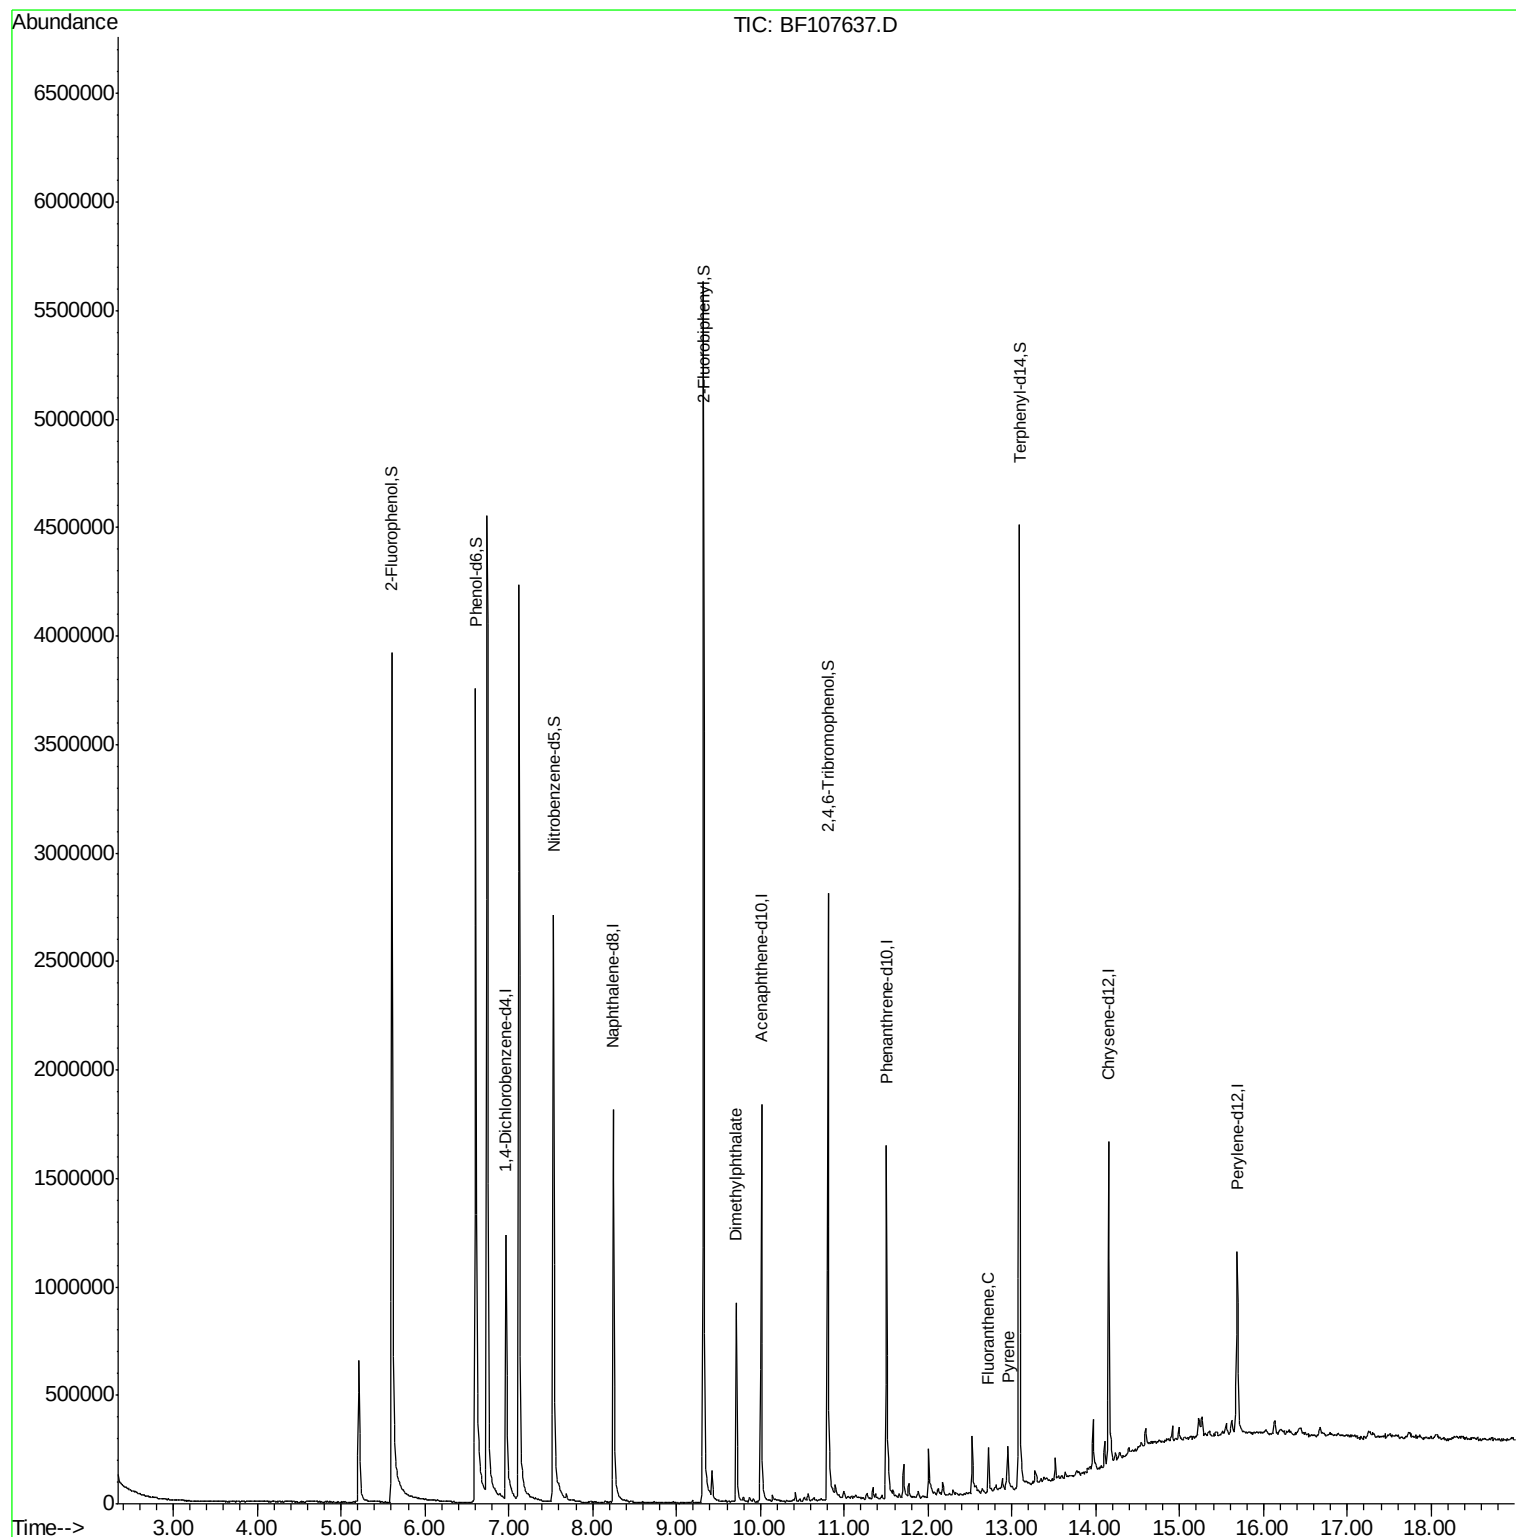

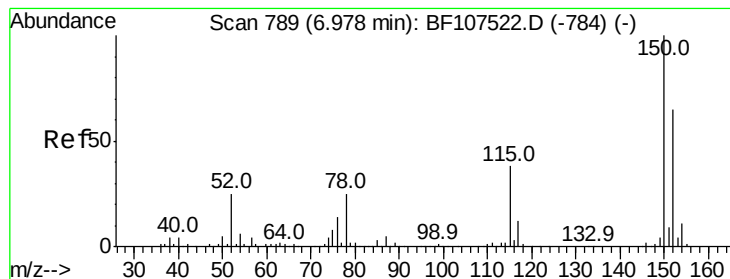


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 787
Delta R.T. -0.01 min
Lab File: BF107637.D
Acq: 24 Jul 2018 23:28

Instrument :
BNA_F
ClientSampleId :
PLANTER-DOC-7

Tot Ion:152 Resp: 264562
Ion Ratio Lower Upper
152 100
150 159.2 124.6 186.8
115 63.1 50.1 75.1

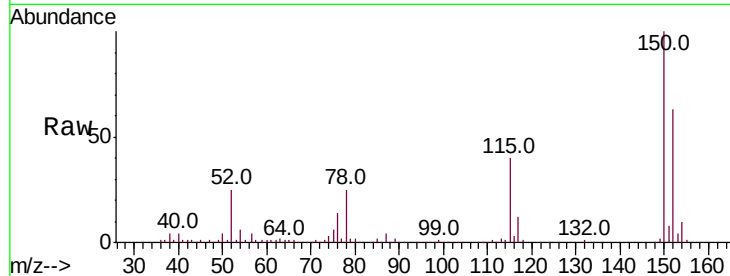


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

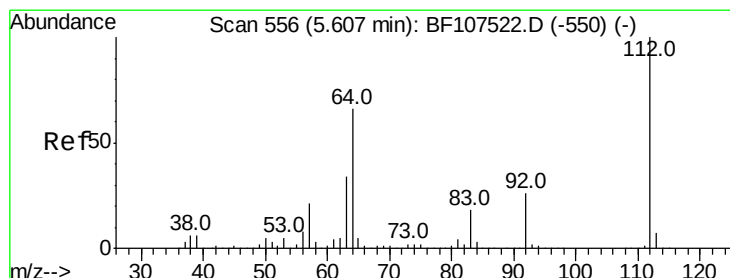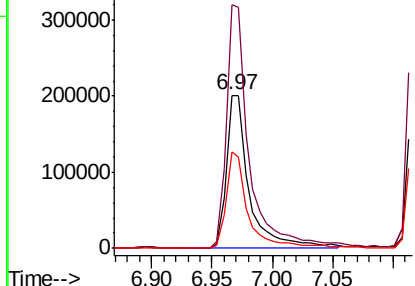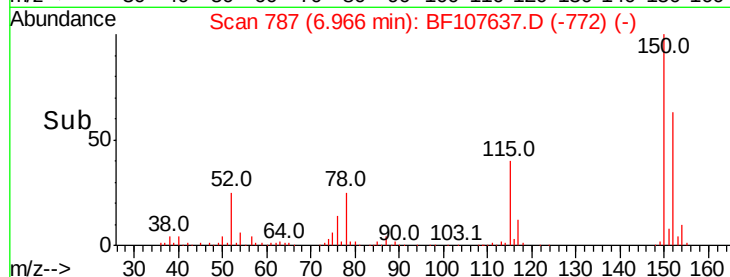



#5


2-Fluorophenol
Concen: 95.747 ng
RT: 5.61 min Scan# 556
Delta R.T. 0.00 min
Lab File: BF107637.D
Acq: 24 Jul 2018 23:28

Tgt Ion:112 Resp: 1575507
Ion Ratio Lower Upper
112 100
64 66.5 47.9 71.9
63 34.7 23.7 35.5

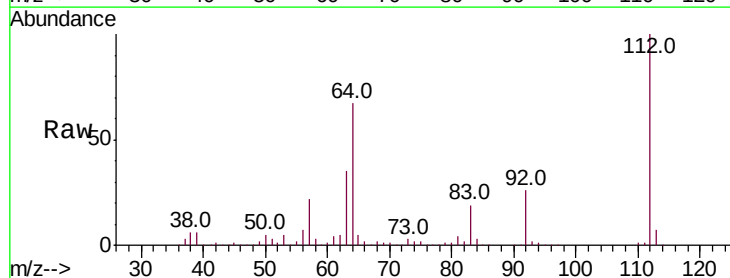

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

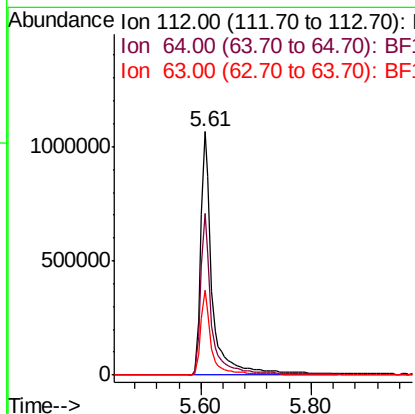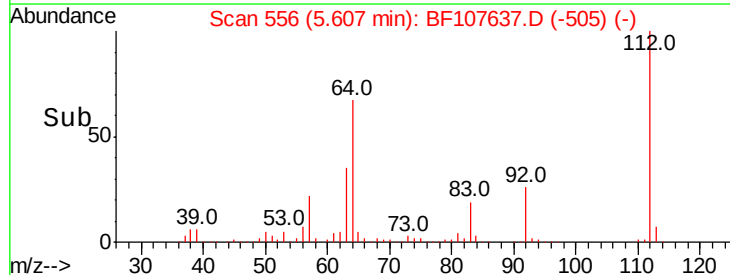

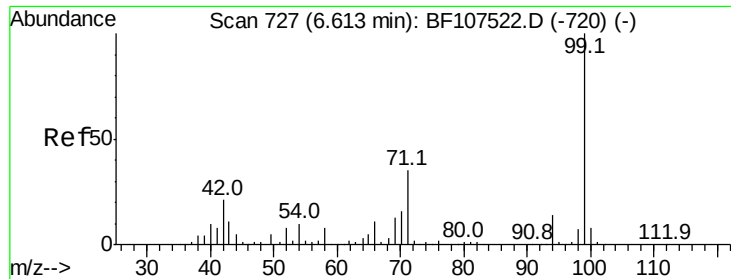

#7

Phenol-d6

Concen: 97.793 ng

RT: 6.61 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28

Instrument :

BNA_F

ClientSampleId :

PLANTER-DOC-7


Tot Ion: 99 Resp: 1932180

Ion Ratio Lower Upper




99 100

42 19.6 14.5 21.7

71 36.8 25.4 38.0

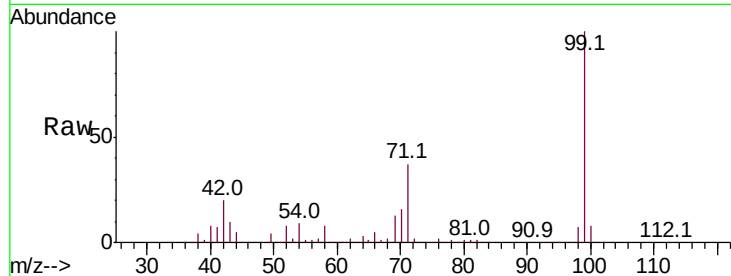

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

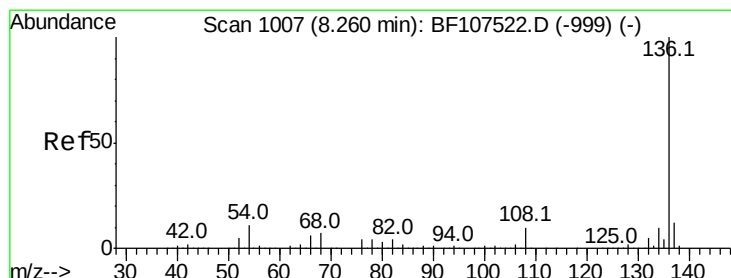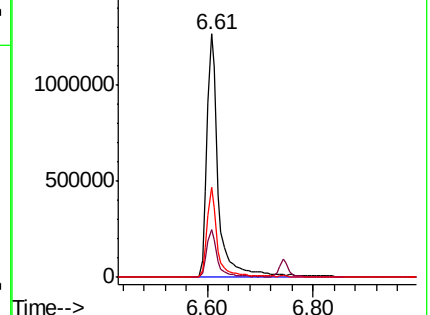

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1005

Delta R.T. -0.01 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28

Tgt Ion:136 Resp: 1000874


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 10.0 6.6 9.8#

68 5.6 5.0 7.4

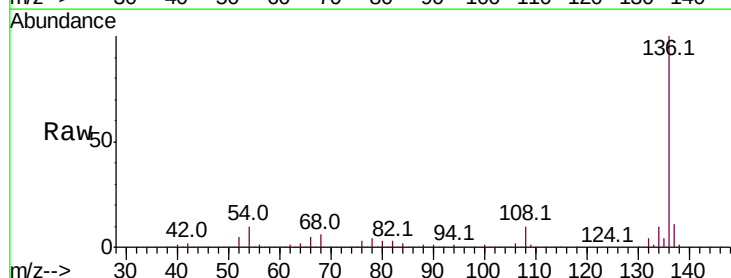

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

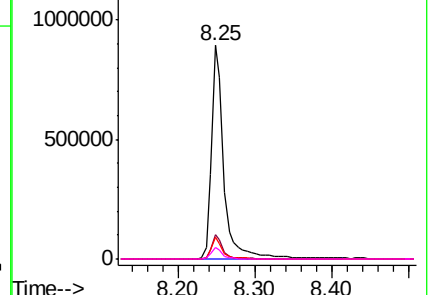







#23
Nitrobenzene-d5
Concen: 79.217 ng
RT: 7.54 min Scan# 884
Delta R.T. -0.01 min
Lab File: BF107637.D
Acq: 24 Jul 2018 23:28

Instrument :
BNA_F
ClientSampleId :
PLANTER-DOC-7

Tot Ion: 82 Resp: 1174825
Ion Ratio Lower Upper
82 100
128 48.3 36.1 54.1
54 59.1 41.4 62.2

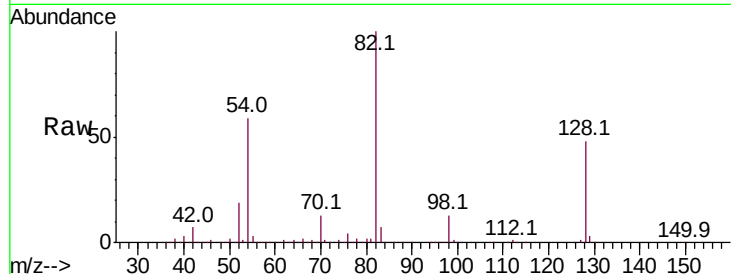


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

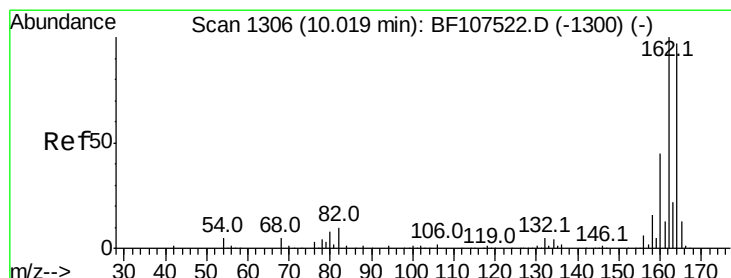
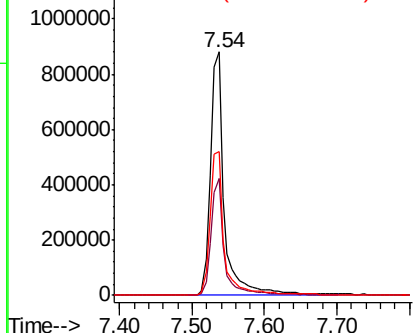



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.01 min Scan# 1305
Delta R.T. -0.01 min
Lab File: BF107637.D
Acq: 24 Jul 2018 23:28

Tgt Ion:164 Resp: 413606
Ion Ratio Lower Upper
164 100
162 104.3 86.1 129.1
160 48.1 38.3 57.5

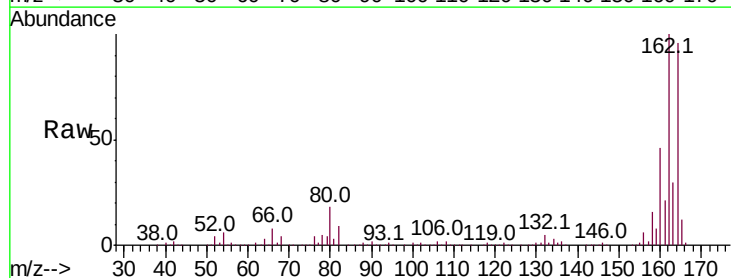

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

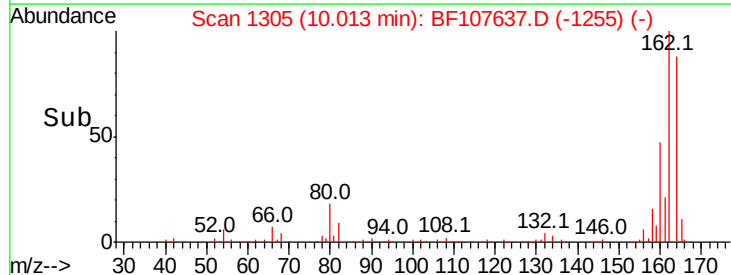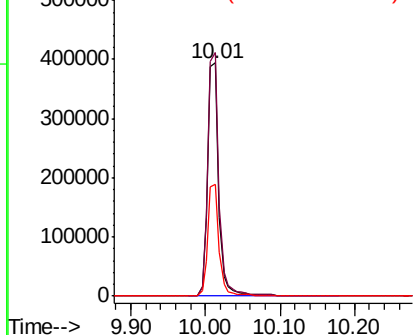


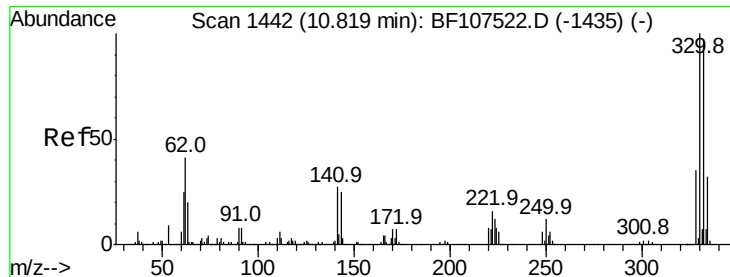




#41
 2,4,6-Tribromophenol
 Concen: 95.406 ng
 RT: 10.81 min Scan# 1440
 Delta R.T. -0.01 min
 Lab File: BF107637.D
 Acq: 24 Jul 2018 23:28

Instrument :
 BNA_F
 ClientSampleId :
 PLANTER-DOC-7

Tot Ion:330 Resp: 448729
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.0 115.6
 141 28.6 29.9 44.9#

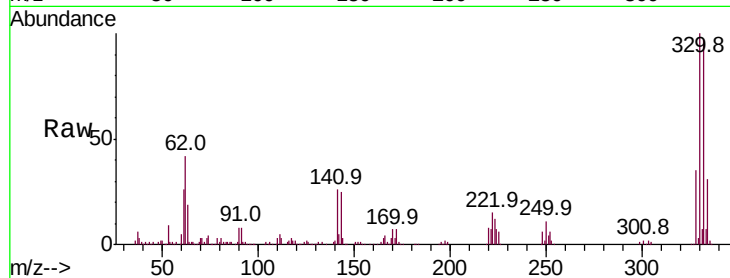


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

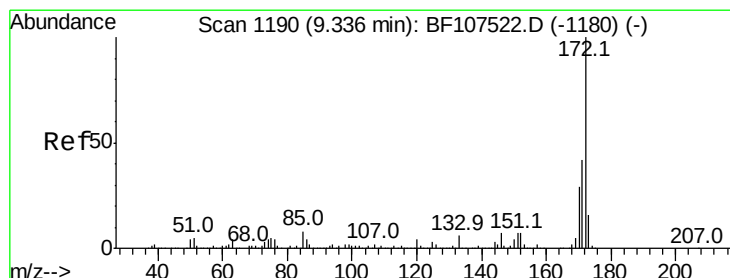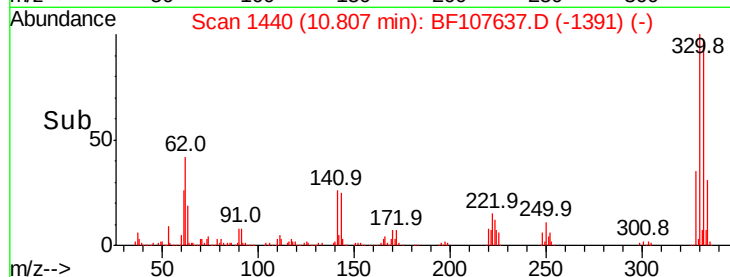
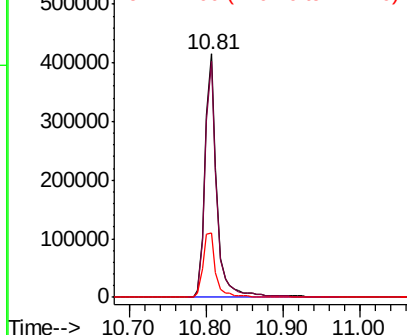



#44
 2-Fluorobiphenyl
 Concen: 81.187 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. -0.01 min
 Lab File: BF107637.D
 Acq: 24 Jul 2018 23:28

Tgt Ion:172 Resp: 1984996
 Ion Ratio Lower Upper
 172 100
 171 38.3 29.7 44.5
 170 26.0 19.6 29.4

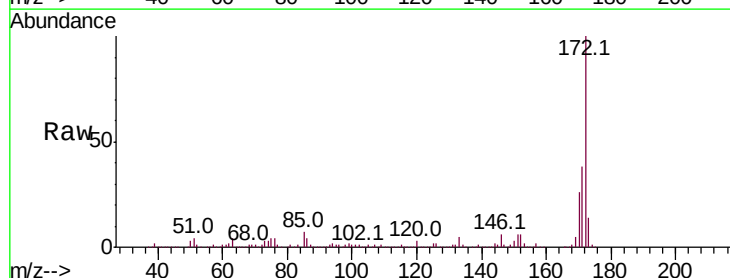

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

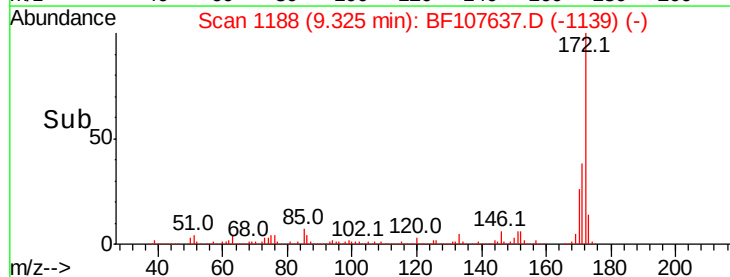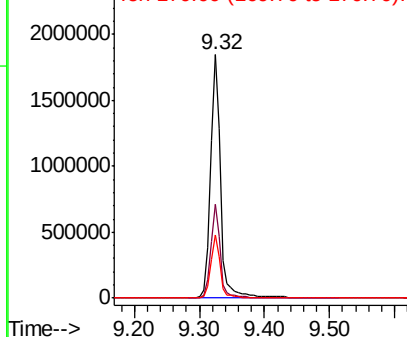



#49

Dimethylphthalate

Concen: 13.585 ng

RT: 9.72 min Scan# 1255

Delta R.T. -0.02 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28

Instrument :

BNA_F

ClientSampleId :

PLANTER-DOC-7


Tot Ion:163 Resp: 423457

Ion Ratio Lower Upper

163 100

194 3.7 2.7 4.1




164 9.1 8.2 12.2

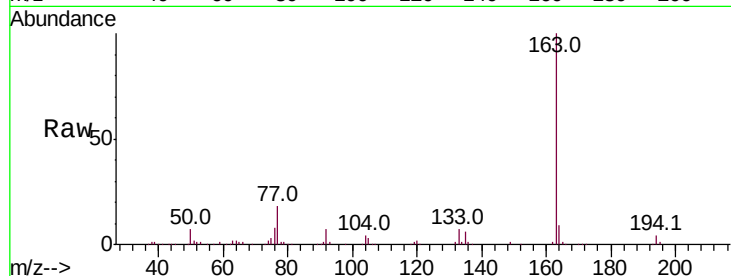

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

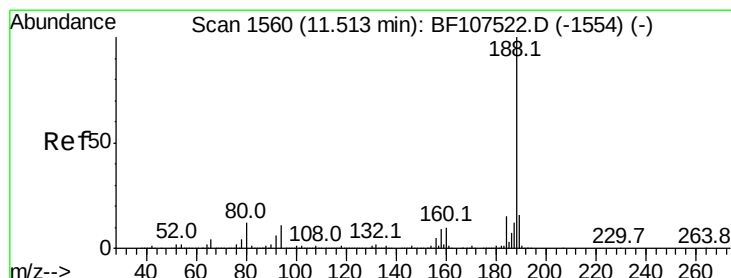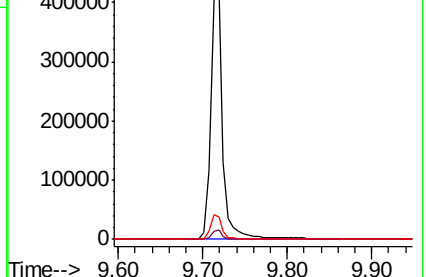

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.51 min Scan# 1559

Delta R.T. -0.01 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28


Tgt Ion:188 Resp: 725584

Ion Ratio Lower Upper

188 100

94 8.6 8.5 12.7



80 9.7 9.2 13.8

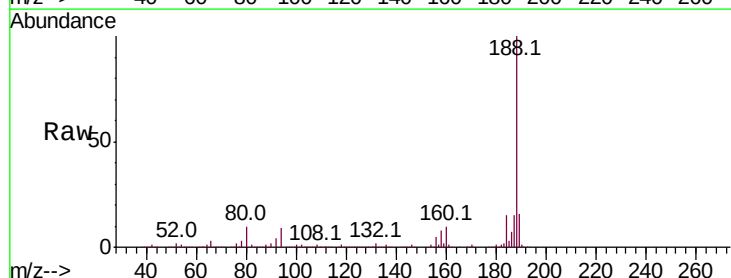


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

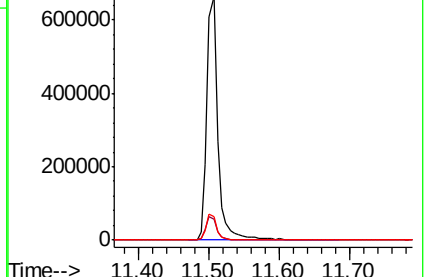

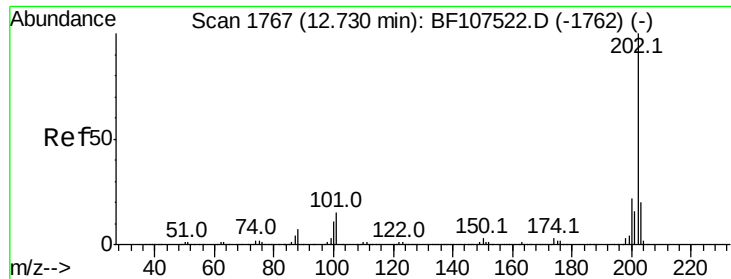

#74

Fluoranthene

Concen: 2.657 ng

RT: 12.72 min Scan# 1765

Delta R.T. -0.01 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28

Instrument :

BNA_F

ClientSampleId :

PLANTER-DOC-7


Tot Ion:202 Resp: 100826

Ion Ratio Lower Upper

202 100

101 11.5 0.0 34.1




203 16.6 0.0 38.1

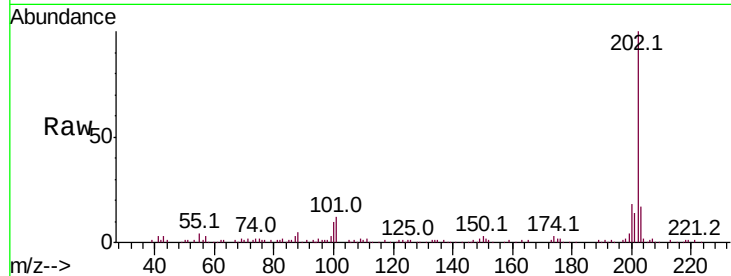

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

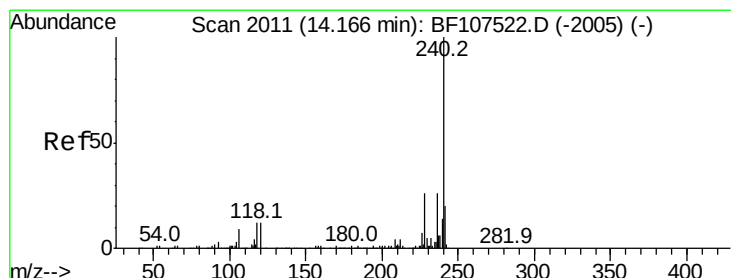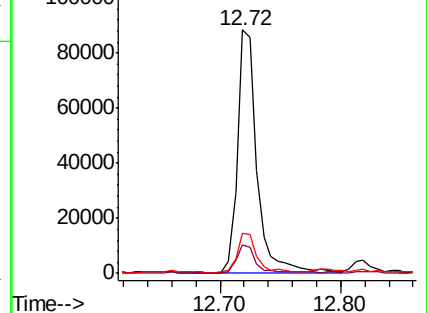

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2009

Delta R.T. -0.01 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28


Tgt Ion:240 Resp: 528535

Ion Ratio Lower Upper

240 100

120 11.0 9.5 14.3



236 25.8 20.7 31.1

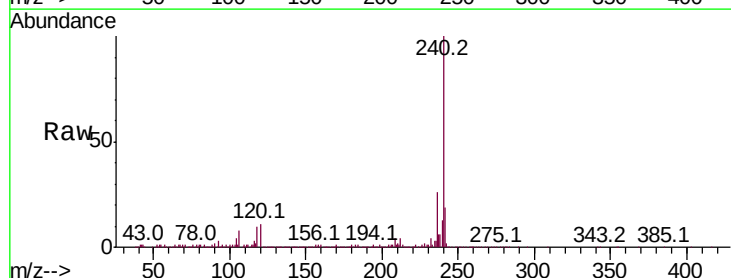


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

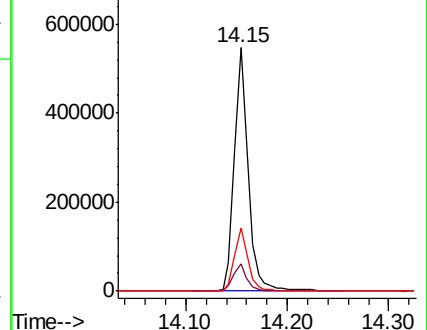



#77

Pvrene

Concen: 2.657 ng

RT: 12.95 min Scan# 1805

Delta R.T. -0.01 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28

Instrument :

BNA_F

ClientSampleId :

PLANTER-DOC-7


Tot Ion:202 Resp: 96042

Ion Ratio Lower Upper

202 100

200 18.6 17.4 26.2




203 16.5 14.3 21.5

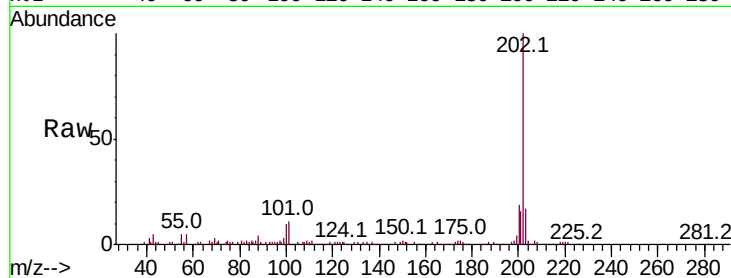

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

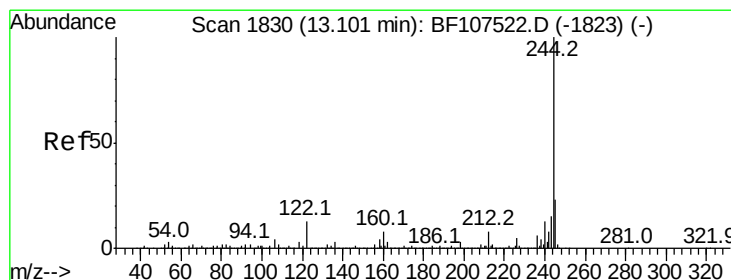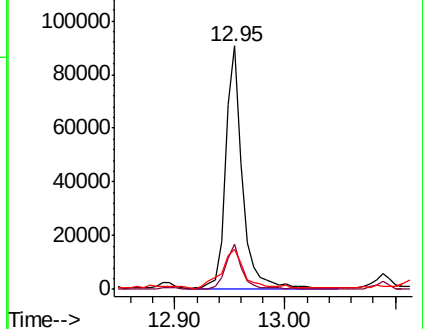

#78

Terphenyl-d14

Concen: 80.699 ng

RT: 13.09 min Scan# 1828

Delta R.T. -0.01 min

Lab File: BF107637.D

Acq: 24 Jul 2018 23:28


Tgt Ion:244 Resp: 1666041

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0



122 11.9 11.0 16.4

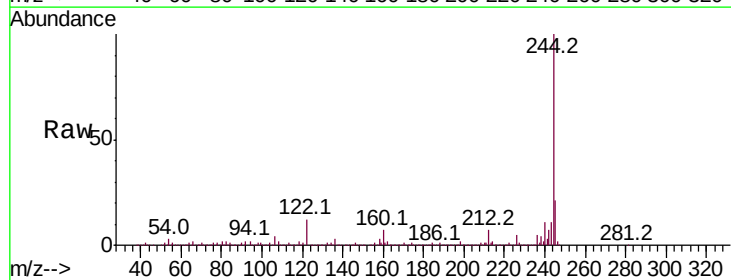


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

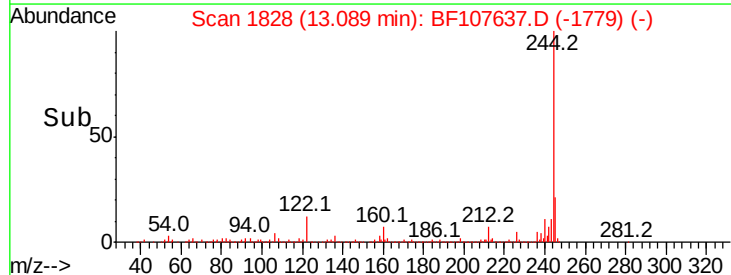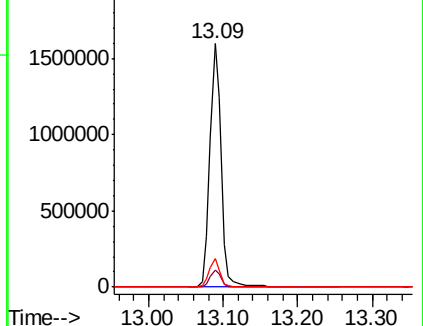


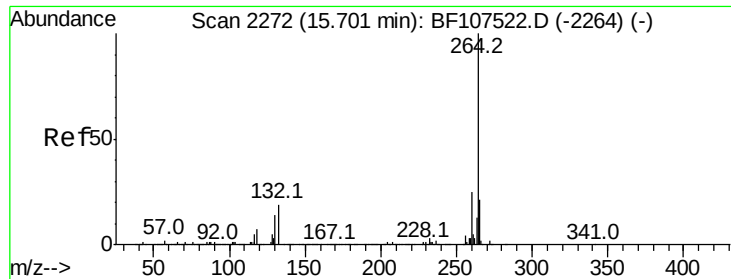

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.69 min Scan# 2270
Delta R.T. -0.01 min
Lab File: BF107637.D
Acq: 24 Jul 2018 23:28

Instrument :
BNA_F
ClientSampleId :
PLANTER-DOC-7

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.2	28.8
265	22.3	17.5	26.3

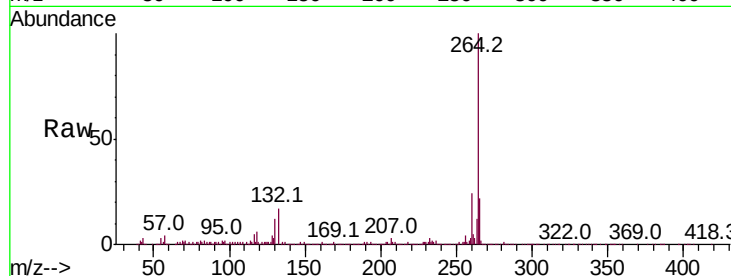

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

