


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072418\
 Data File : BF107612.D
 Acq On : 24 Jul 2018 11:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 16:29:27 2018

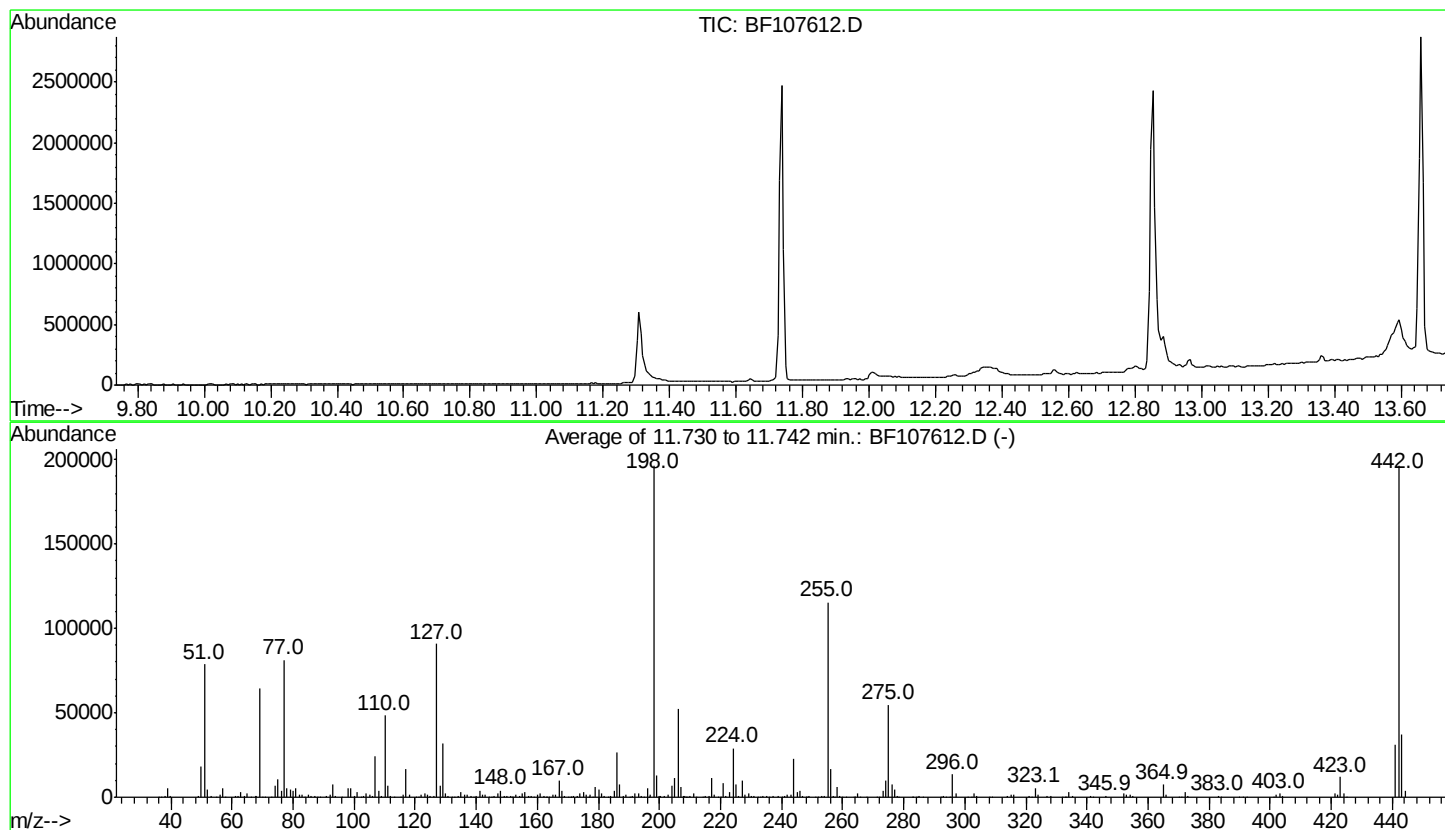

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	78561	PASS
68	69	0.00	2	0.7	471	PASS
69	198	0.00	100	32.8	64341	PASS
70	69	0.00	2	0.5	315	PASS
127	198	10	80	46.3	90890	PASS
197	198	0.00	2	0.8	1509	PASS
198	198	100	100	100.0	196341	PASS
199	198	5	9	6.4	12639	PASS
275	198	10	60	27.9	54821	PASS
365	198	1	100	3.7	7257	PASS
441	198	0.01	100	15.9	31264	PASS
442	198	50	100	99.9	196237	PASS
443	442	15	24	19.0	37266	PASS