
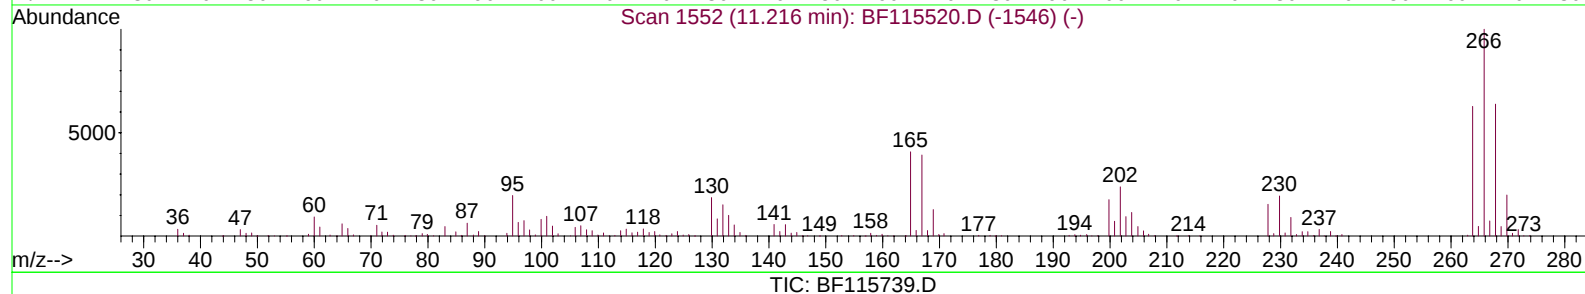
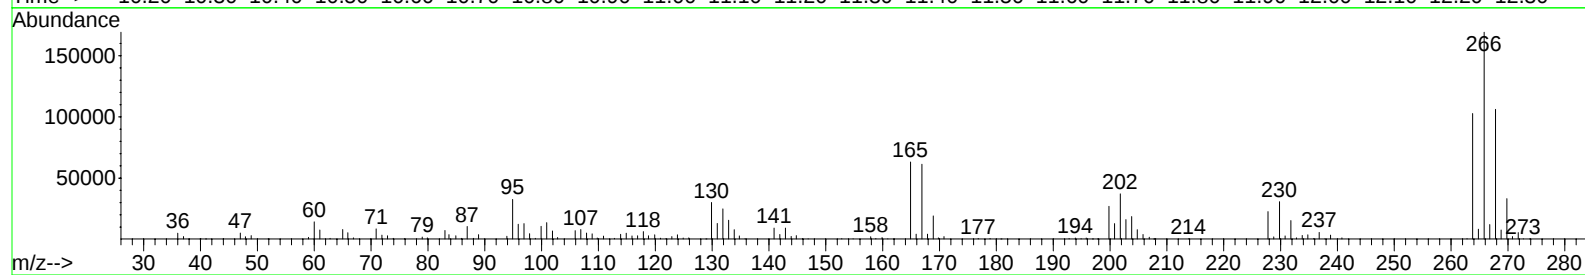


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072419\
Data File : BF115739.D
Acq On : 24 Jul 2019 8:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 18:03:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

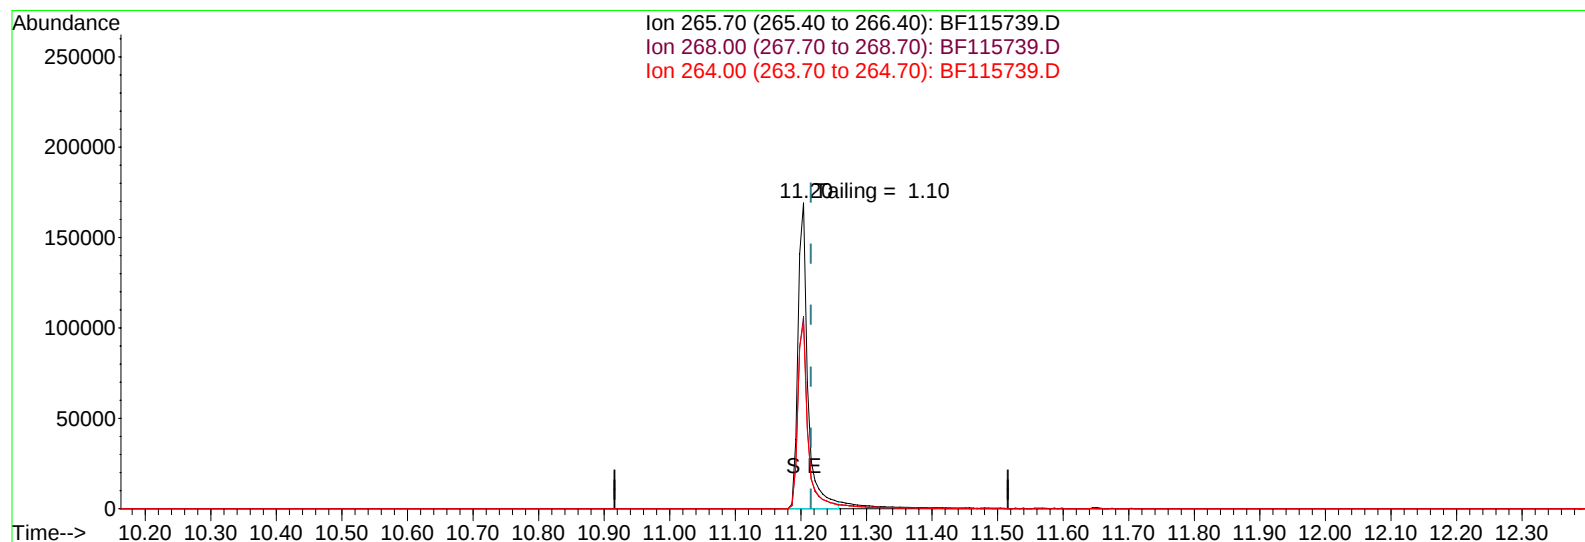

(70) Pentachlorophenol (C)




11.204min (-0.012) 205544.59ng

response 188673

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.79
264.00	63.30	60.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072419\
Data File : BF115739.D
Acq On : 24 Jul 2019 8:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 18:03:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 14:03:52 2019
Response via : Initial Calibration

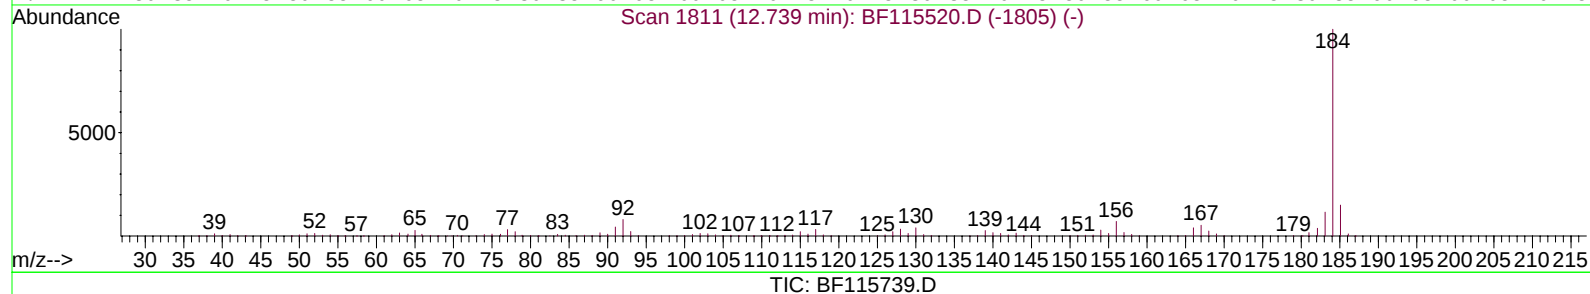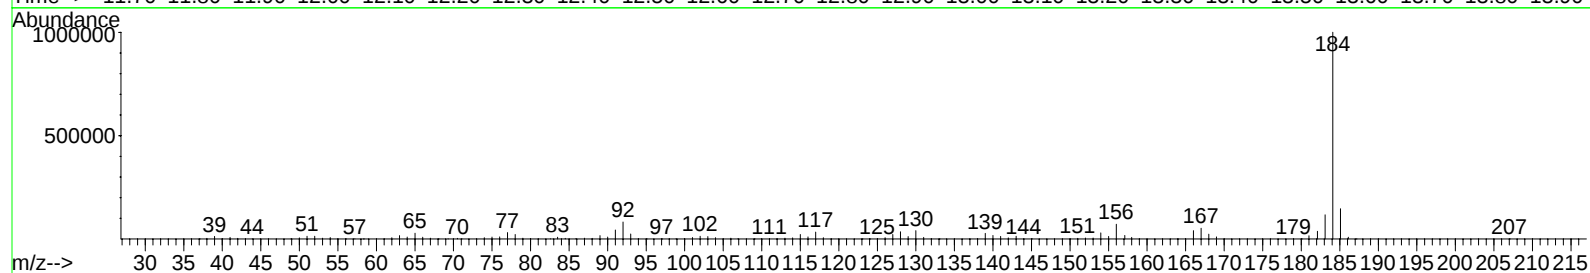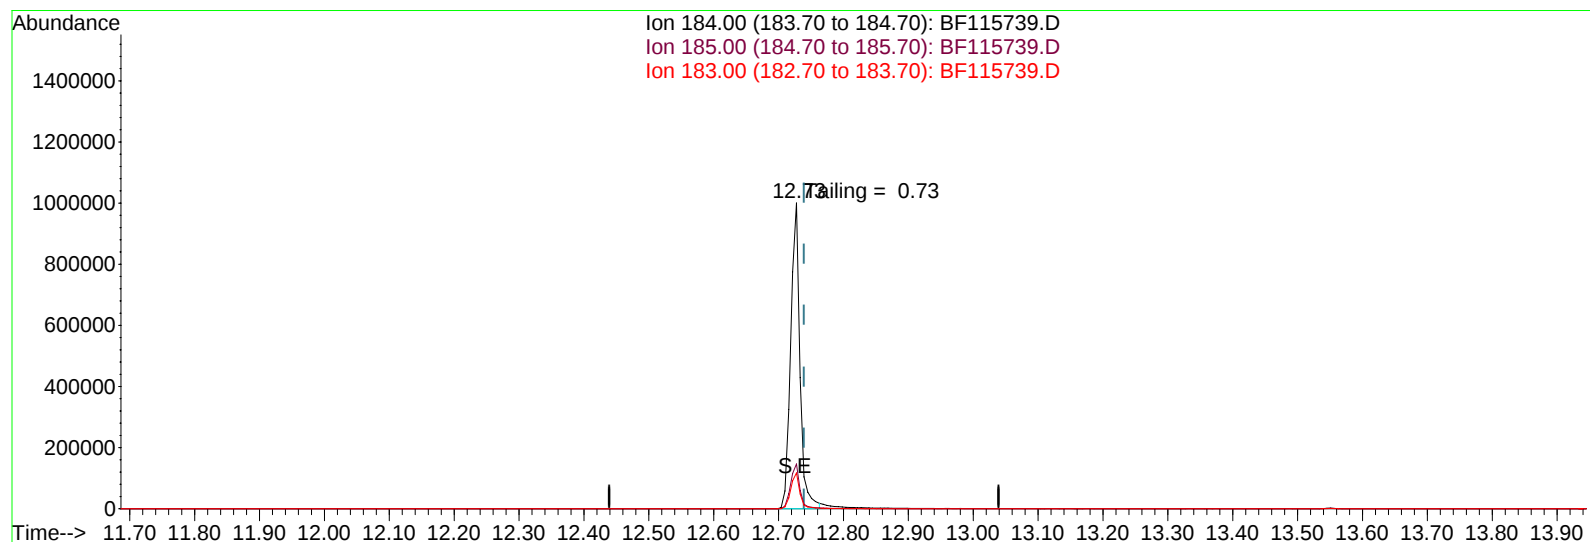

(77) Benzidine

12.727min (-0.012) 0.00ng

response 1034686

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.63
183.00	11.60	11.75
0.00	0.00	0.00