


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072419\
 Data File : BF115739.D
 Acq On : 24 Jul 2019 8:23
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 25 13:16:07 2019

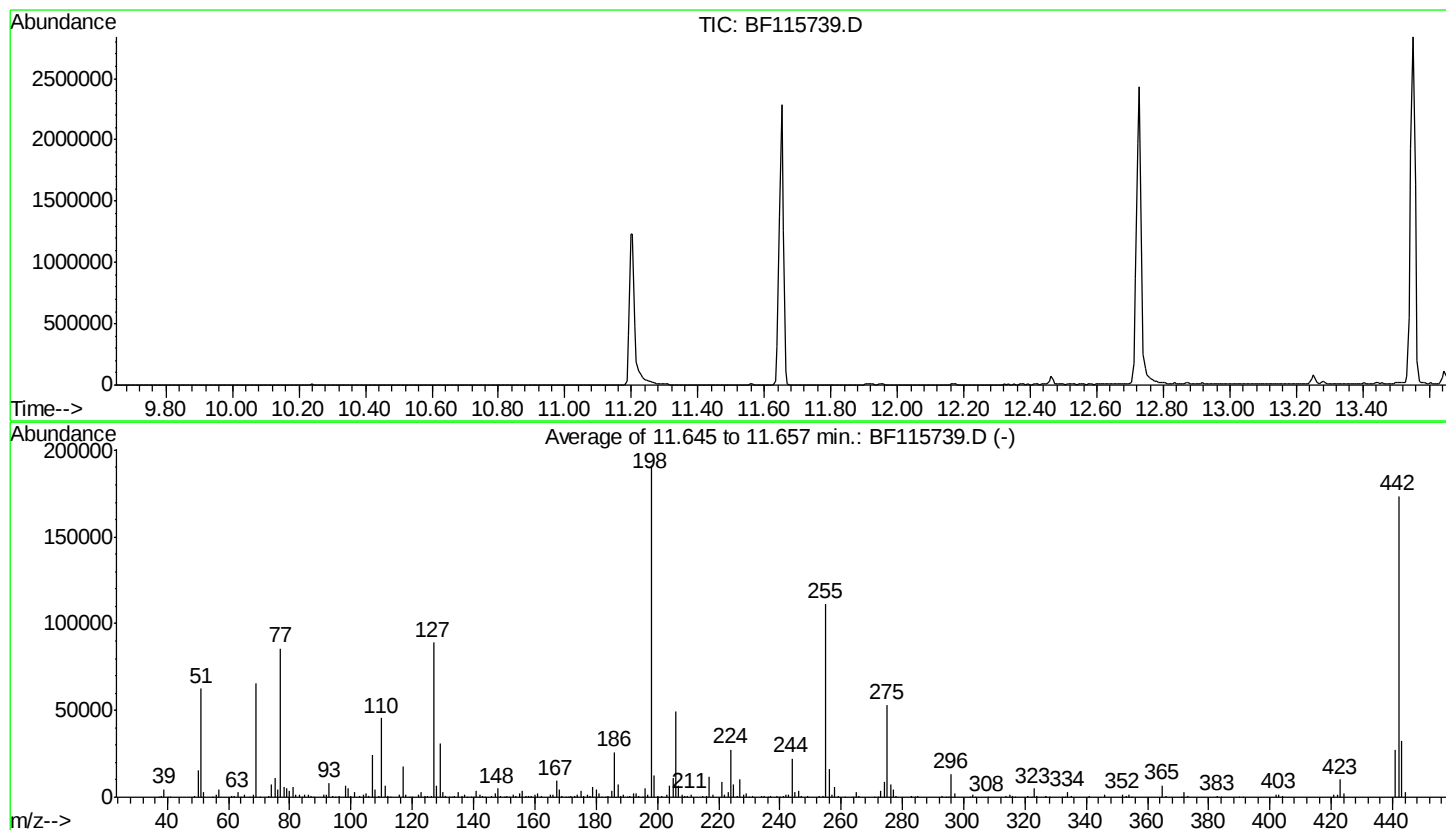

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	62488	PASS
68	69	0.00	2	1.8	1158	PASS
69	198	0.00	100	34.5	65864	PASS
70	69	0.00	2	0.5	325	PASS
127	198	10	80	46.7	89216	PASS
197	198	0.00	2	0.6	1175	PASS
198	198	100	100	100.0	191040	PASS
199	198	5	9	6.7	12732	PASS
275	198	10	60	27.9	53288	PASS
365	198	1	100	3.5	6655	PASS
441	198	0.01	100	14.2	27046	PASS
442	198	50	100	90.8	173536	PASS
443	442	15	24	18.8	32568	PASS