
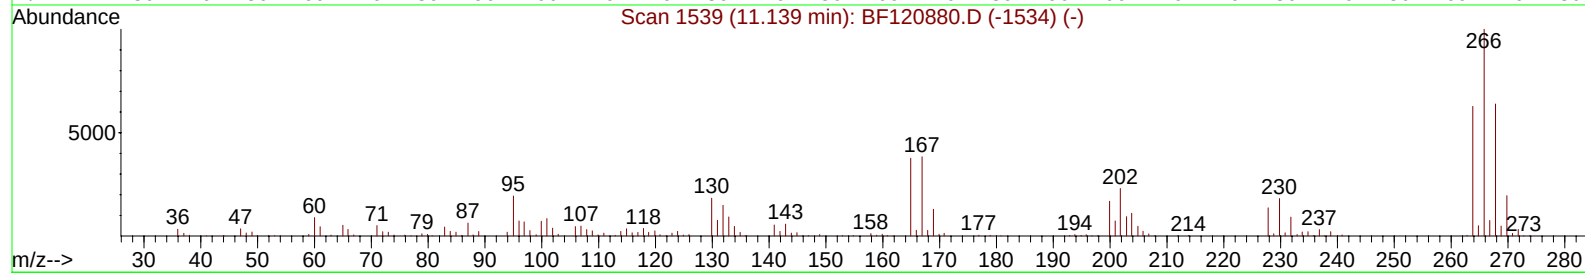
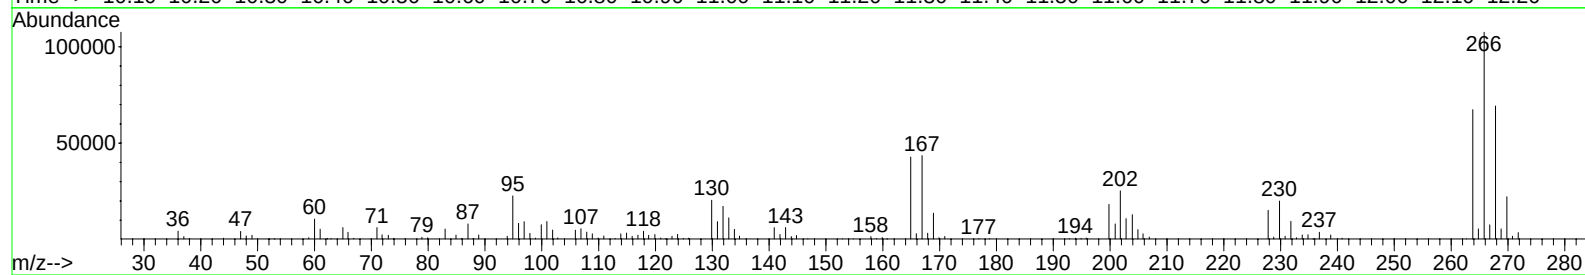


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072420\
 Data File : BF120996.D
 Acq On : 24 Jul 2020 11:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 17:01:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

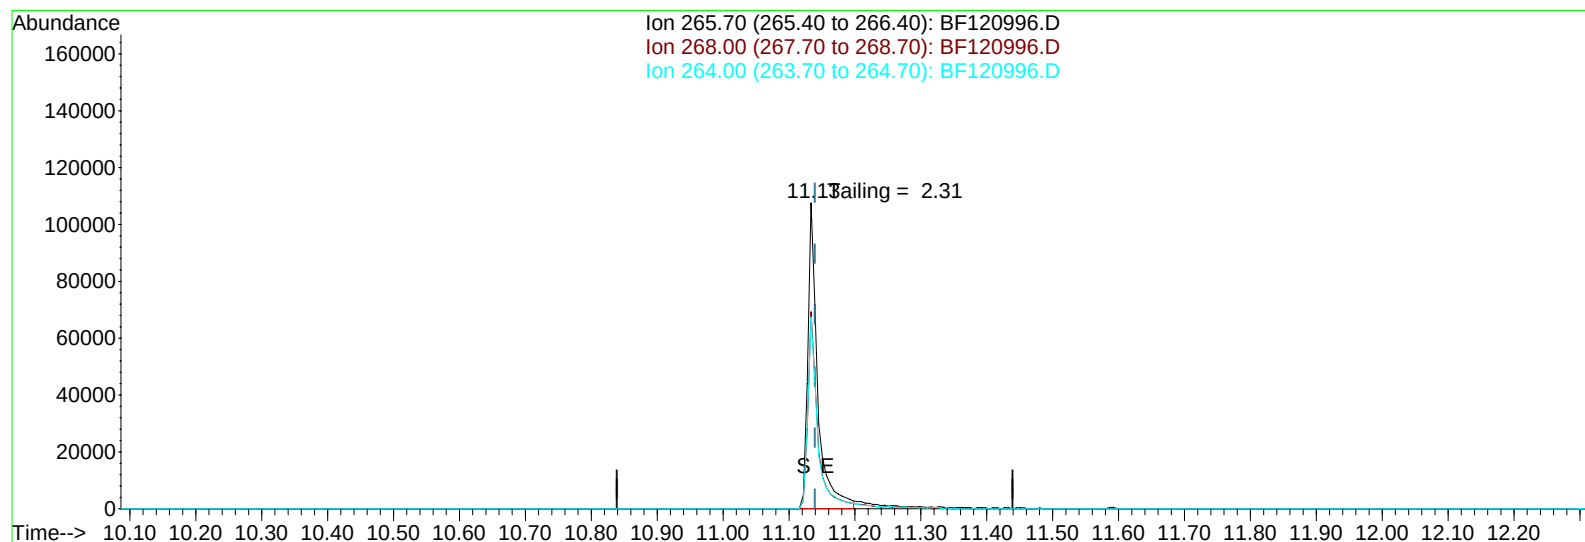

TIC: BF120996.D

(70) Pentachlorophenol (C)




11.133min (-0.006) 40923.64ng

response 121584

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.39
264.00	62.70	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072420\
Data File : BF120996.D
Acq On : 24 Jul 2020 11:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 17:01:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

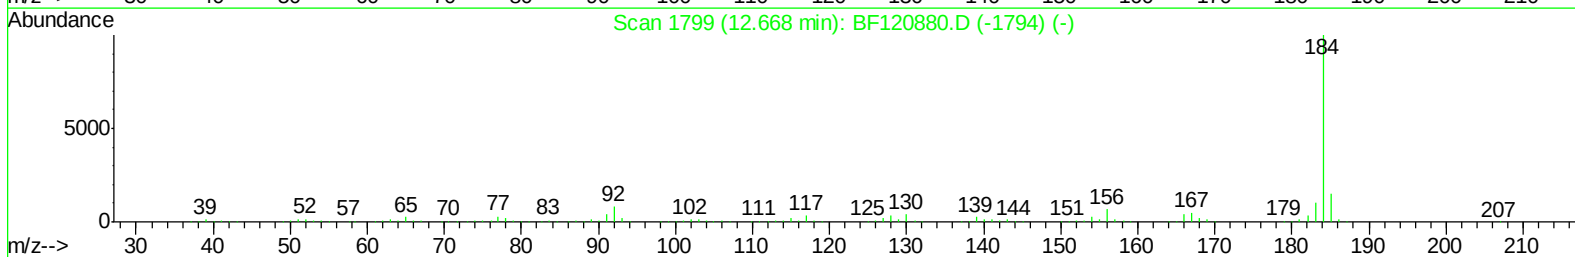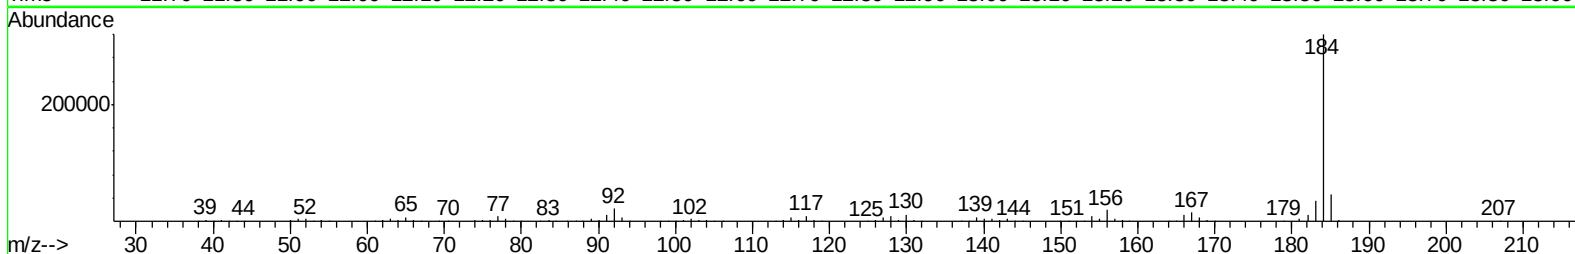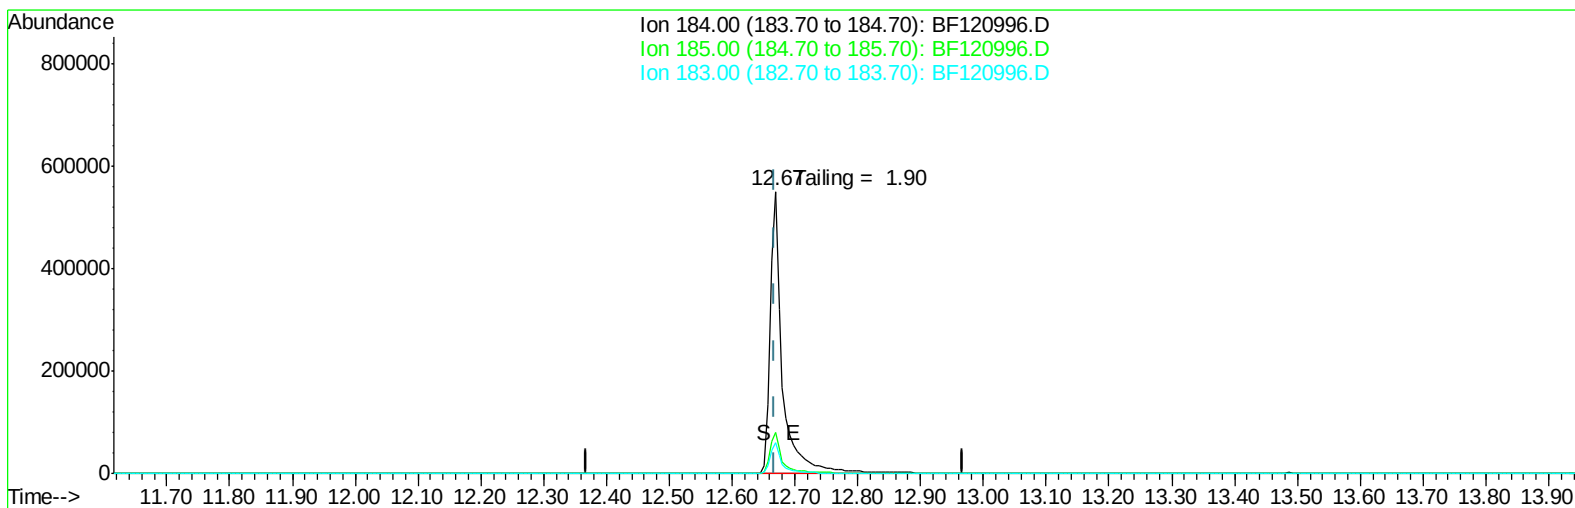

TIC: BF120996.D

(77) Benzidine

12.669min (+0.000) 0.00ng

response 753232

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.67
183.00	10.60	10.74
0.00	0.00	0.00