

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072421\
 Data File : BF124738.D
 Acq On : 24 Jul 2021 9:53
 Operator : JU/CG
 Sample : PB137907BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137907BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.492	574	579	582	rBB	161525	164084	47.20%	8.709%
2	6.492	743	749	752	rBB	161437	160874	46.28%	8.539%
3	6.869	810	813	816	rBB	60524	45474	13.08%	2.414%
4	7.028	835	840	843	rBB	255685	220543	63.44%	11.706%
5	7.433	903	909	911	rBB	158609	168688	48.53%	8.953%
6	8.151	1026	1031	1034	rBB	69052	62806	18.07%	3.334%
7	9.227	1208	1214	1217	rBB	333438	336234	96.72%	17.846%
8	9.904	1325	1329	1332	rBB	84877	71794	20.65%	3.811%
9	10.692	1459	1463	1466	rBB	147873	126406	36.36%	6.709%
10	11.392	1578	1582	1585	rVB	96366	73700	21.20%	3.912%
11	12.986	1847	1853	1856	rBV	368261	347624	100.00%	18.451%
12	14.027	2027	2030	2034	rBB	65560	57006	16.40%	3.026%
13	15.498	2275	2280	2285	rBB	40079	48819	14.04%	2.591%




Sum of corrected areas: 1884052

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072421\
Data File : BF124738.D
Acq On : 24 Jul 2021 9:53
Operator : JU/CG
Sample : PB137907BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137907BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

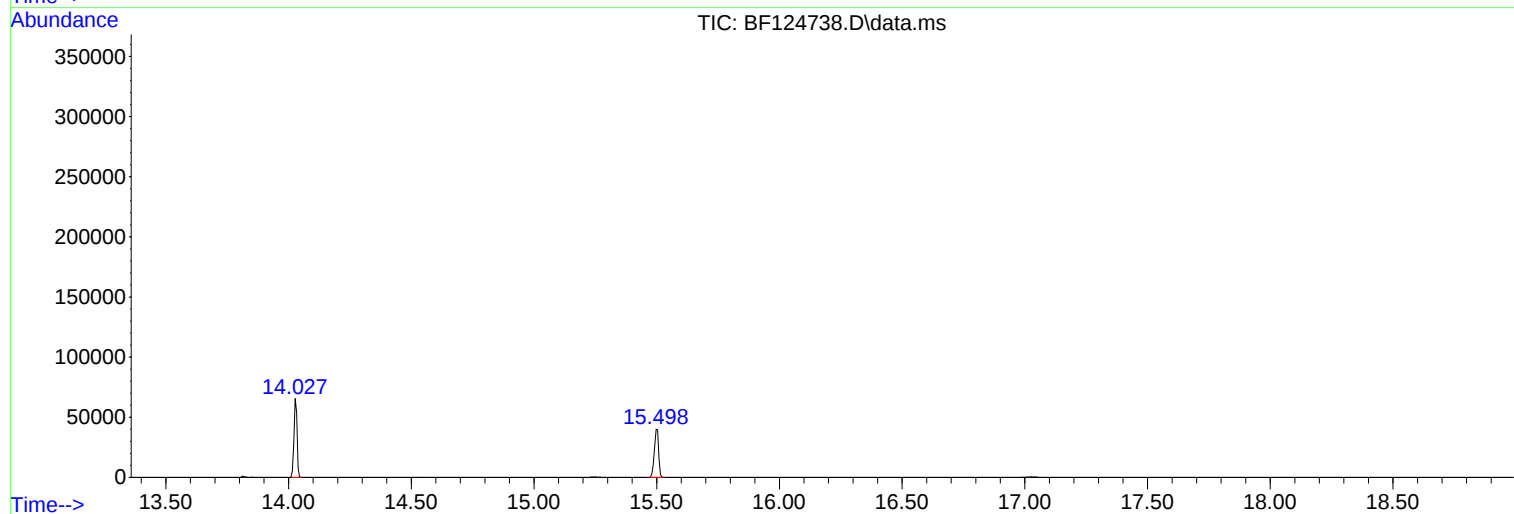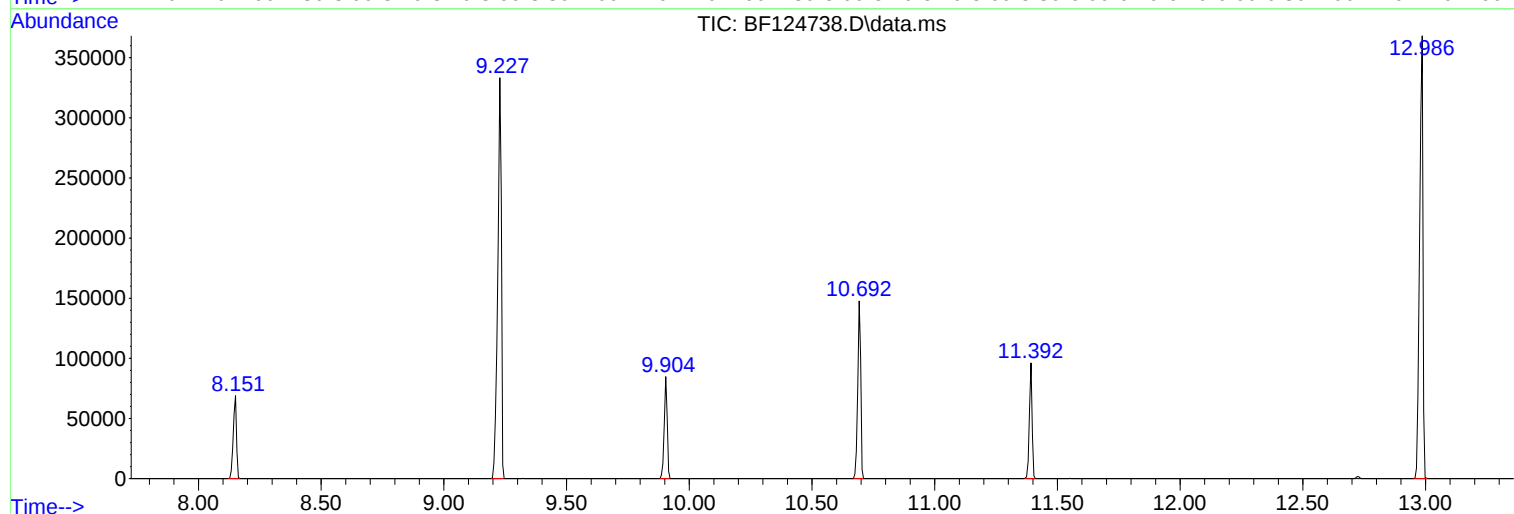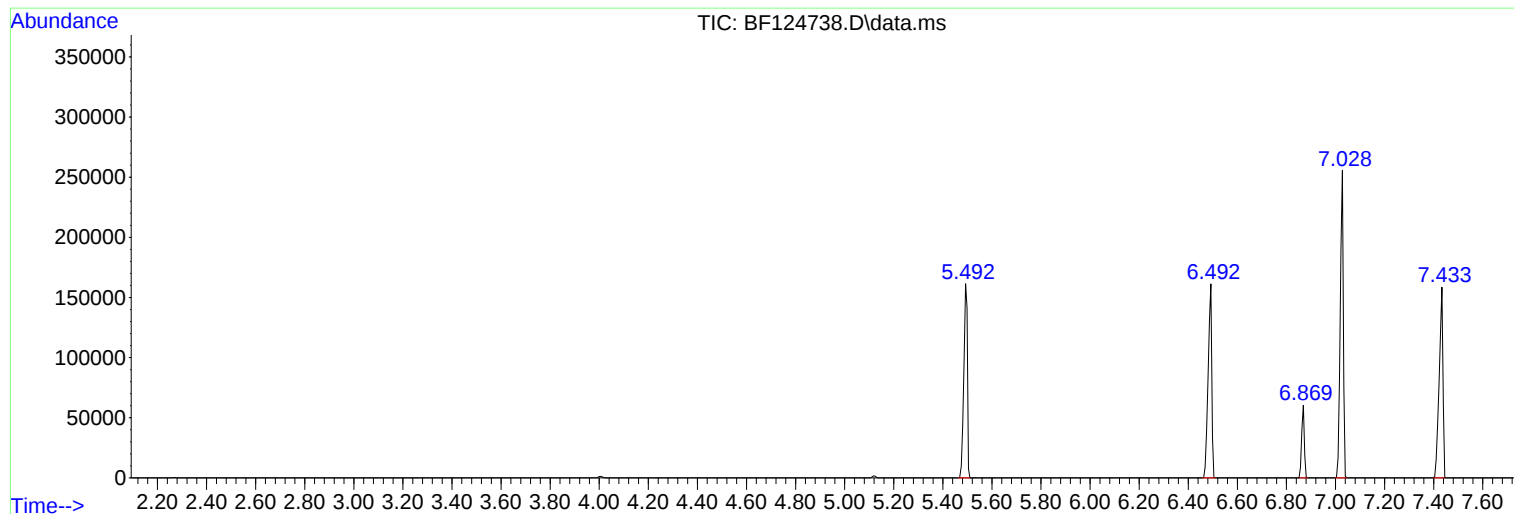

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072421\
Data File : BF124738.D
Acq On : 24 Jul 2021 9:53
Operator : JU/CG
Sample : PB137907BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137907BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072421\
Data File : BF124738.D
Acq On : 24 Jul 2021 9:53
Operator : JU/CG
Sample : PB137907BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137907BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------