


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072421\
 Data File : BF124736.D
 Acq On : 24 Jul 2021 8:50
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 15:28:57 2021

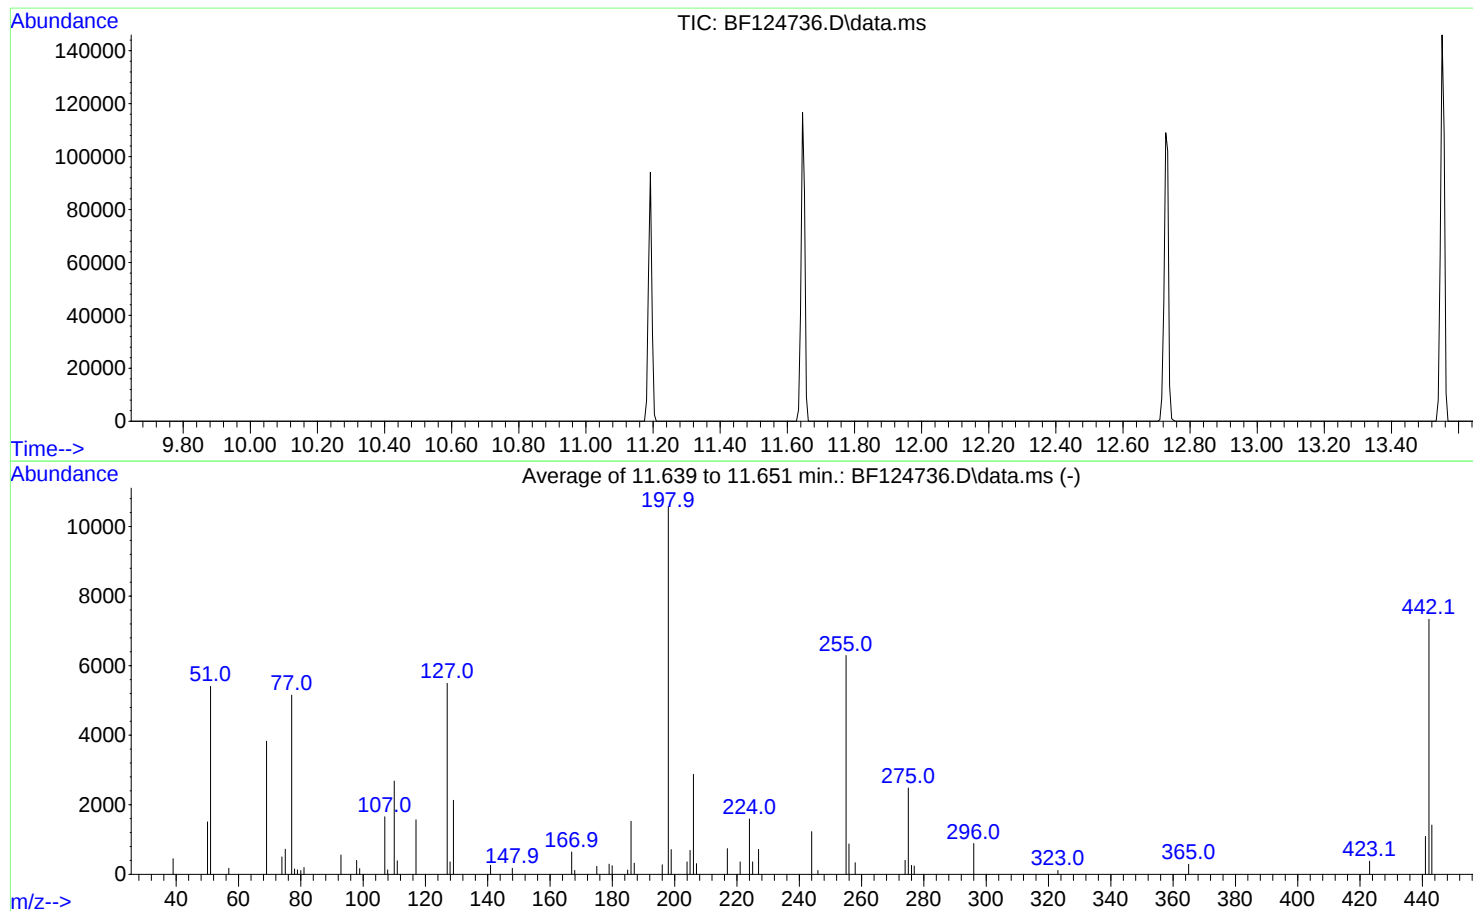




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.1	5407	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.2	3825	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	5493	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10575	PASS
199	198	5	9	6.8	714	PASS
275	198	10	60	23.5	2482	PASS
365	198	1	100	2.8	291	PASS
441	198	0.01	100	10.3	1092	PASS
442	442	50	100	100.0	7334	PASS
443	442	15	24	19.3	1416	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072421\  
Data File : BF124736.D  
Acq On    : 24 Jul 2021    8:50  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 26 07:06:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

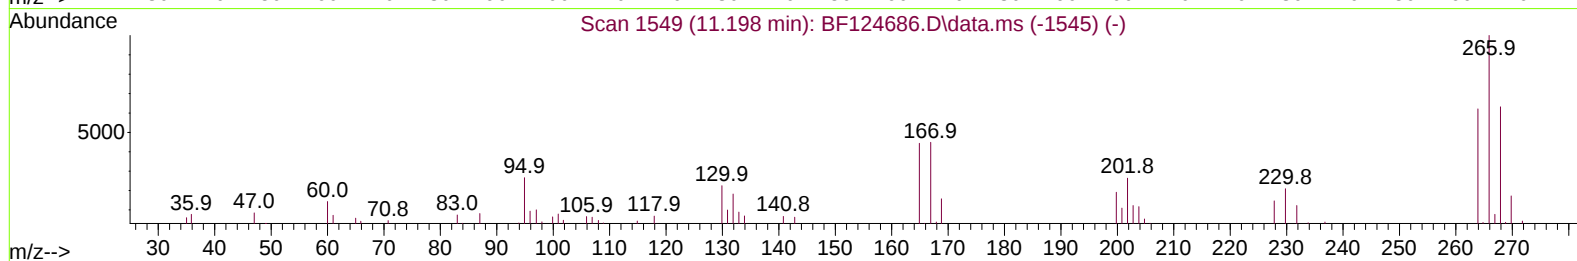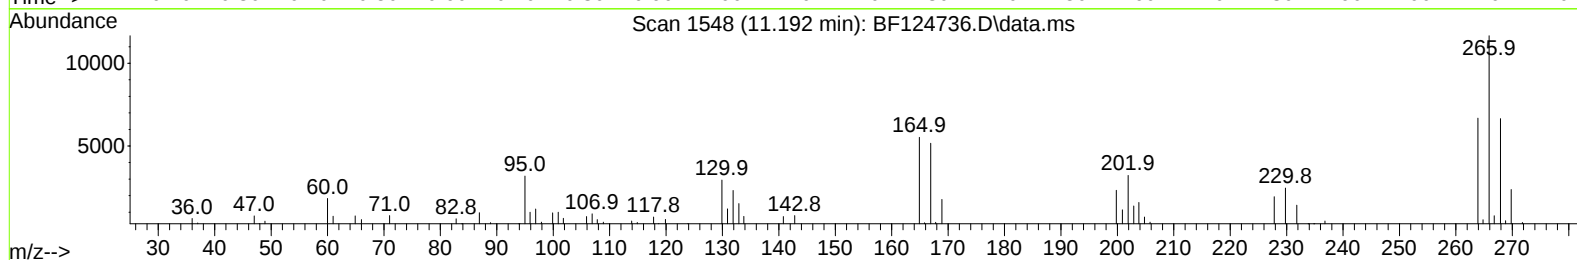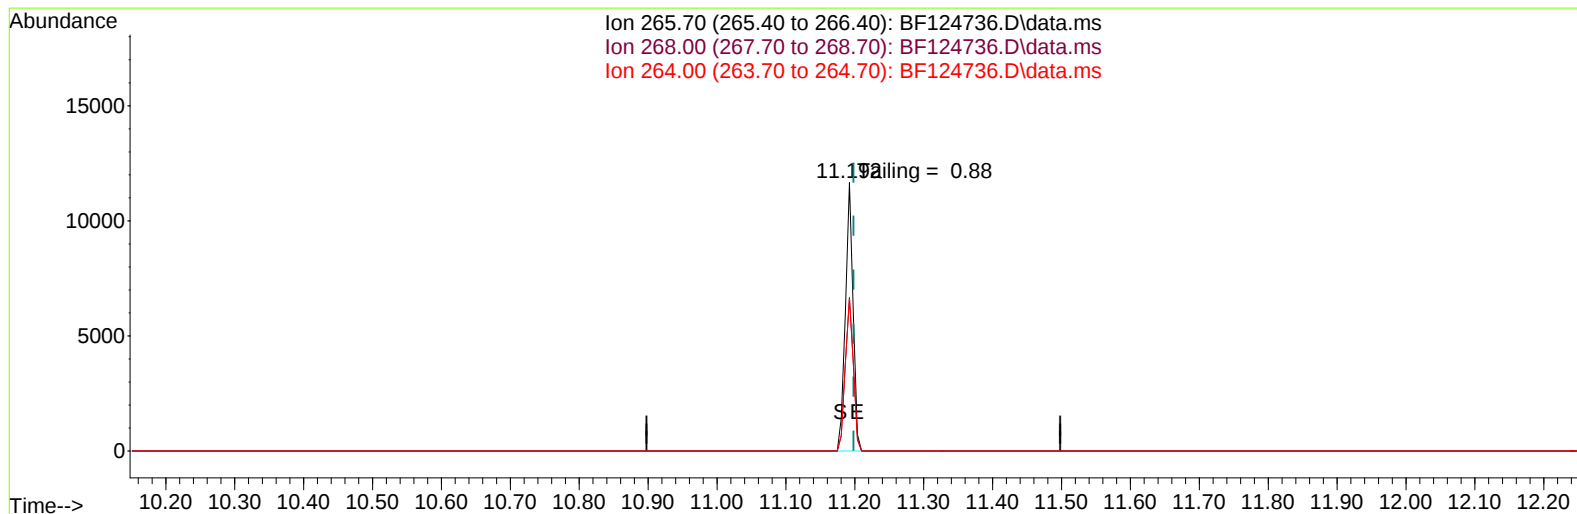

TIC: BF124736.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 0.00 ng




response 9007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	57.03
264.00	69.90	57.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072421\
 Data File : BF124736.D
 Acq On : 24 Jul 2021 8:50
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 26 07:06:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 15:28:57 2021
 Response via : Initial Calibration

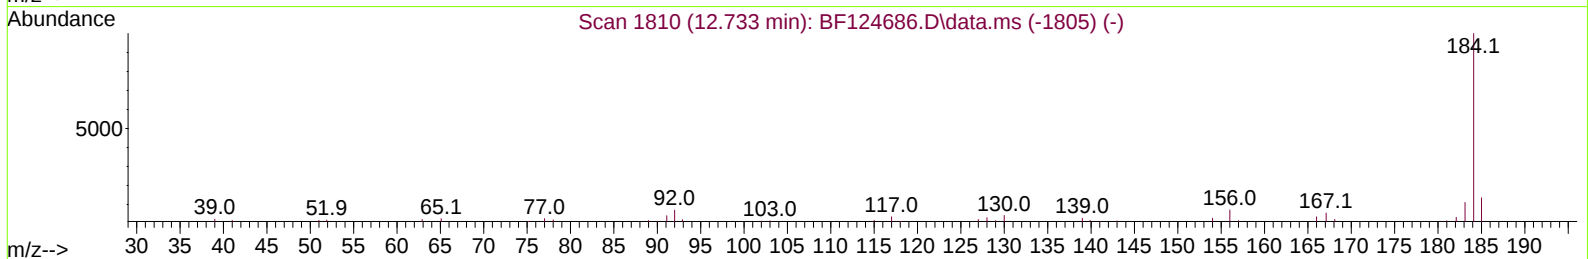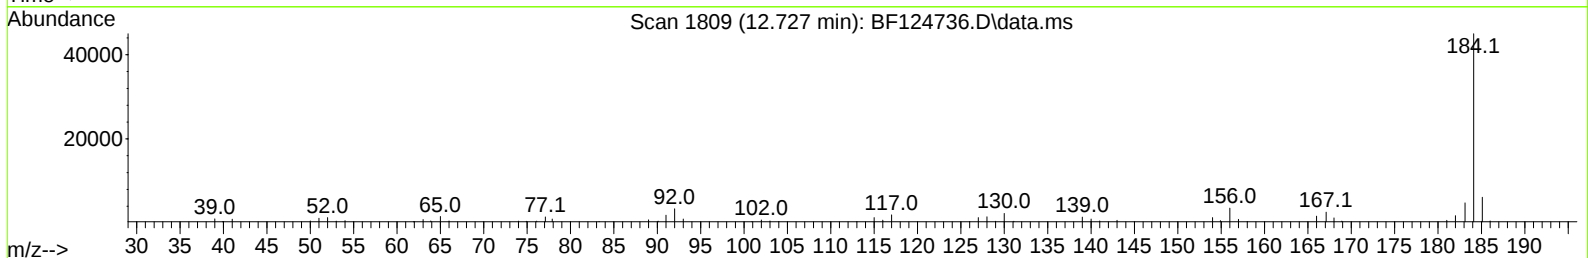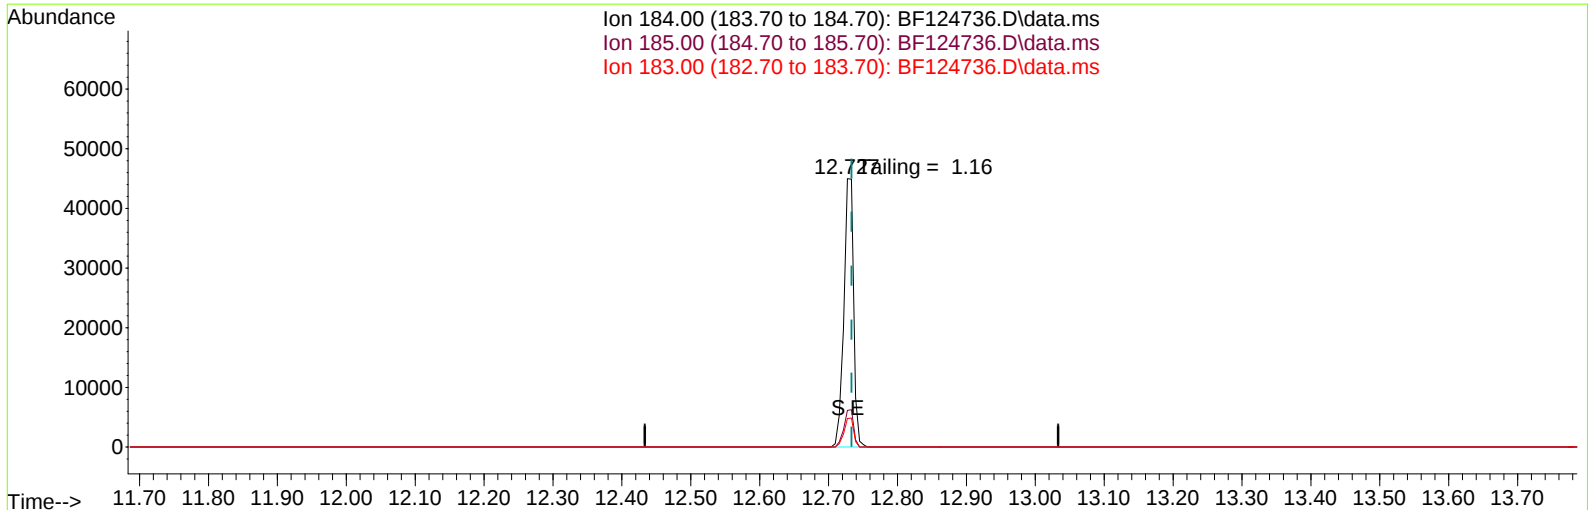

TIC: BF124736.D\data.ms

(77) Benzidine

12.727min (-0.006) 0.00 ng

response 44197

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.64
183.00	10.10	10.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/24/2021	BNA_F	<u>BF124736.D</u>
Compound Name	Response	Retention Time
DDT	24952	13.592
DDD	0	13.25
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	24952	0.00