
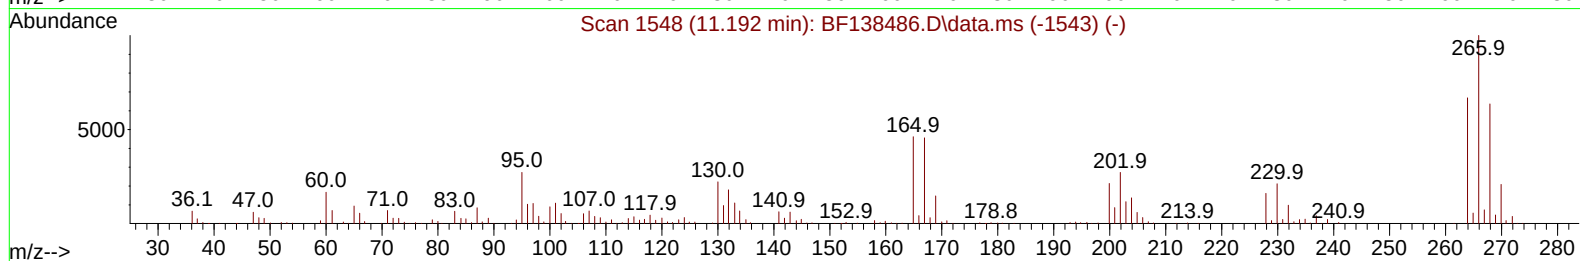
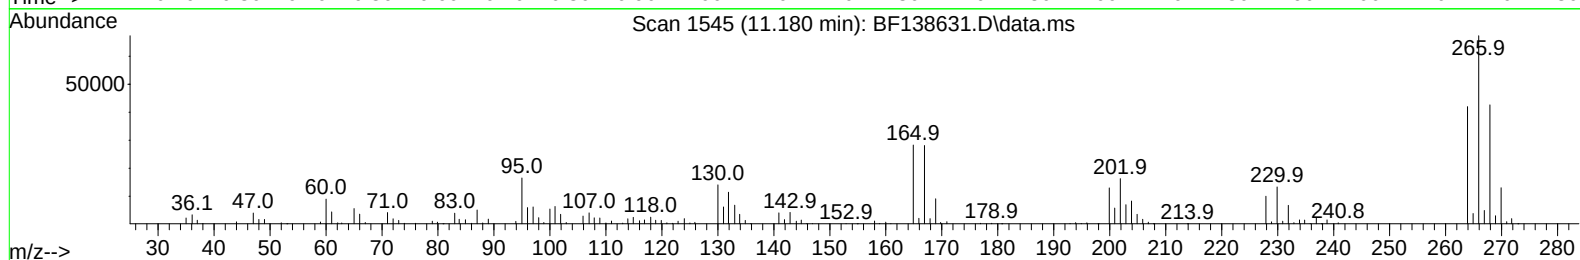


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072424\
Data File : BF138631.D
Acq On : 24 Jul 2024 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 12:46:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

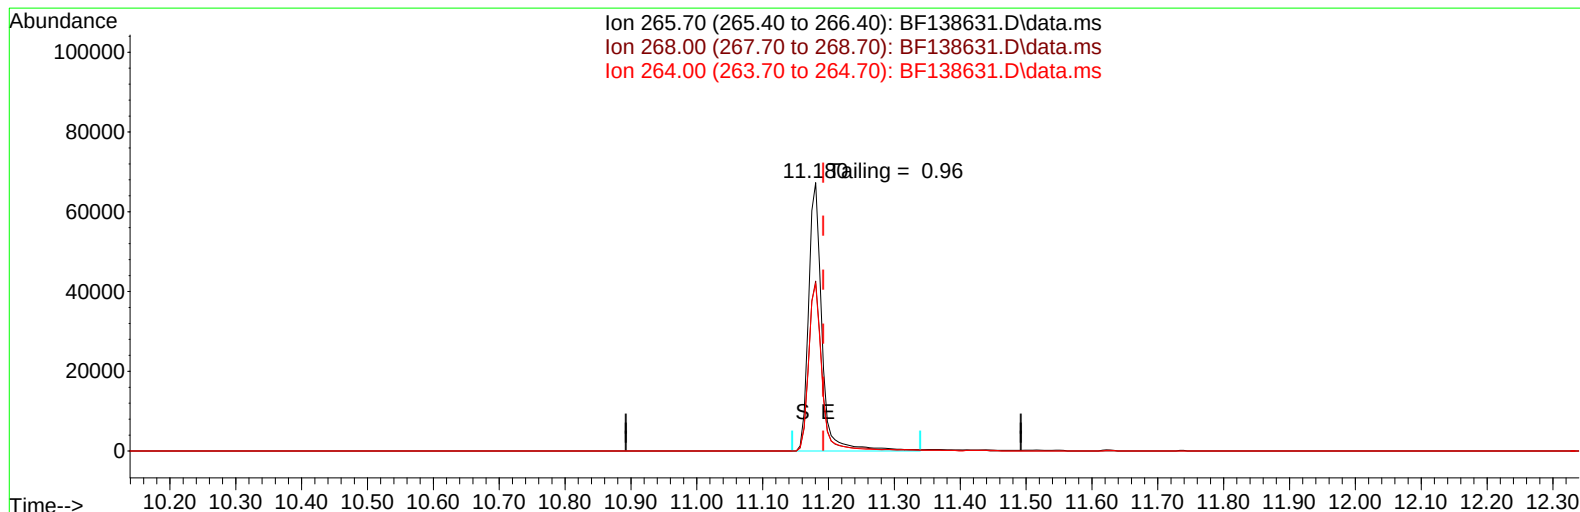

TIC: BF138631.D\data.ms

(70) Pentachlorophenol (C)




11.180min (-0.012) 247762.20 ng

response 95418

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.31
264.00	66.90	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072424\
Data File : BF138631.D
Acq On : 24 Jul 2024 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 12:46:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

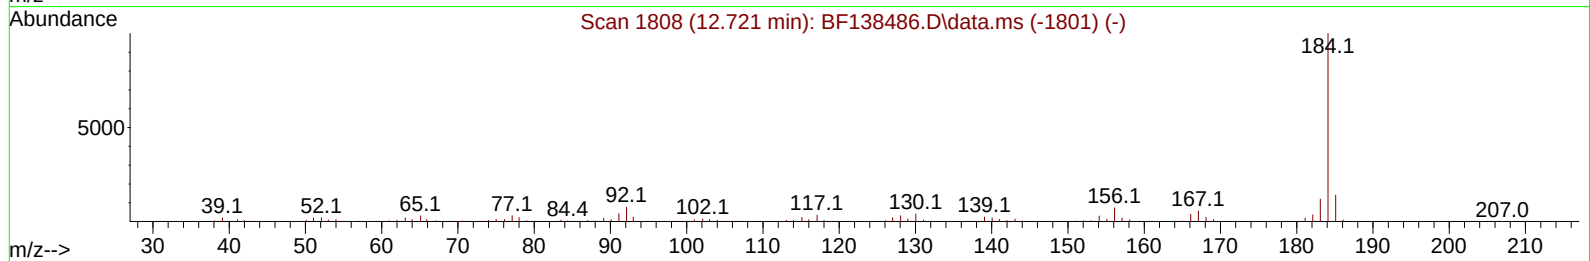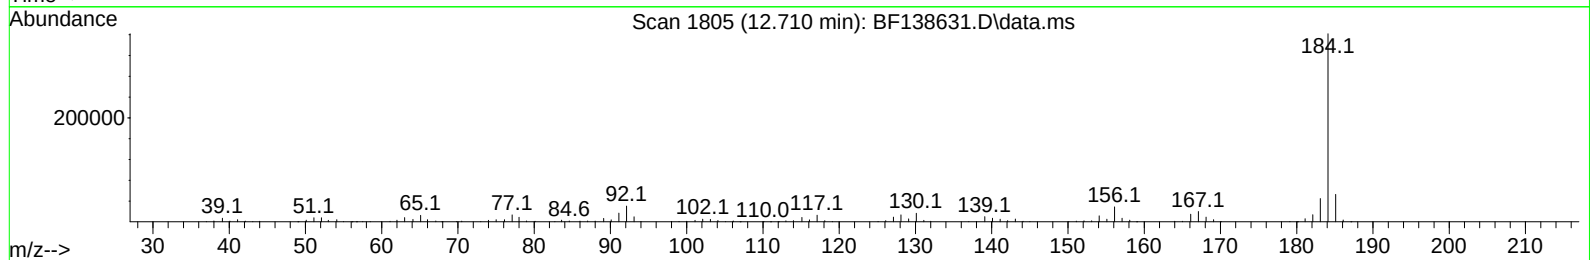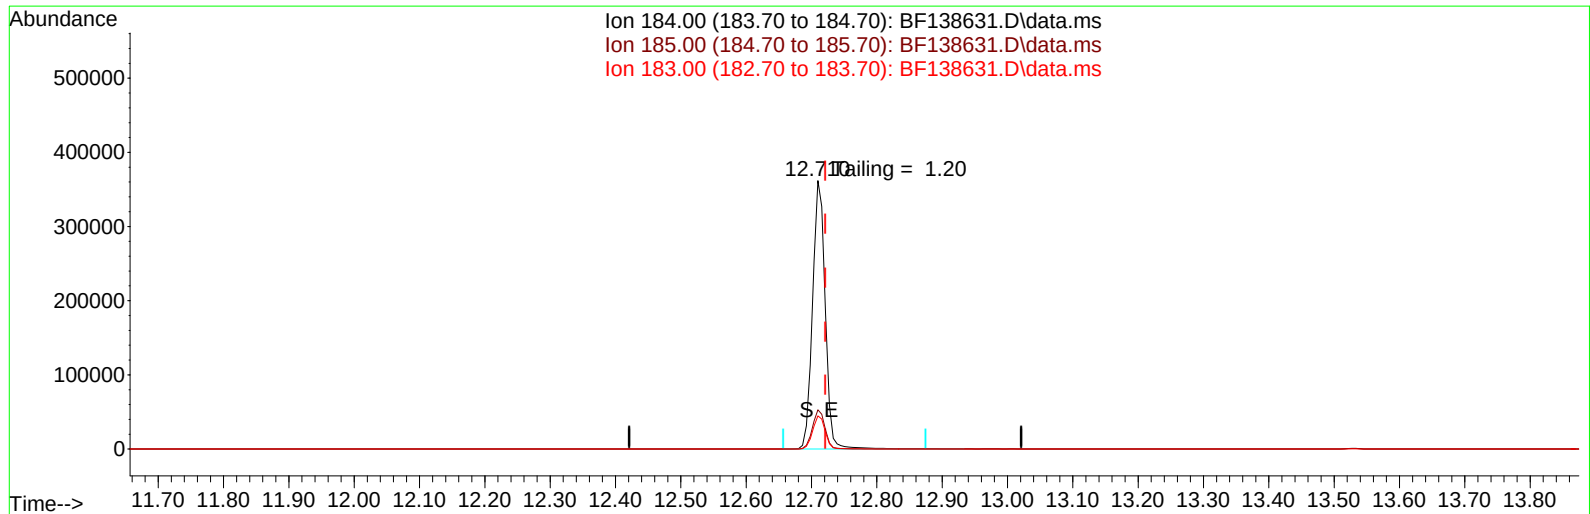

TIC: BF138631.D\data.ms

(77) Benzidine

12.710min (-0.011) 0.00 ng

response 488382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.60
183.00	11.90	12.36
0.00	0.00	0.00