


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072424\
Data File : BF138631.D
Acq On : 24 Jul 2024 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

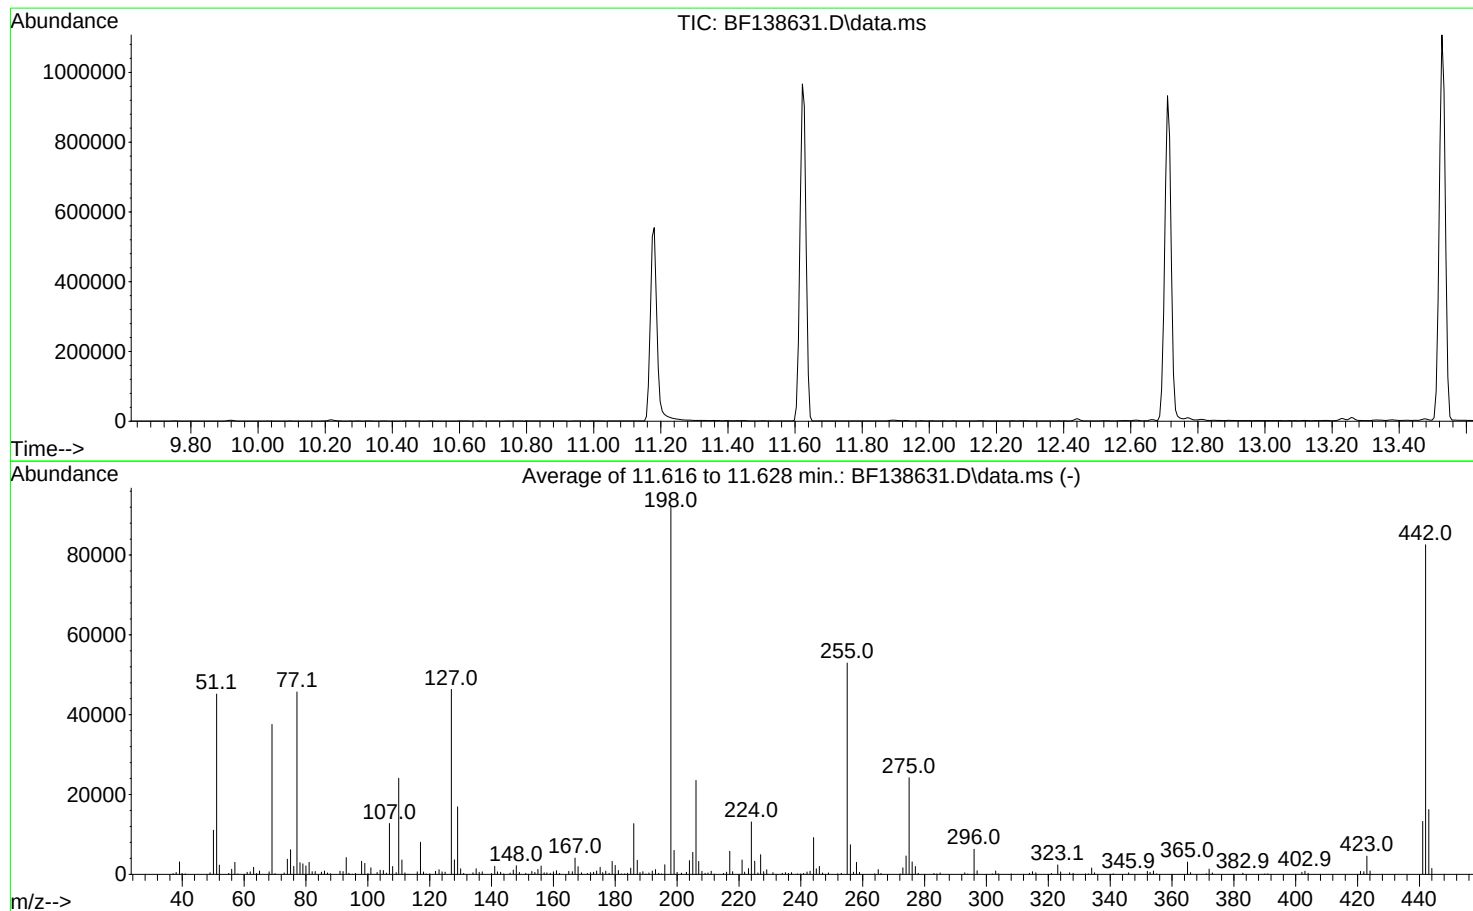




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	45168	PASS
68	69	0.00	2	1.7	644	PASS
69	198	0.00	100	40.8	37565	PASS
70	69	0.00	2	0.5	201	PASS
127	198	10	80	50.3	46325	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92165	PASS
199	198	5	9	6.5	6025	PASS
275	198	10	60	26.3	24213	PASS
365	198	1	100	3.4	3096	PASS
441	198	0.01	100	14.4	13271	PASS
442	442	50	100	100.0	82597	PASS
443	442	15	24	19.7	16238	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072424\
Data File : BF138631.D
Acq On : 24 Jul 2024 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 24 12:46:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

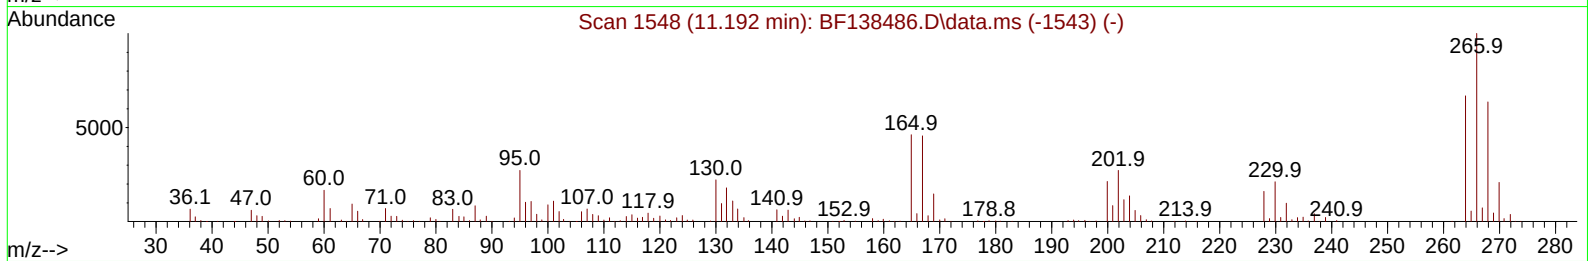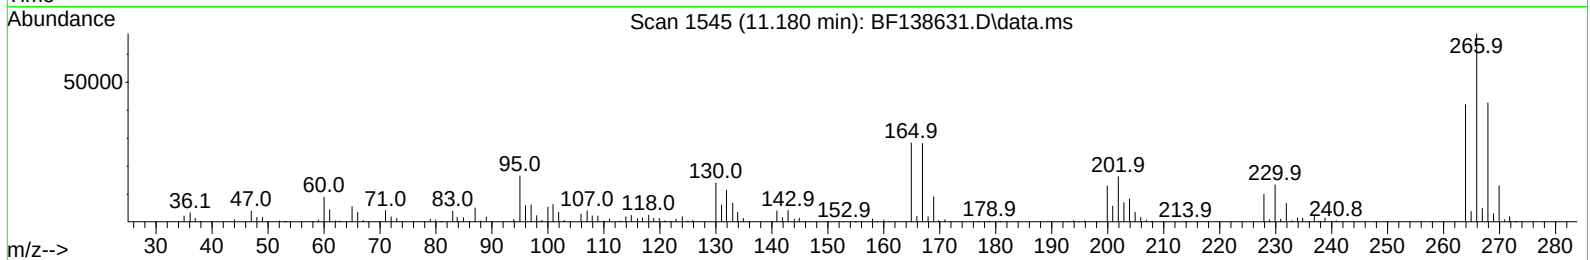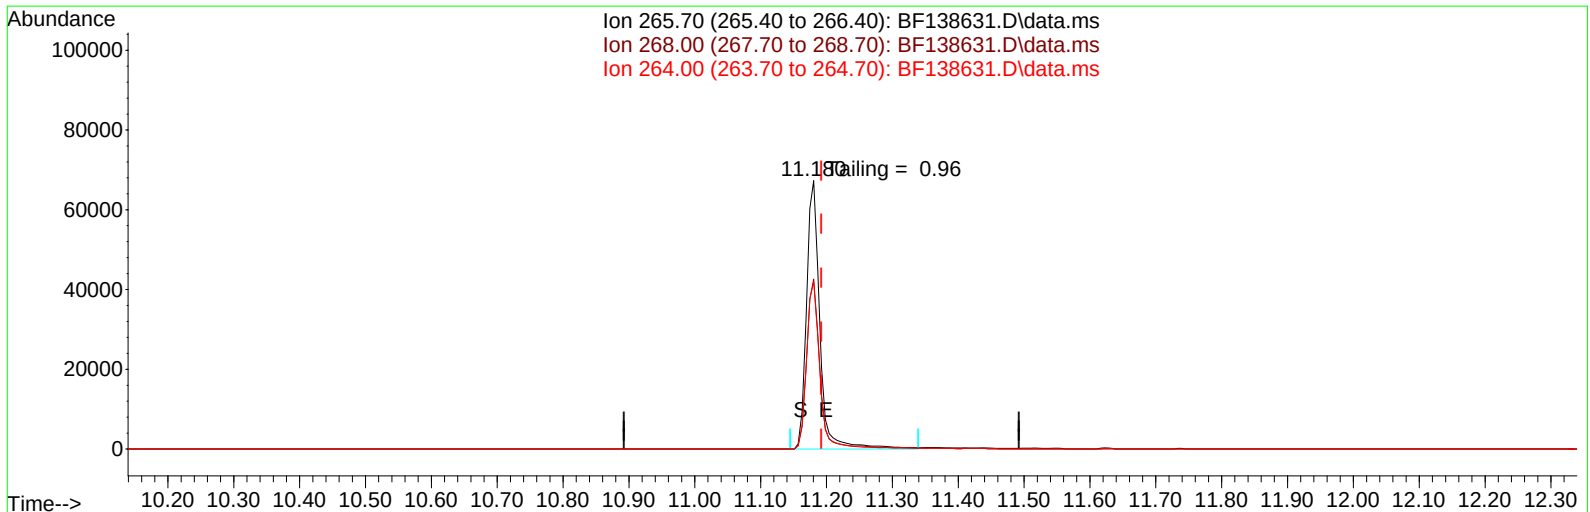

TIC: BF138631.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.012) 247762.20 ng




response 95418

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.31
264.00	66.90	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072424\
Data File : BF138631.D
Acq On : 24 Jul 2024 10:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 24 12:46:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

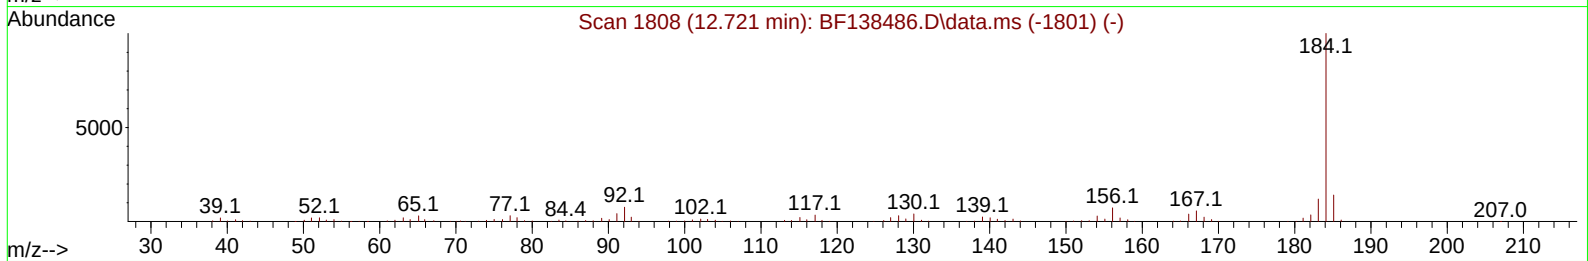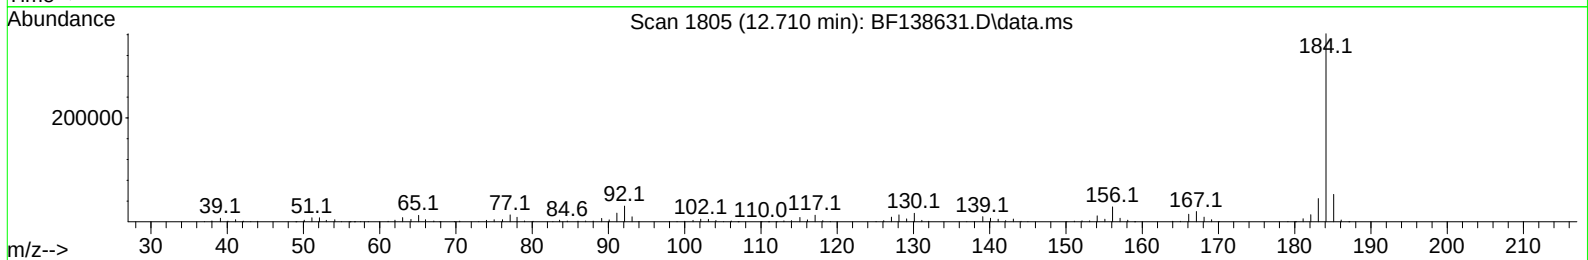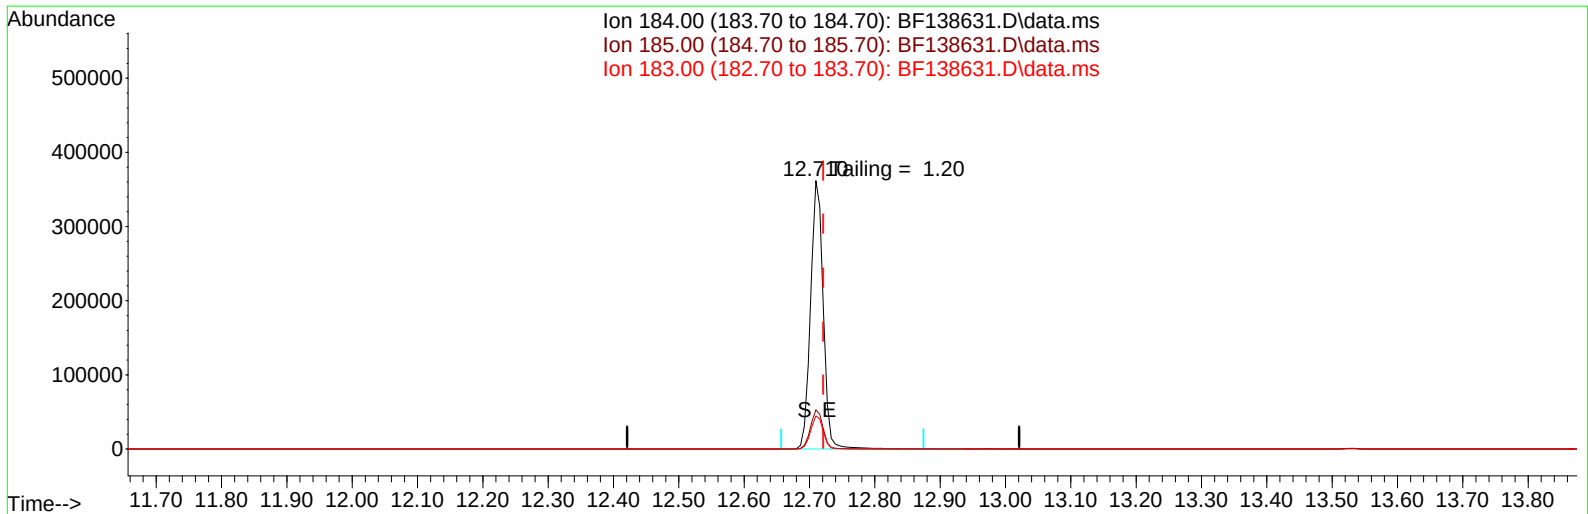

TIC: BF138631.D\data.ms

(77) Benzidine

12.710min (-0.011) 0.00 ng

response 488382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.60
183.00	11.90	12.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/24/2024	BNA_F	<u>BF138631.D</u>
Compound Name	Response	Retention Time
DDT	262266	13.527
DDD	4734	13.257
DDE	490	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5224	267490	1.95

Instrument :
BNA_F
ClientSampleId :
DFTPP