
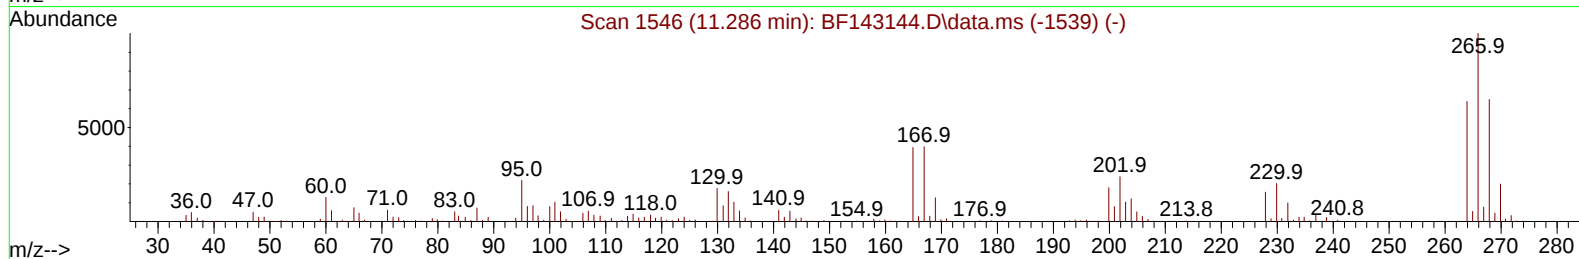
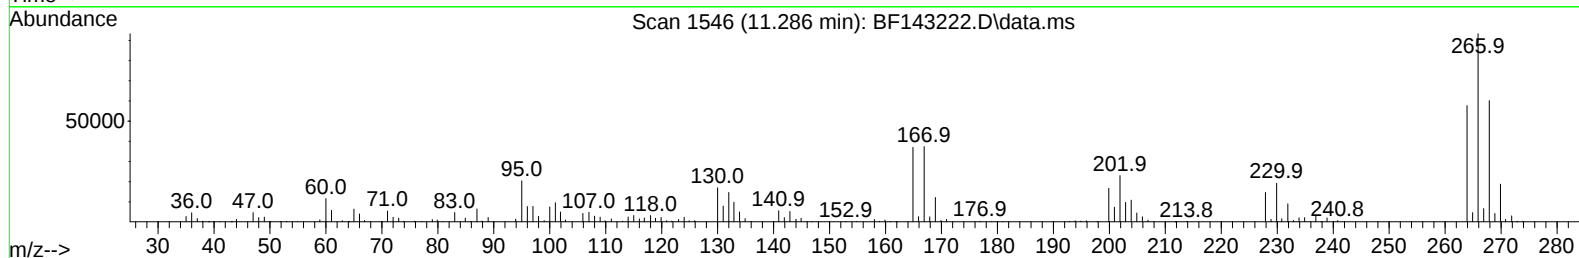


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072425\
Data File : BF143222.D
Acq On : 24 Jul 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 11:14:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

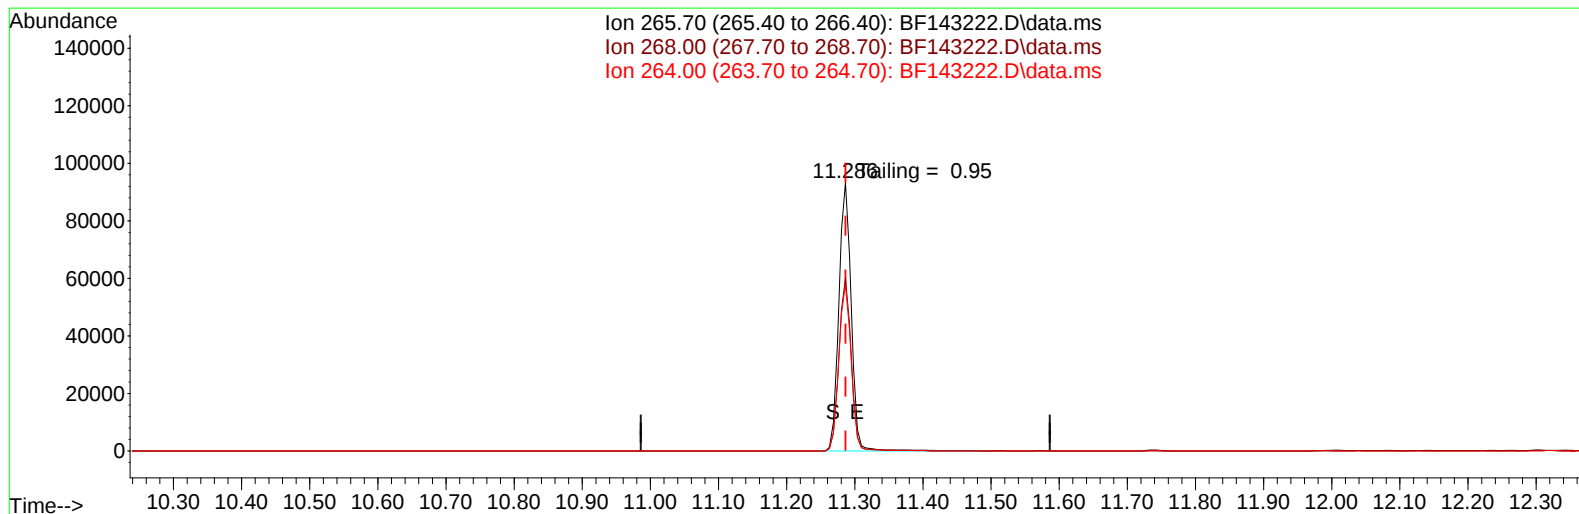

TIC: BF143222.D\data.ms

(70) Pentachlorophenol (C)




11.286min (-0.000) 17494.42 ng

response 116745

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.48
264.00	63.80	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072425\
Data File : BF143222.D
Acq On : 24 Jul 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 11:14:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

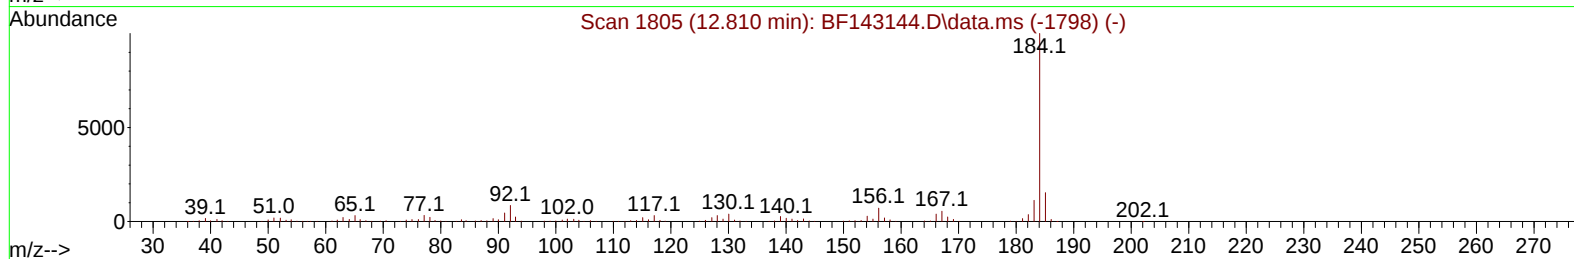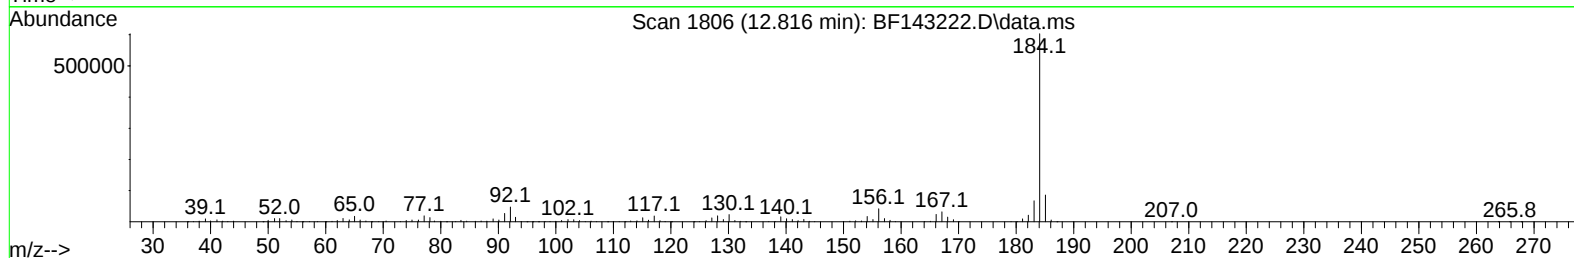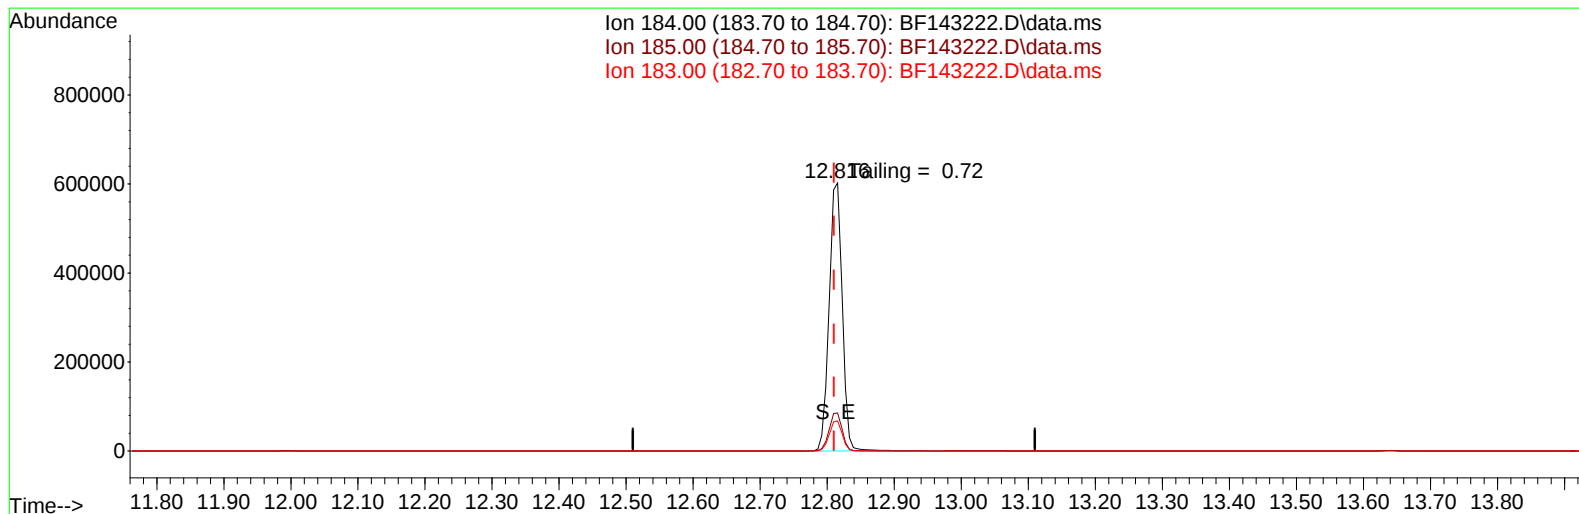

TIC: BF143222.D\data.ms

(77) Benzidine

12.816min (+ 0.005) 7214.05 ng

response 820751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.23
183.00	11.20	11.21
0.00	0.00	0.00