
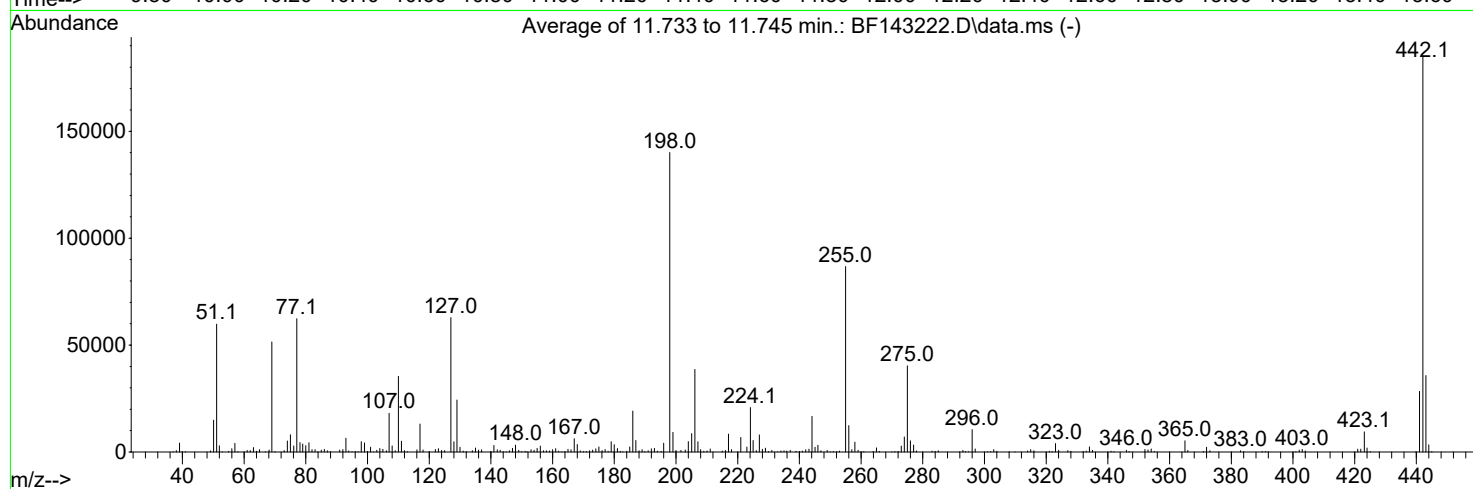


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072425\
Data File : BF143222.D
Acq On : 24 Jul 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

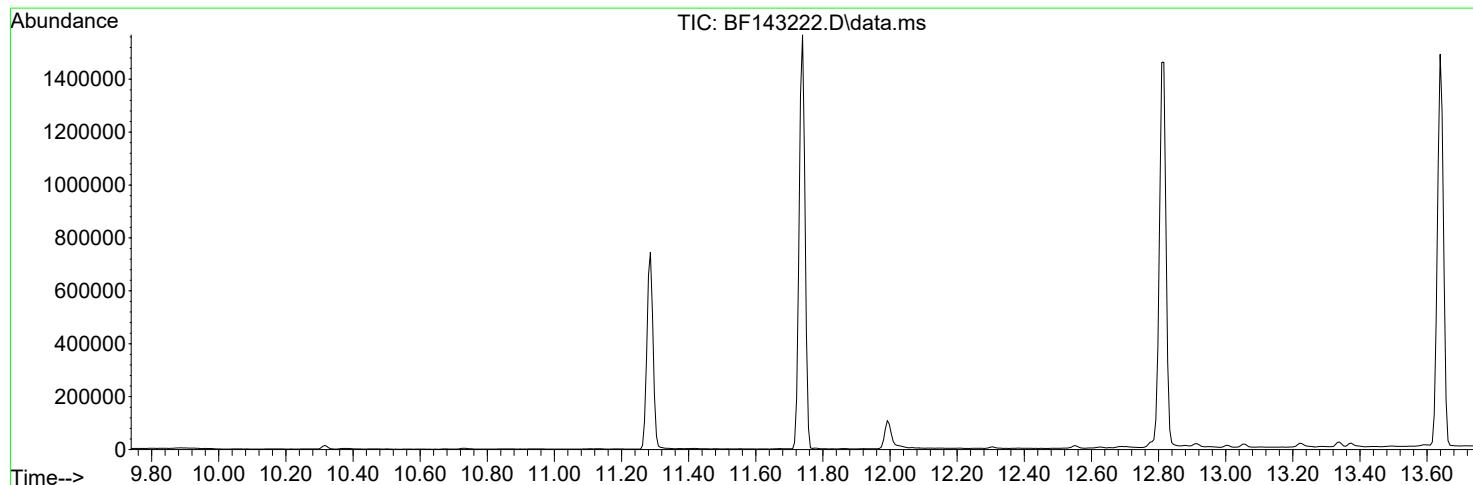

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1003	PASS
69	69	100	100	100.0	51483	PASS
70	69	0.00	2	0.4	219	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140141	PASS
199	198	5	9	6.6	9197	PASS
365	198	1	100	3.7	5252	PASS
441	443	0.01	150	79.4	28376	PASS
442	442	100	100	100.0	184683	PASS
443	442	15	24	19.4	35760	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/24/2025	BNA_F	<u>BF143222.D</u>
Compound Name	Response	Retention Time
DDT	368644	13.639
DDD	8567	13.339
DDE	1840	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10407	379051	2.75

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072425\
Data File : BF143222.D
Acq On : 24 Jul 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 24 11:14:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

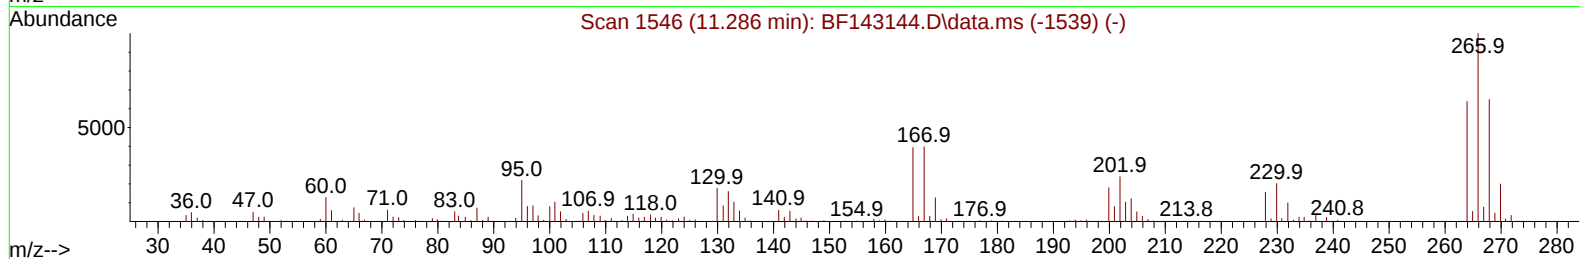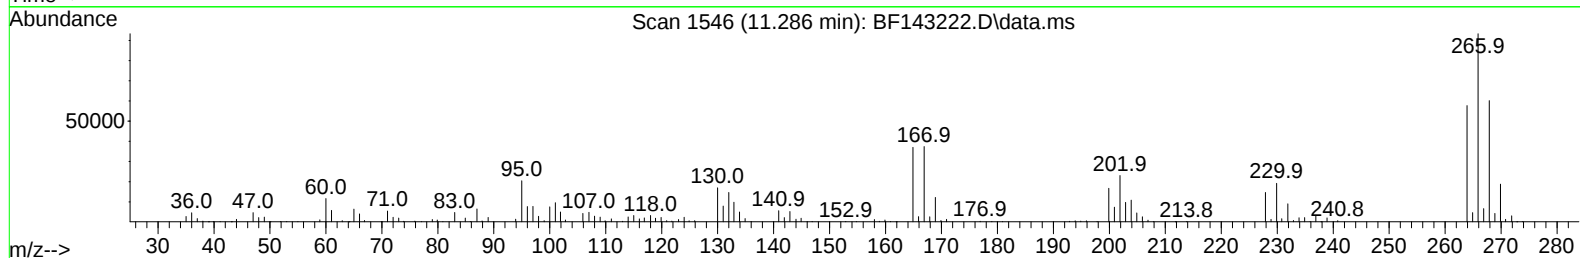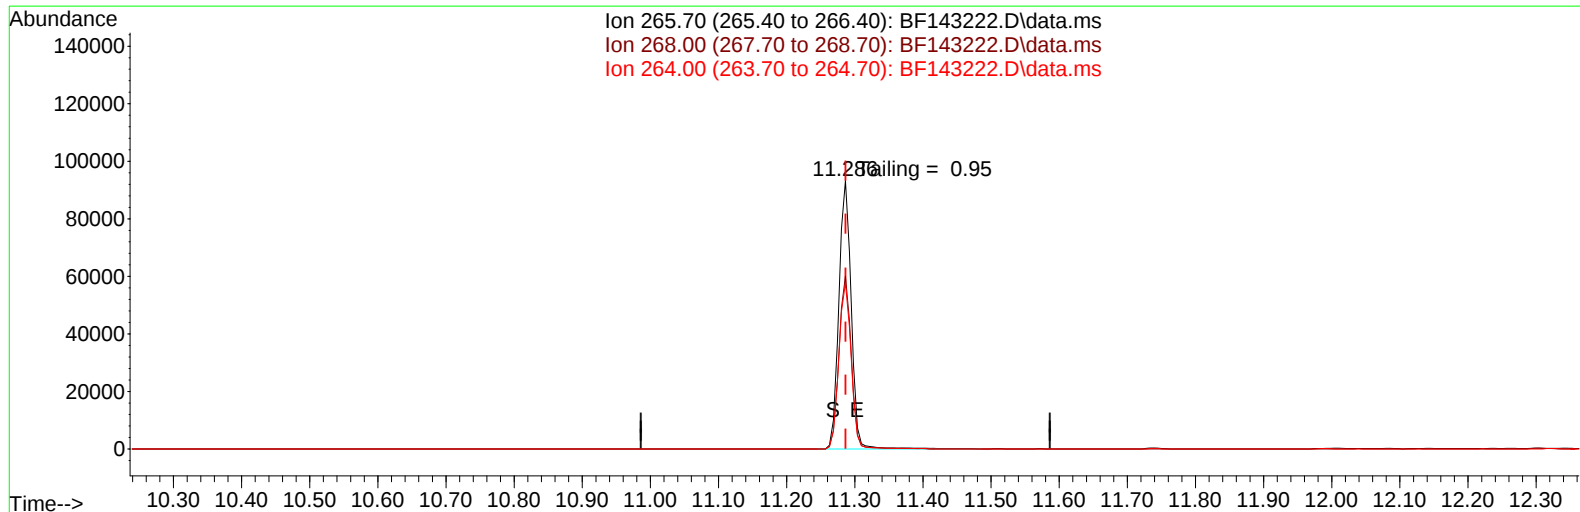

TIC: BF143222.D\data.ms

(70) Pentachlorophenol (C)

11.286min (-0.000) 17494.42 ng




response 116745

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.48
264.00	63.80	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072425\
Data File : BF143222.D
Acq On : 24 Jul 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 24 11:14:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

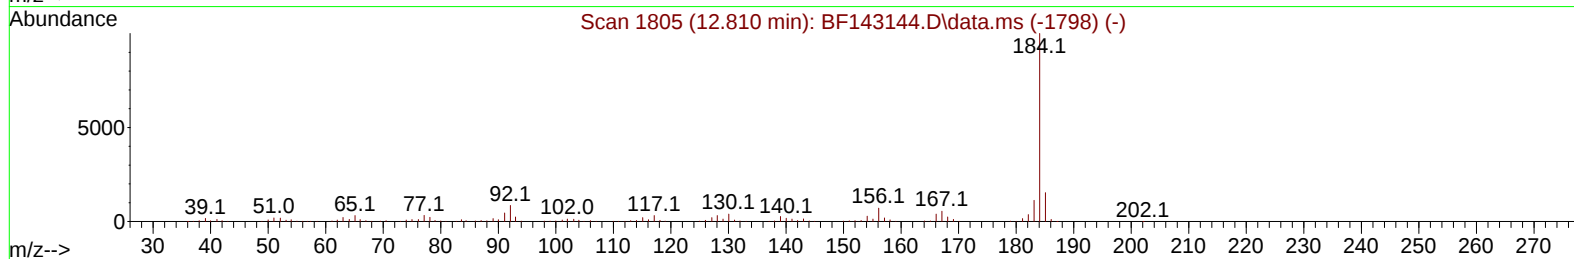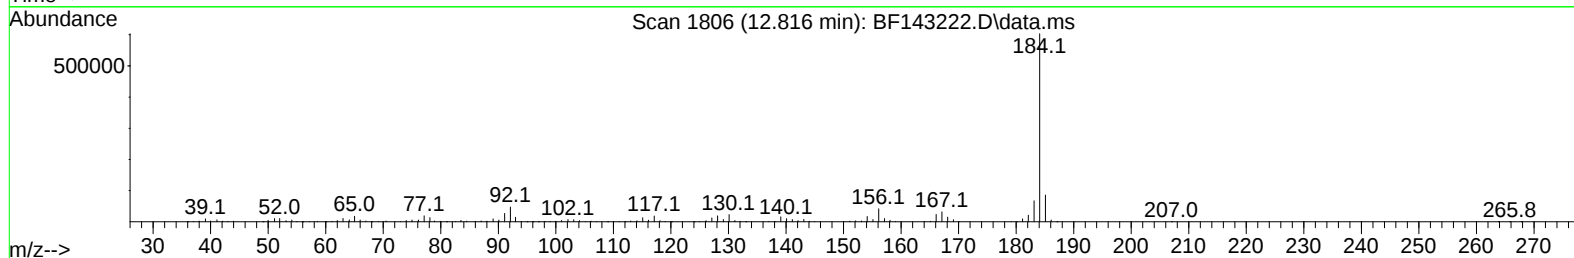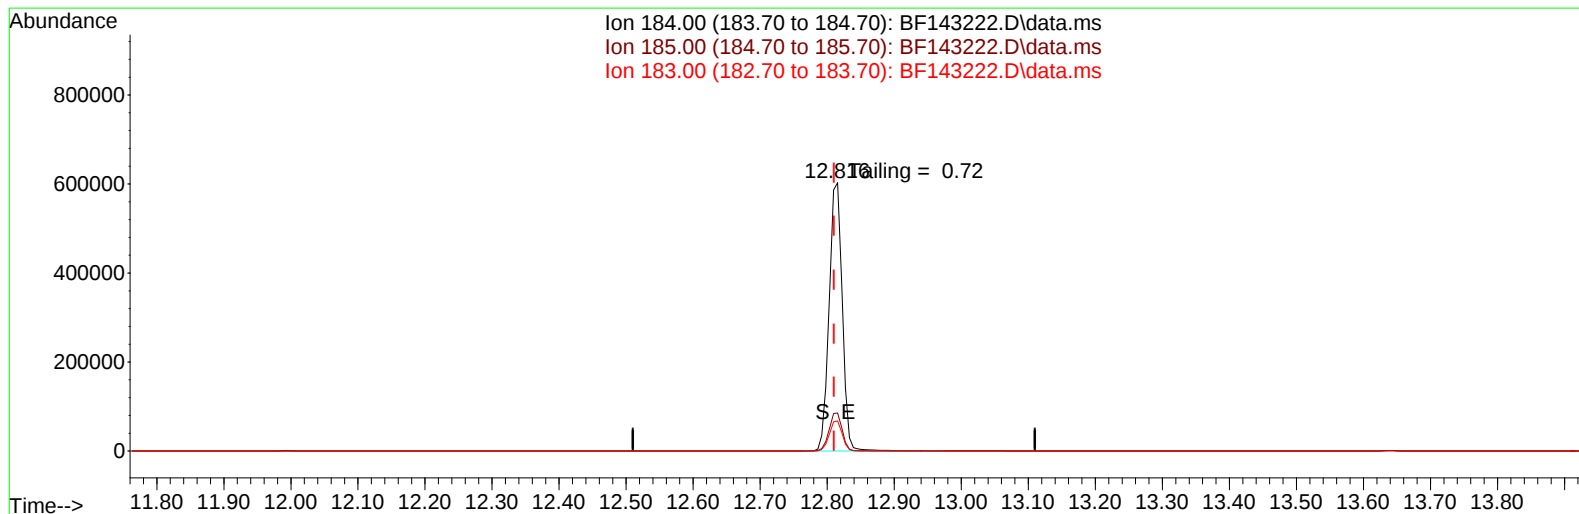

TIC: BF143222.D\data.ms

(77) Benzidine

12.816min (+ 0.005) 7214.05 ng

response 820751

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.23
183.00	11.20	11.21
0.00	0.00	0.00