

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072516\
 Data File : BF089279.D
 Acq On : 25 Jul 2016 15:12
 Operator : UM/SJ
 Sample : H4129-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0

Quant Time: Jul 25 17:18:10 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 16:56:43 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.56	152	54335	20.00	ng	-0.01
21) Naphthalene-d8	7.85	136	215018	20.00	ng	0.00
38) Acenaphthene-d10	9.59	164	87824	20.00	ng	-0.01
63) Phenanthrene-d10	11.06	188	147981	20.00	ng	-0.01
75) Chrysene-d12	13.68	240	108261	20.00	ng	-0.01
86) Perylene-d12	15.02	264	85257	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	478606	133.97	ng	0.01
7) Phenol-d6	6.23	99	579894	125.87	ng	0.00
23) Nitrobenzene-d5	7.13	82	358368	88.56	ng	-0.01
41) 2,4,6-Tribromophenol	10.38	330	86686	109.63	ng	-0.01
44) 2-Fluorobiphenyl	8.92	172	513998	80.64	ng	-0.01
78) Terphenyl-d14	12.65	244	333286	66.77	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.13	70	46752	15.51	ng	# 82
49) Dimethylphthalate	9.32	163	214108	31.77	ng	98
56) 2,4-Dinitrotoluene	9.59	165	11241	5.74	ng	# 10
66) 4-Bromophenyl-phenylether	10.38	248	6832	4.67	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072516\
Data File : BF089279.D
Acq On : 25 Jul 2016 15:12
Operator : UM/SJ
Sample : H4129-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KSB-14-5.0-7.0

Quant Time: Jul 25 17:18:10 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 16:56:43 2016
Response via : Initial Calibration

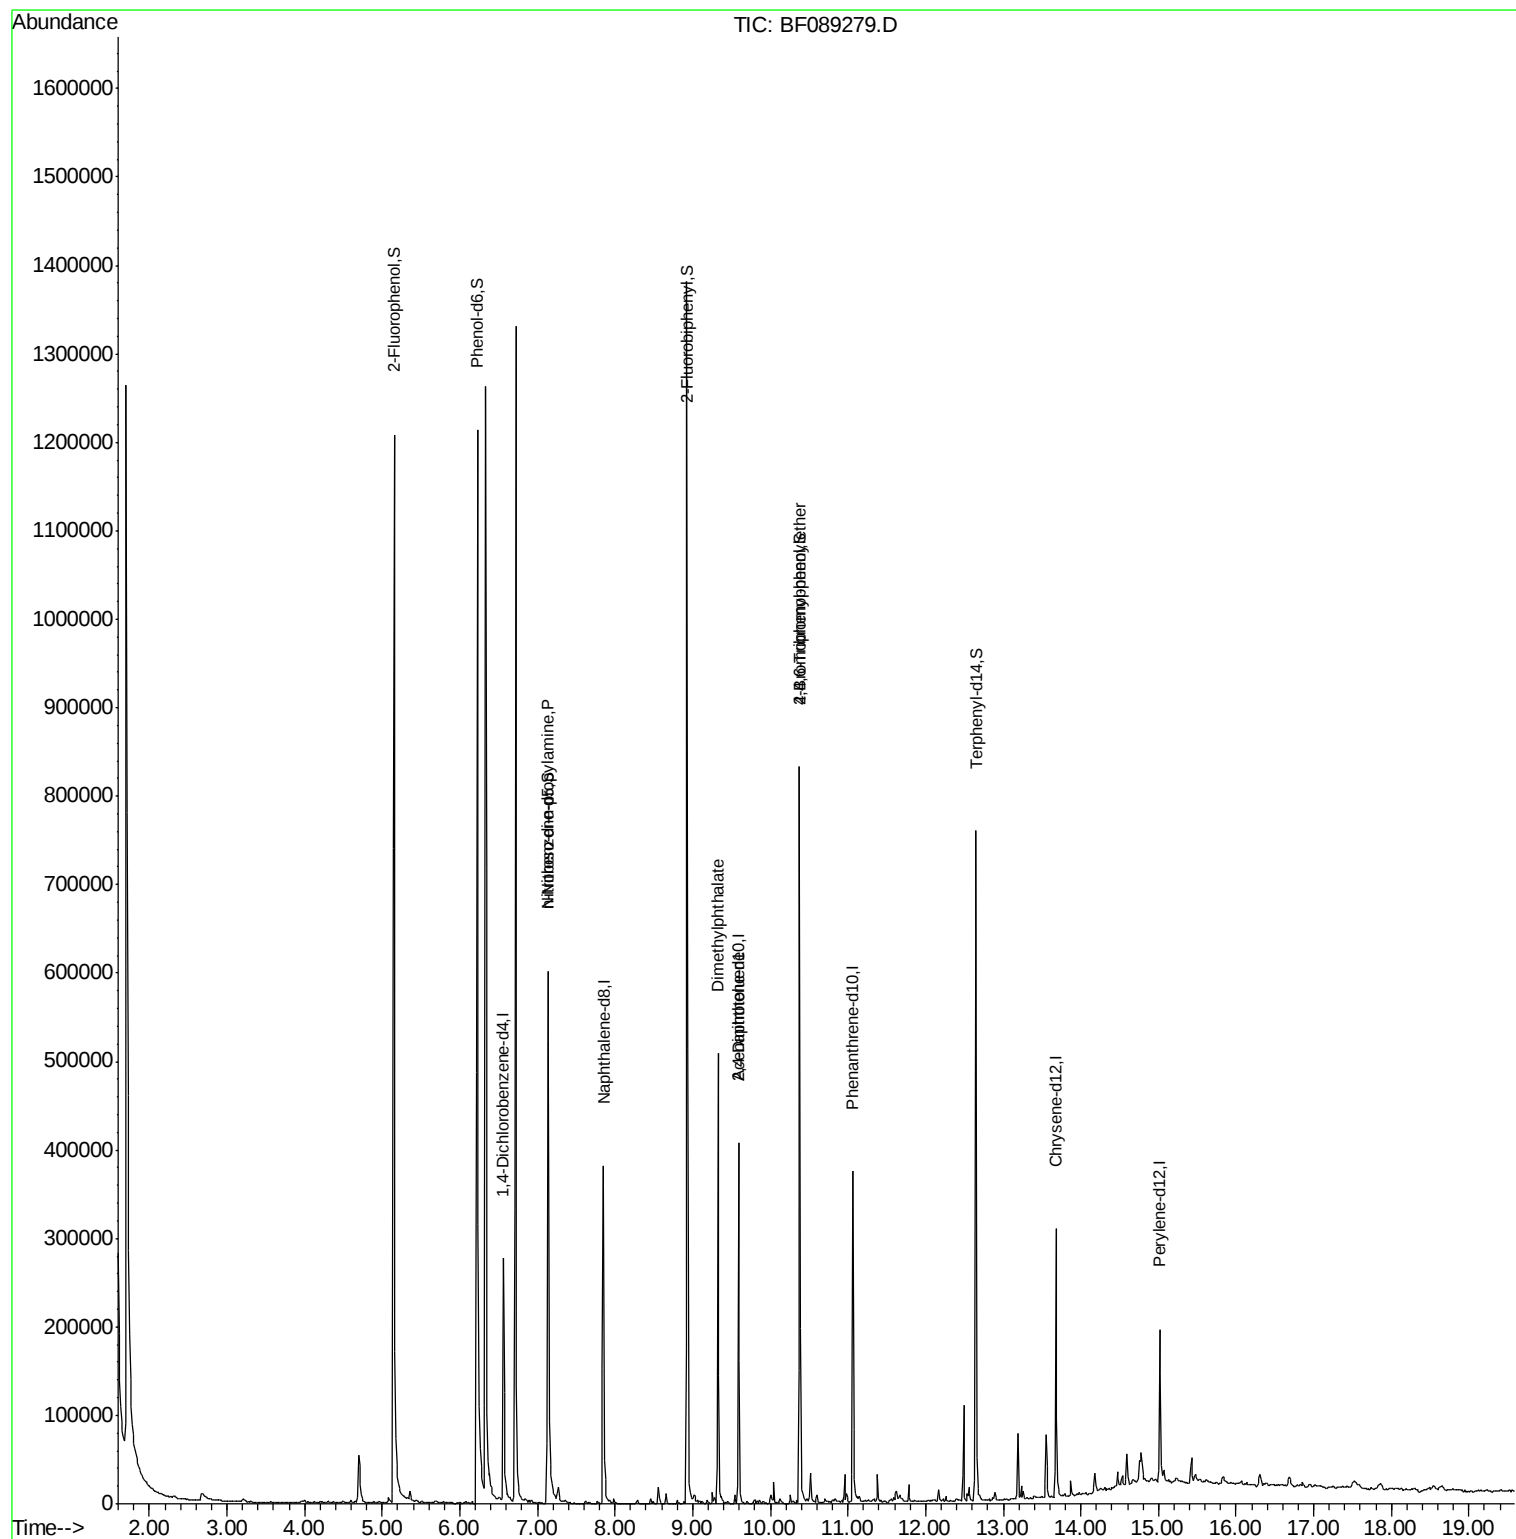

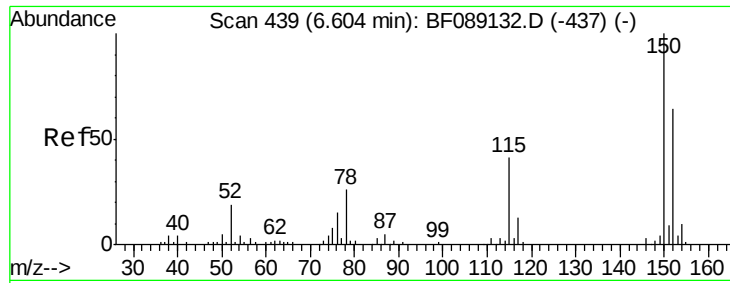


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.56 min Scan# 435
Delta R.T. -0.01 min
Lab File: BF089279.D
Acq: 25 Jul 2016 15:12

Instrument :
BNA_F
ClientSampleId :
KSB-14-5.0-7.0

Tgt Ion:152 Resp: 54335
Ion Ratio Lower Upper
152 100
150 160.3 125.1 187.7
115 72.2 51.1 76.7

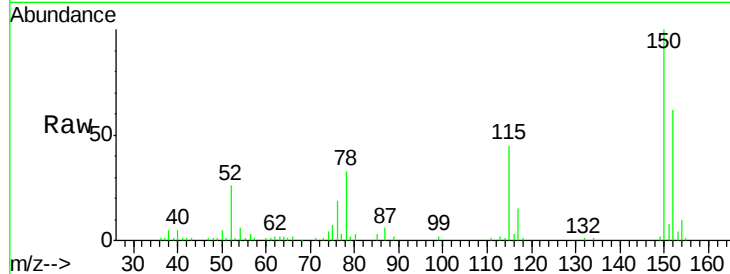


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

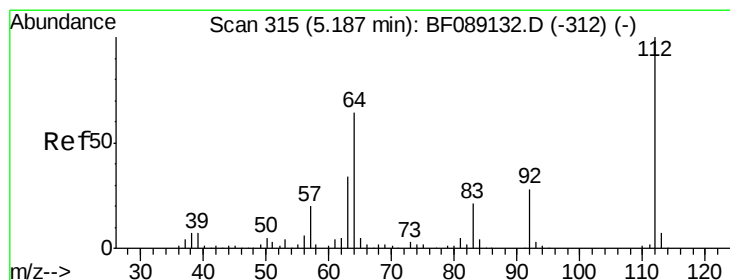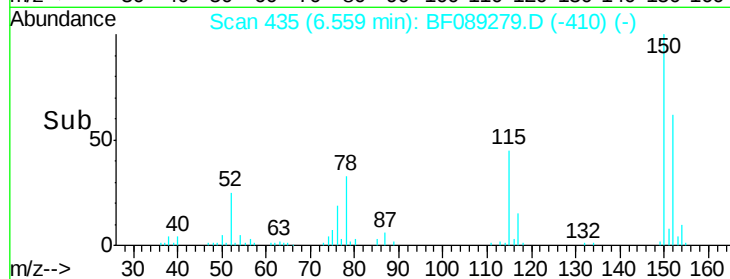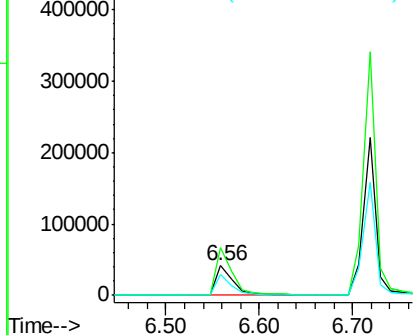



#5


2-Fluorophenol
Concen: 133.97 ng
RT: 5.15 min Scan# 312
Delta R.T. 0.01 min
Lab File: BF089279.D
Acq: 25 Jul 2016 15:12

Tgt Ion:112 Resp: 478606
Ion Ratio Lower Upper
112 100
64 54.0 51.0 76.4
63 29.3 27.3 40.9

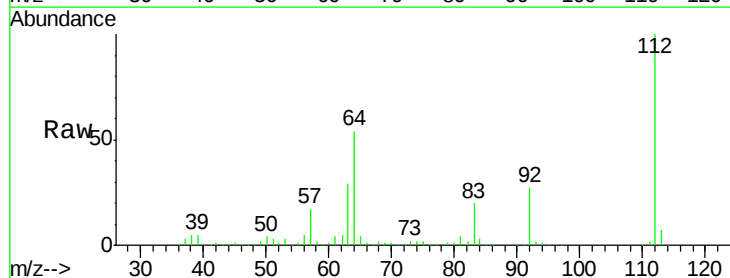

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

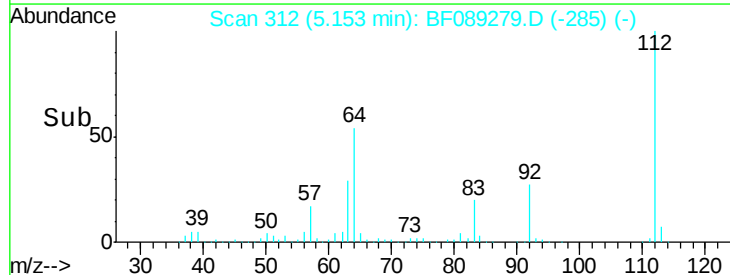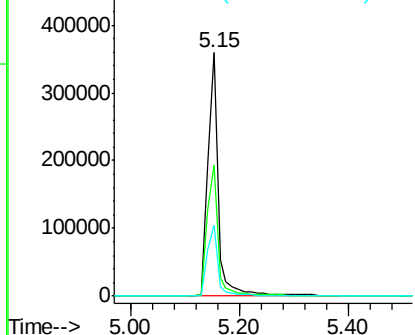

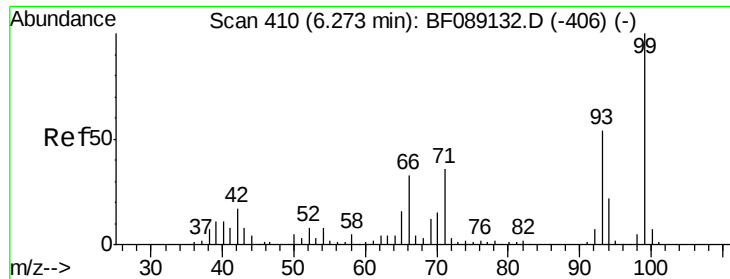

#7

Phenol-d6

Concen: 125.87 ng

RT: 6.23 min Scan# 406

Delta R.T. 0.00 min

Lab File: BF089279.D

Acq: 25 Jul 2016 15:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-5.0-7.0


Tgt Ion: 99 Resp: 579894

Ion Ratio Lower Upper

99 100

42 18.5 13.5 20.3




71 38.3 28.9 43.3

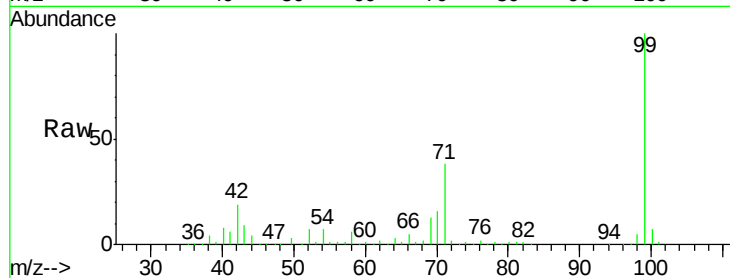

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

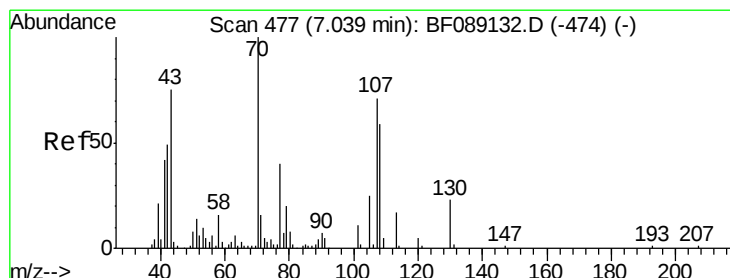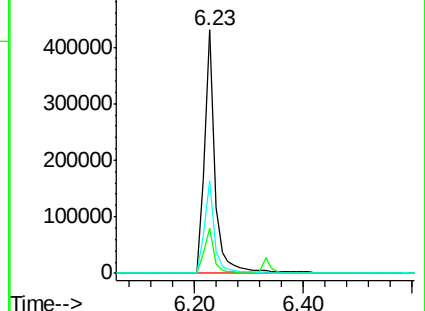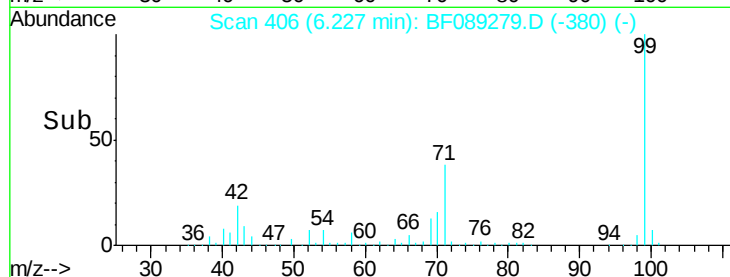

#19

n-Nitroso-di-n-propylamine

Concen: 15.51 ng

RT: 7.13 min Scan# 485

Delta R.T. 0.13 min

Lab File: BF089279.D

Acq: 25 Jul 2016 15:12

Tgt Ion: 70 Resp: 46752


Ion Ratio Lower Upper

70 100

42 46.7 39.2 58.8

101 0.0 8.5 12.7#

130 1.9 18.4 27.6#


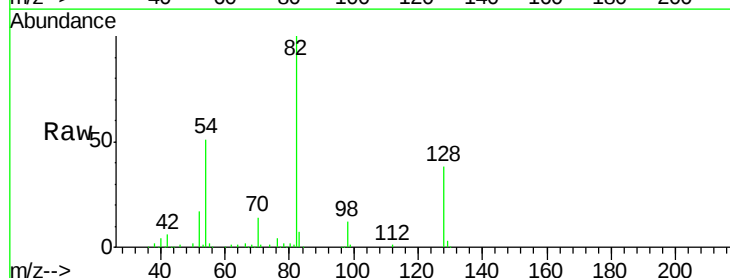



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

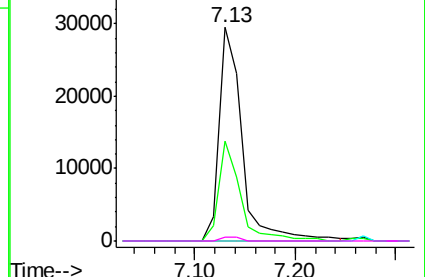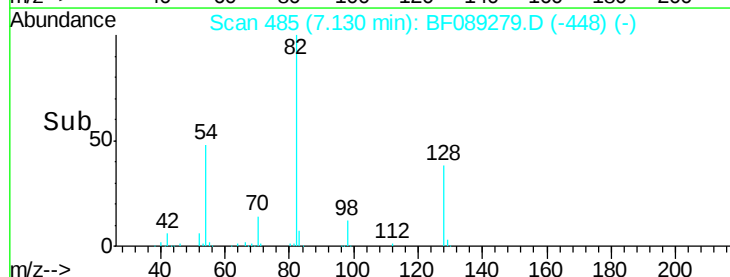

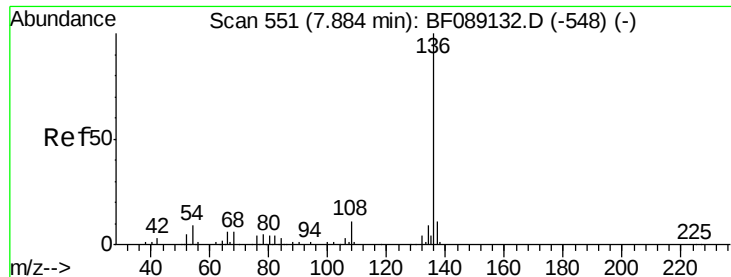

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.85 min Scan# 548

Delta R.T. 0.00 min

Lab File: BF089279.D

Acq: 25 Jul 2016 15:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-5.0-7.0

Tgt Ion:136 Resp: 215018


Ion Ratio Lower Upper

136 100

137 10.6 8.8 13.2

54 6.0 7.0 10.4#

68 4.9 5.0 7.6#



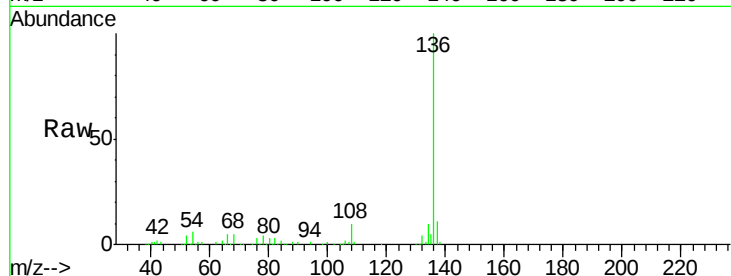


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

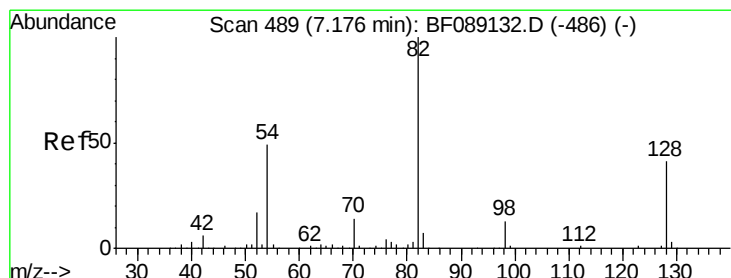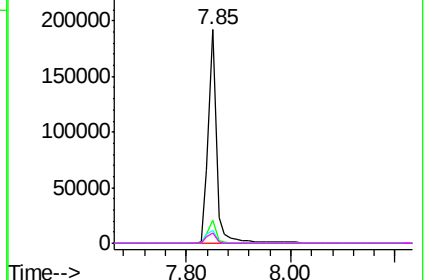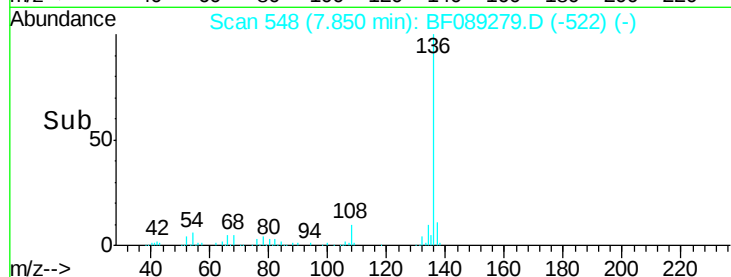

#23

Nitrobenzene-d5

Concen: 88.56 ng

RT: 7.13 min Scan# 485

Delta R.T. -0.01 min

Lab File: BF089279.D

Acq: 25 Jul 2016 15:12


Tgt Ion: 82 Resp: 358368

Ion Ratio Lower Upper

82 100

128 37.6 33.0 49.6



54 50.8 39.0 58.4

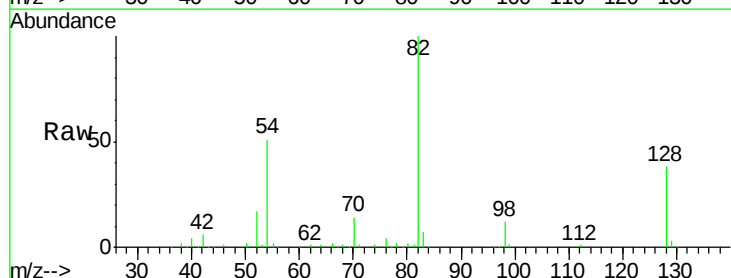


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

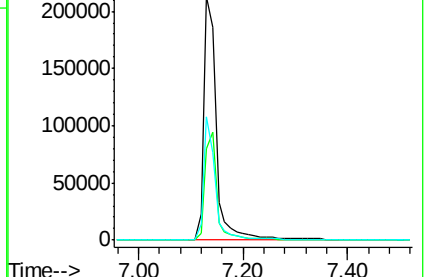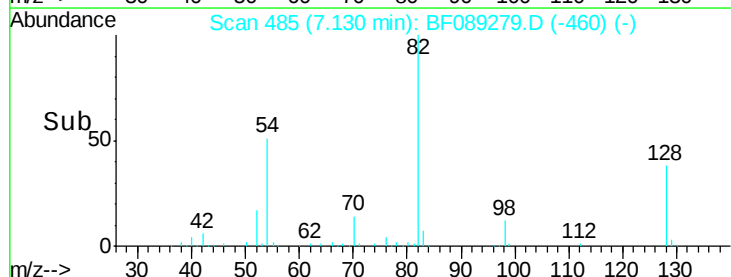


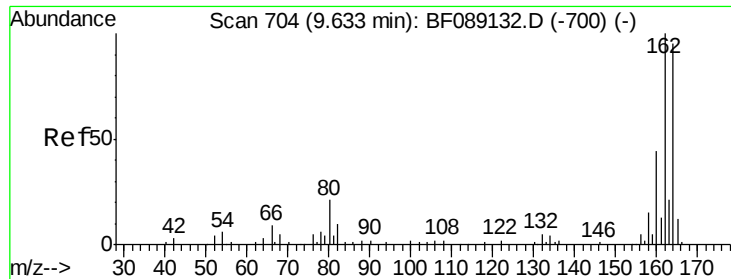




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.59 min Scan# 700
 Delta R.T. -0.01 min
 Lab File: BF089279.D
 Acq: 25 Jul 2016 15:12

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0

Tgt Ion:164 Resp: 87824
 Ion Ratio Lower Upper
 164 100
 162 106.1 84.1 126.1
 160 46.1 37.1 55.7

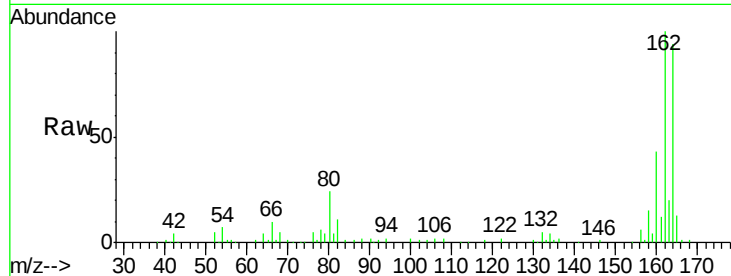


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

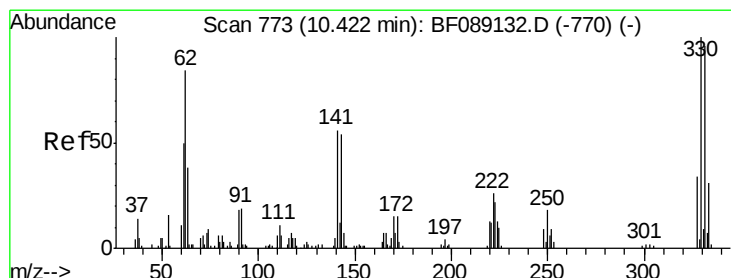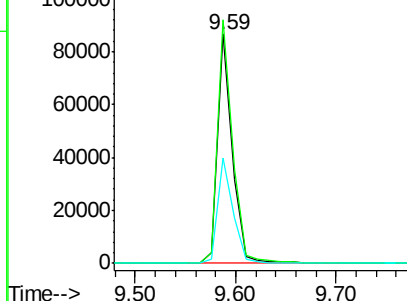
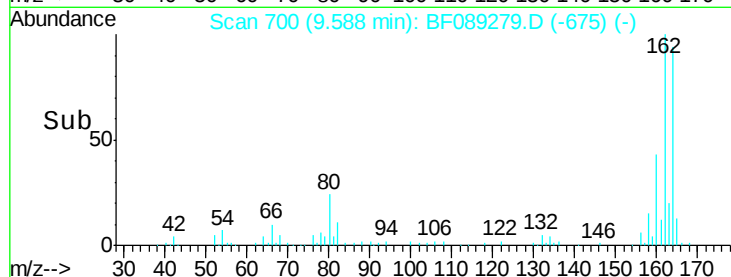



#41
 2,4,6-Tribromophenol
 Concen: 109.63 ng
 RT: 10.38 min Scan# 769
 Delta R.T. -0.01 min
 Lab File: BF089279.D
 Acq: 25 Jul 2016 15:12

Tgt Ion:330 Resp: 86686
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.2 115.8
 141 50.8 42.2 63.2

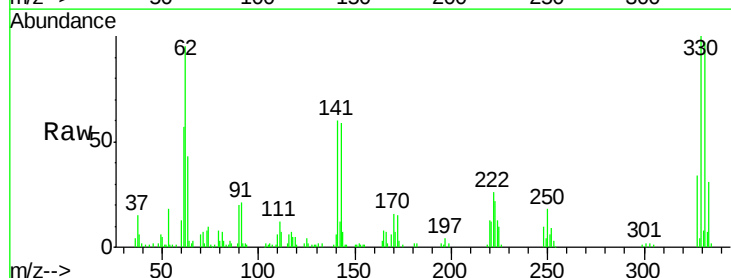

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

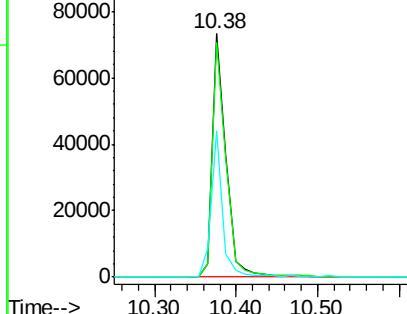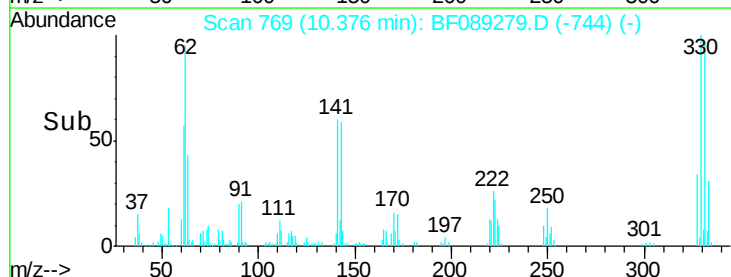


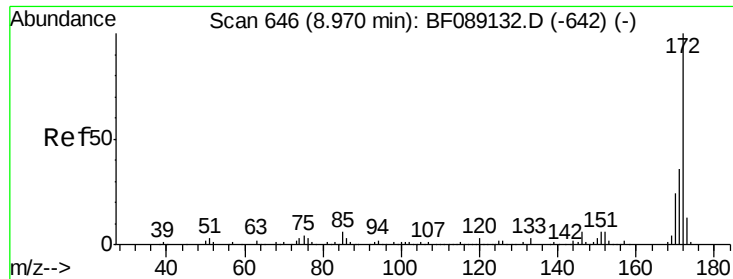




#44
 2-Fluorobiphenyl
 Concen: 80.64 ng
 RT: 8.92 min Scan# 642
 Delta R.T. -0.01 min
 Lab File: BF089279.D
 Acq: 25 Jul 2016 15:12

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0

Tgt Ion:172 Resp: 513998
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.2 43.8
 170 23.9 19.1 28.7

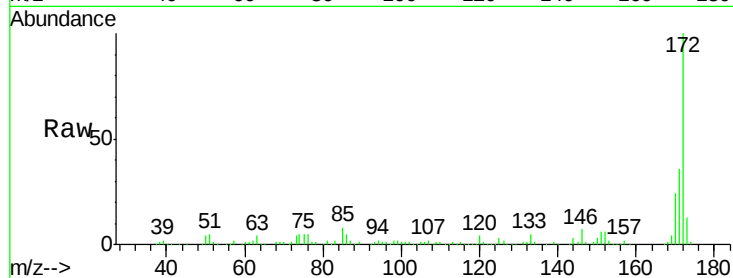


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

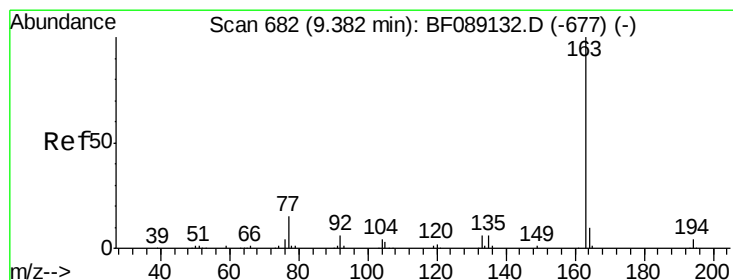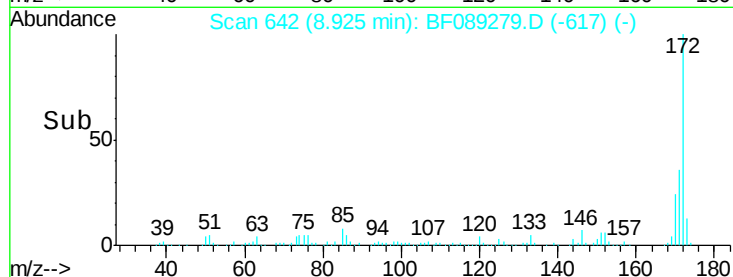
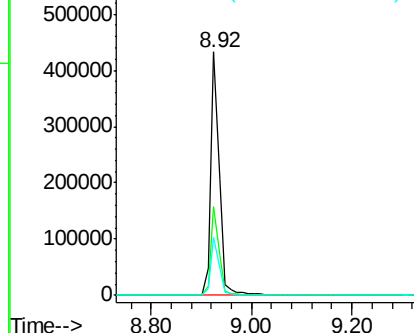



#49
 Dimethylphthalate
 Concen: 31.77 ng
 RT: 9.32 min Scan# 677
 Delta R.T. -0.02 min
 Lab File: BF089279.D
 Acq: 25 Jul 2016 15:12

Tgt Ion:163 Resp: 214108
 Ion Ratio Lower Upper
 163 100
 194 3.0 2.9 4.3
 164 10.3 7.6 11.4

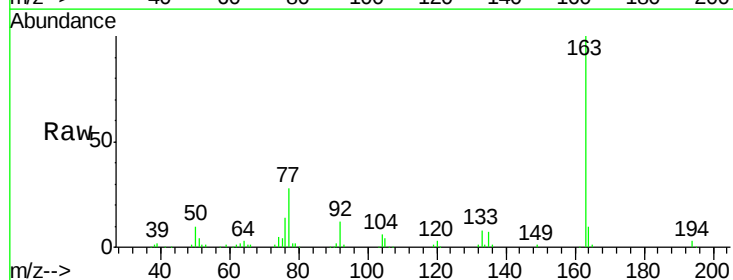

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

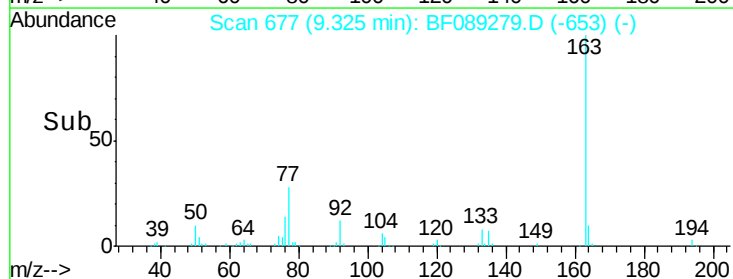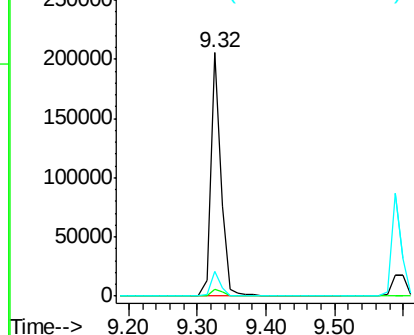


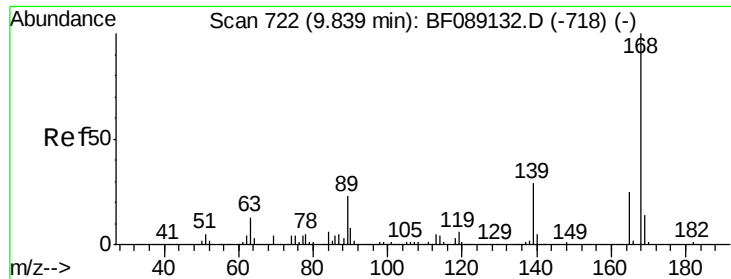




#56
2,4-Dinitrotoluene
Concen: 5.74 ng
RT: 9.59 min Scan# 700
Delta R.T. -0.22 min
Lab File: BF089279.D
Acq: 25 Jul 2016 15:12

Instrument :
BNA_F
ClientSampleId :
KSB-14-5.0-7.0

Tgt Ion:165 Resp: 11241
Ion Ratio Lower Upper
165 100
63 0.0 55.4 83.2#
89 0.0 74.3 111.5#
182 0.0 2.0 3.0#

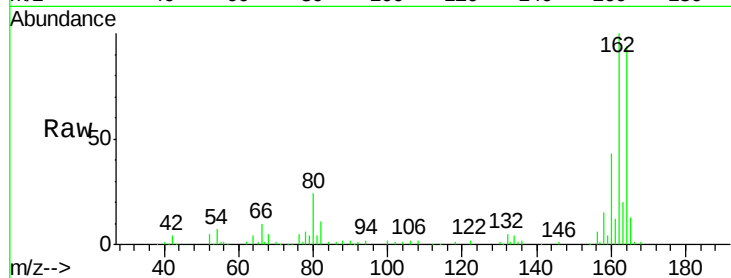


Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0
Ion 182.00 (181.70 to 182.70): E

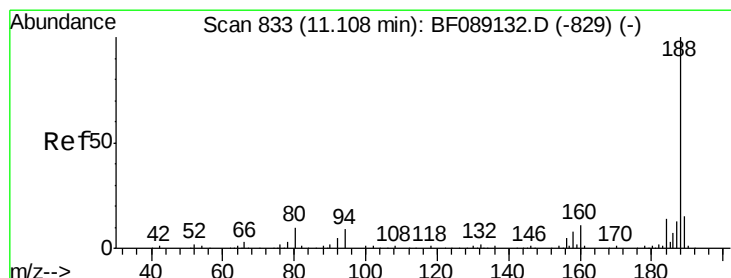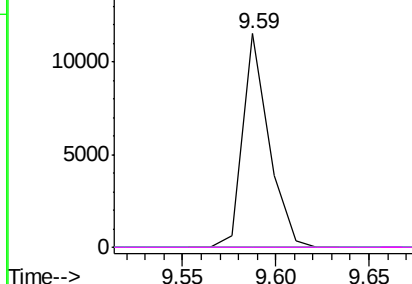
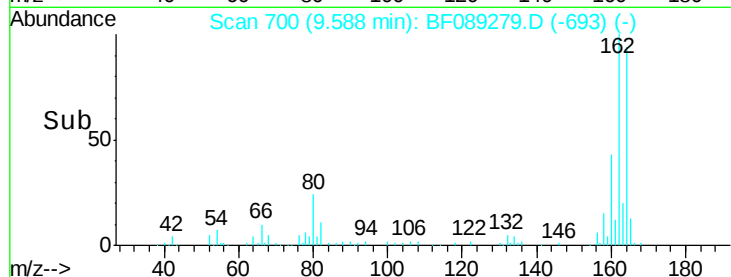



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.06 min Scan# 829
Delta R.T. -0.01 min
Lab File: BF089279.D
Acq: 25 Jul 2016 15:12

Tgt Ion:188 Resp: 147981
Ion Ratio Lower Upper
188 100
94 9.7 7.0 10.4
80 11.0 7.7 11.5

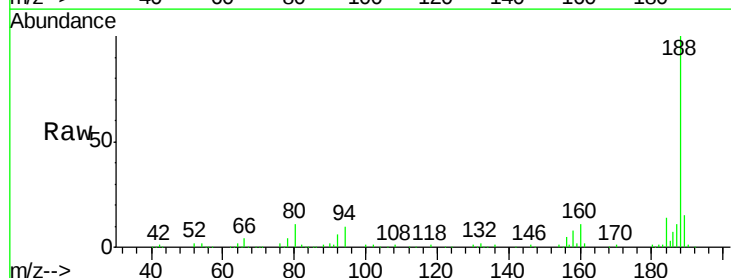

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

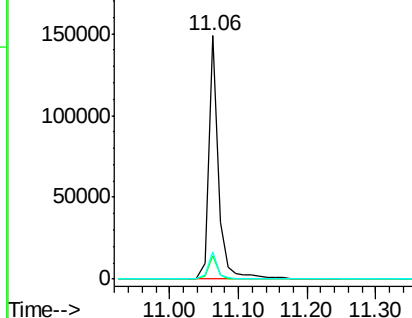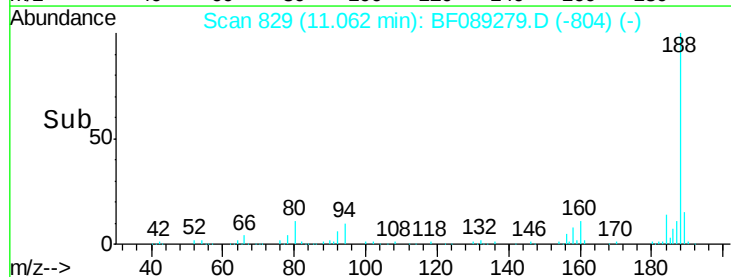

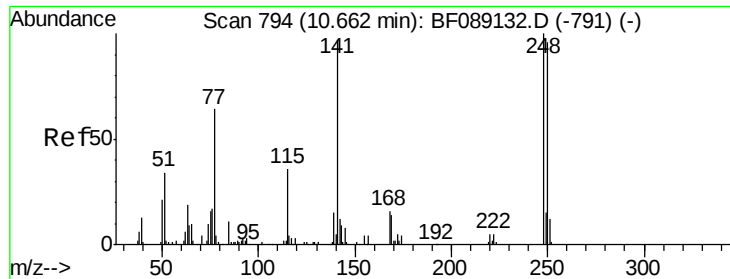

#66

4-Bromophenyl-phenylether

Concen: 4.67 ng

RT: 10.38 min Scan# 769

Delta R.T. -0.25 min

Lab File: BF089279.D

Acq: 25 Jul 2016 15:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-5.0-7.0


Tgt Ion:248 Resp: 6832

Ion Ratio Lower Upper

248 100

250 191.0 76.9 115.3#




141 624.6 77.4 116.2#

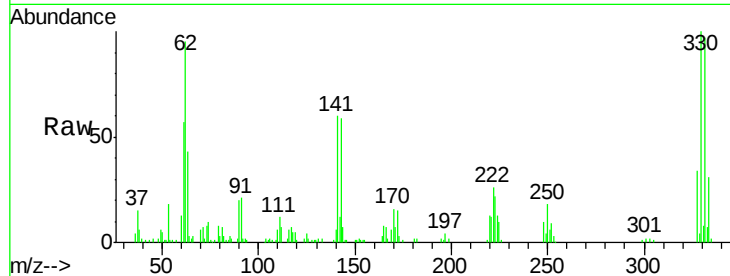

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

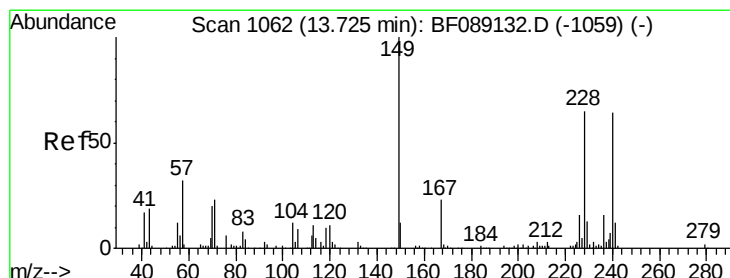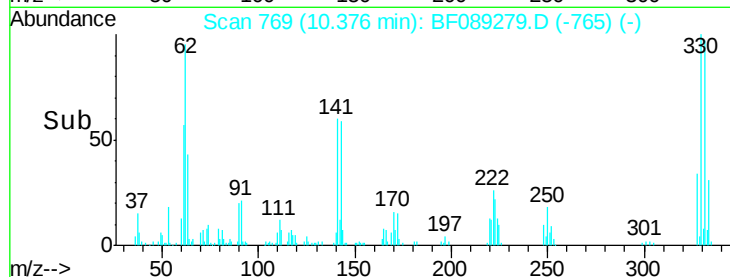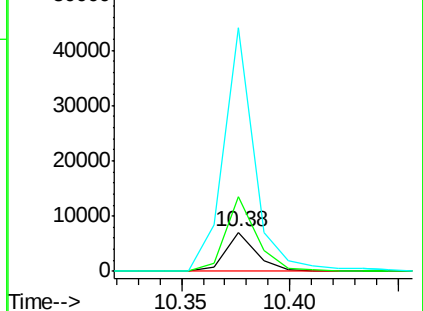

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.68 min Scan# 1058

Delta R.T. -0.01 min

Lab File: BF089279.D

Acq: 25 Jul 2016 15:12


Tgt Ion:240 Resp: 108261

Ion Ratio Lower Upper

240 100

120 13.9 13.6 20.4



236 25.9 20.5 30.7

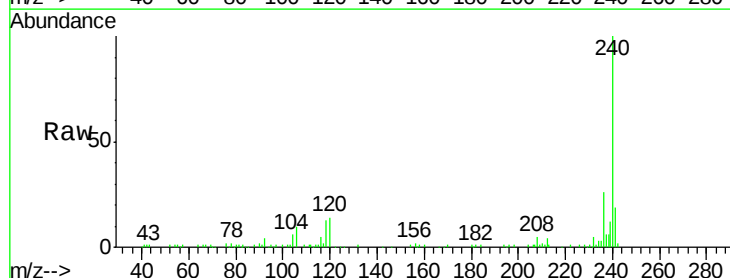


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



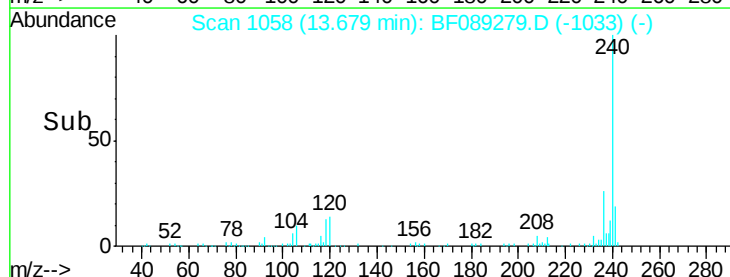
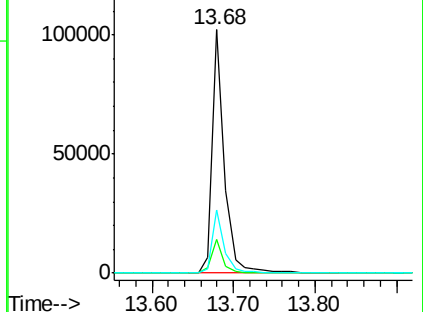


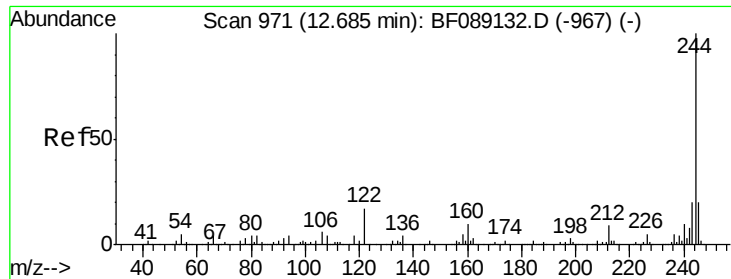

#78
 Terphenyl-d14
 Concen: 66.77 ng
 RT: 12.65 min Scan# 968
 Delta R.T. 0.00 min
 Lab File: BF089279.D
 Acq: 25 Jul 2016 15:12

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-5.0-7.0

Tgt Ion:244 Resp: 333286
 Ion Ratio Lower Upper
 244 100
 212 7.4 7.0 10.4
 122 8.1 13.8 20.8#

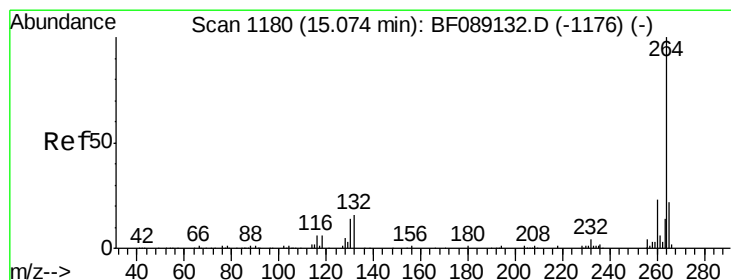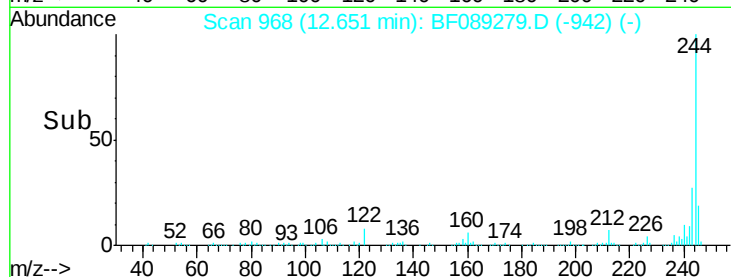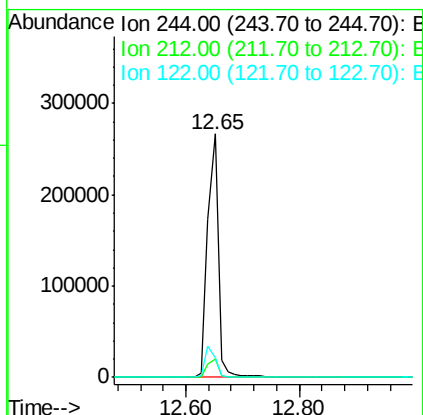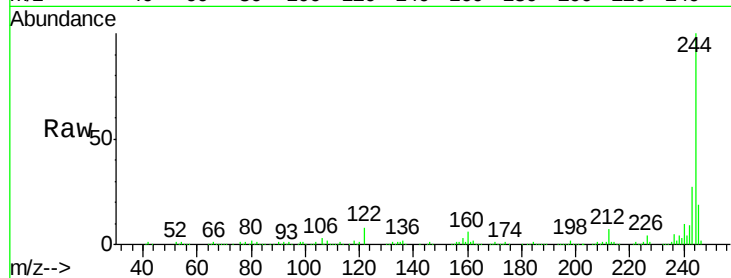

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.02 min Scan# 1175
 Delta R.T. -0.01 min
 Lab File: BF089279.D
 Acq: 25 Jul 2016 15:12

Tgt Ion:264 Resp: 85257
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.5 27.7
 265 22.0 17.3 25.9

