
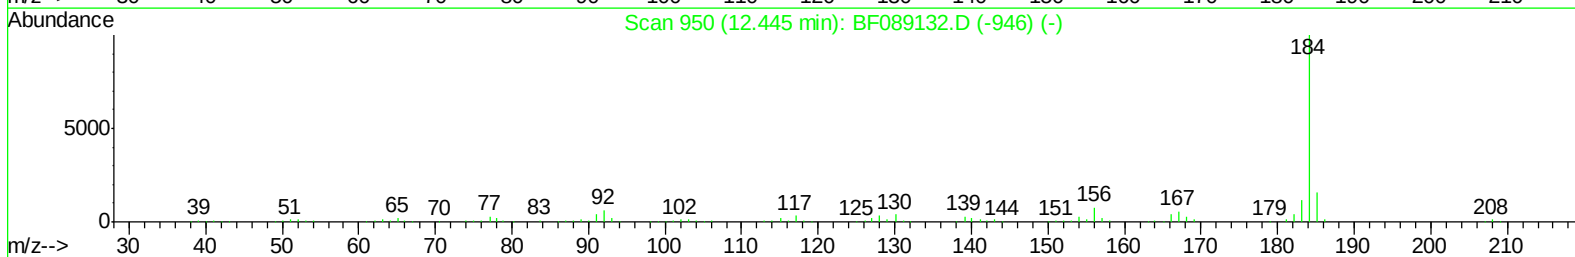
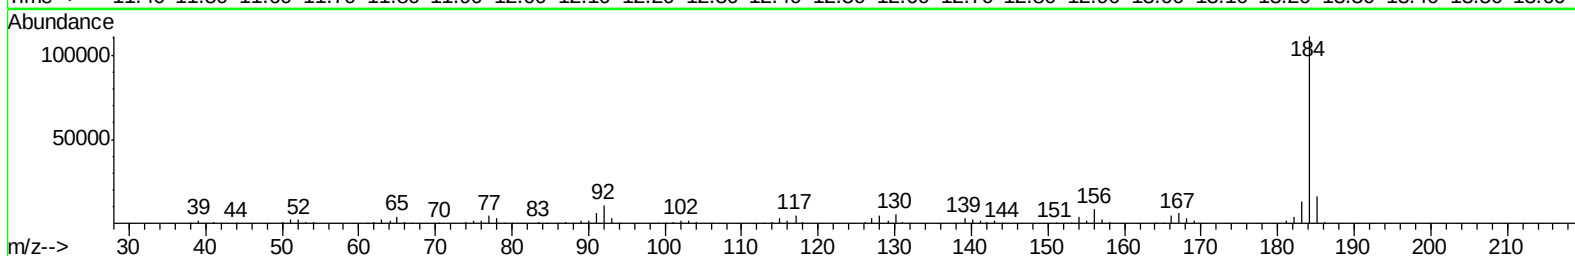


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072516\
Data File : BF089269.D
Acq On : 25 Jul 2016 10:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 05:45:23 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 16:56:43 2016
Response via : Initial Calibration

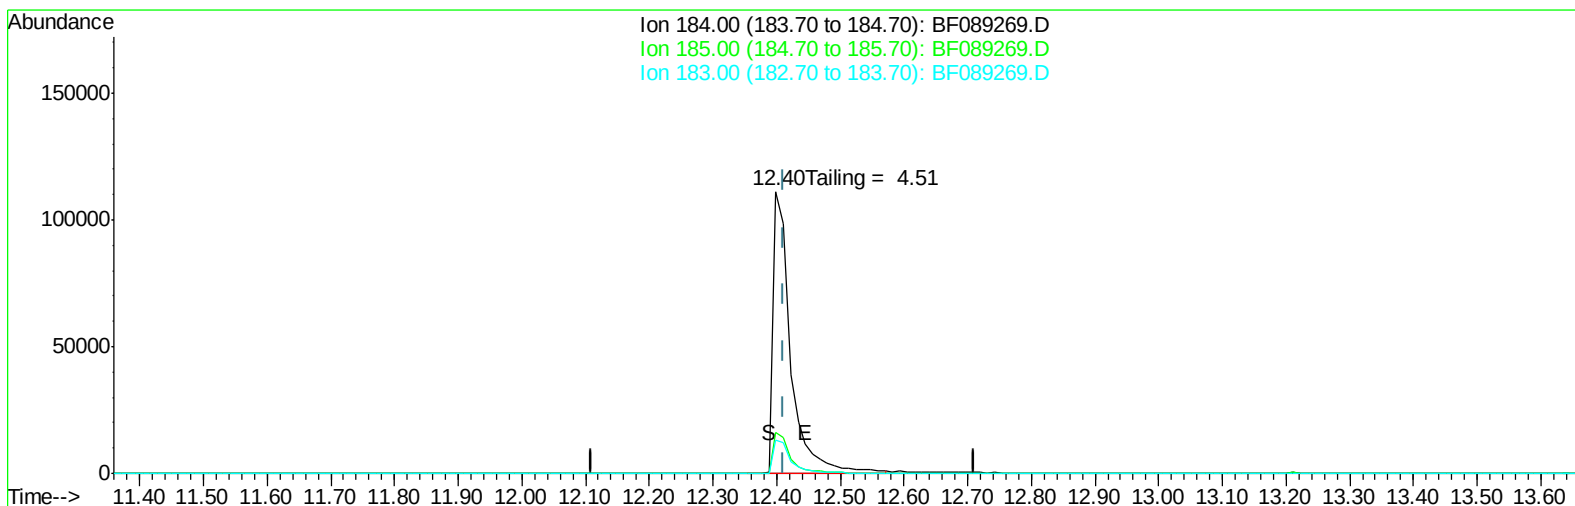

TIC: BF089269.D

(76) Benzidine




12.399min (-0.011) 0.00ng

response 216808

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.42
183.00	12.00	11.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072516\
Data File : BF089269.D
Acq On : 25 Jul 2016 10:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 05:45:23 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 16:56:43 2016
Response via : Initial Calibration

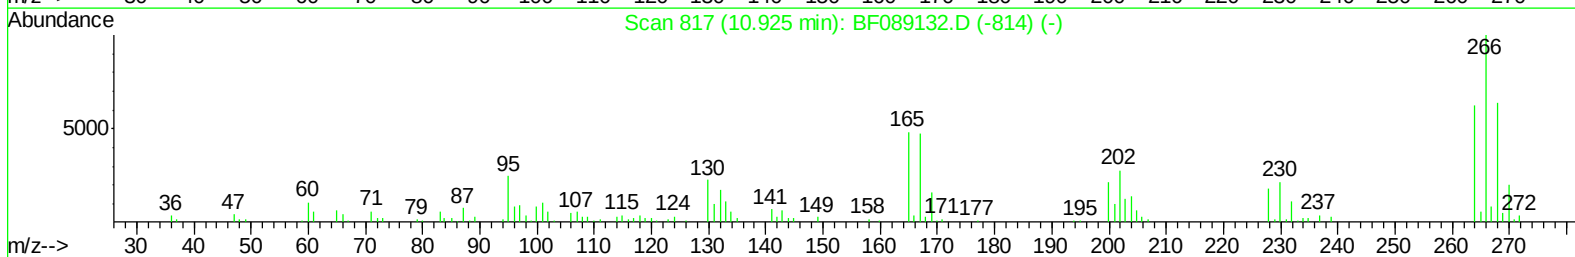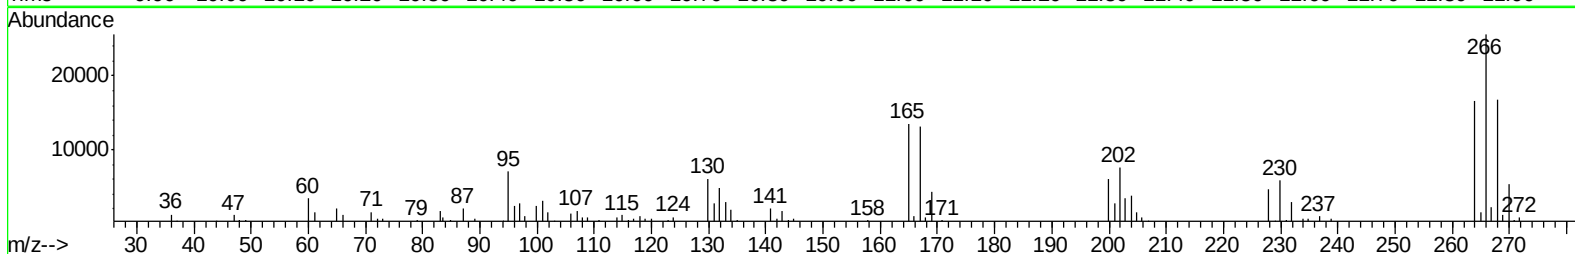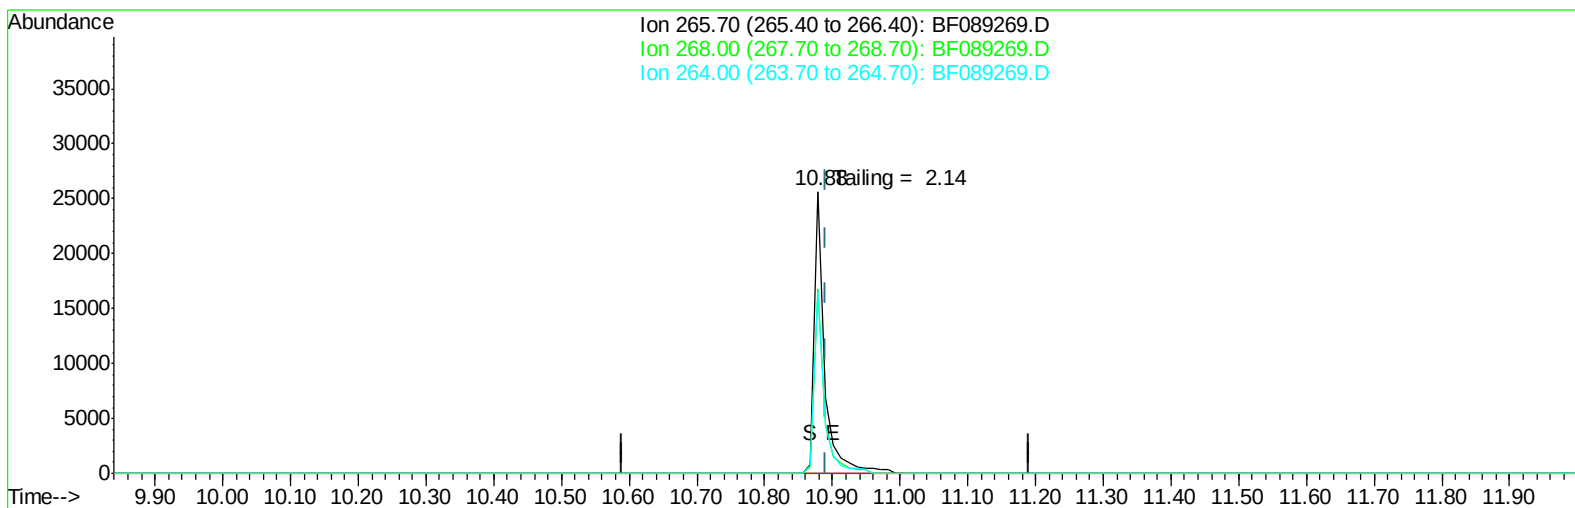

TIC: BF089269.D

(69) Pentachlorophenol (C)

10.879min (-0.011) 0.00ng m

response 27807

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	65.47
264.00	62.10	64.63
0.00	0.00	0.00