

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072516\
 Data File : BF089277.D
 Acq On : 25 Jul 2016 14:12
 Operator : UM/SJ
 Sample : H4129-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-0.2-2.0

Quant Time: Jul 26 12:55:51 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 16:56:43 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.56	152	63044	20.00	ng	-0.01
21) Naphthalene-d8	7.85	136	237074	20.00	ng	0.00
38) Acenaphthene-d10	9.59	164	100586	20.00	ng	-0.01
63) Phenanthrene-d10	11.06	188	169618	20.00	ng	-0.01
75) Chrysene-d12	13.68	240	118301	20.00	ng	-0.01
86) Perylene-d12	15.03	264	95697	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.14	112	357282	86.19	ng	0.00
7) Phenol-d6	6.23	99	511397	95.67	ng	0.00
23) Nitrobenzene-d5	7.13	82	292668	65.59	ng	-0.01
41) 2,4,6-Tribromophenol	10.38	330	70928	78.32	ng	-0.01
44) 2-Fluorobiphenyl	8.92	172	485375	66.49	ng	-0.01
78) Terphenyl-d14	12.65	244	322274	59.09	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	7.87	128	27546	2.15	ng	98
37) 2-Methylnaphthalene	8.56	142	29141	3.57	ng	97
49) Dimethylphthalate	9.32	163	182782	23.68	ng	99
70) Phenanthrene	11.08	178	27887	3.00	ng	99
74) Fluoranthene	12.26	202	29257	2.99	ng	98
77) Pyrene	12.49	202	25980	2.66	ng	97
80) Benzo(a)anthracene	13.67	228	16251	2.16	ng	# 82
87) Benzo(b)fluoranthene	14.67	252	15604m	2.25	ng	


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072516\
Data File : BF089277.D
Acq On : 25 Jul 2016 14:12
Operator : UM/SJ
Sample : H4129-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KSB-14-0.2-2.0

Quant Time: Jul 26 12:55:51 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 16:56:43 2016
Response via : Initial Calibration

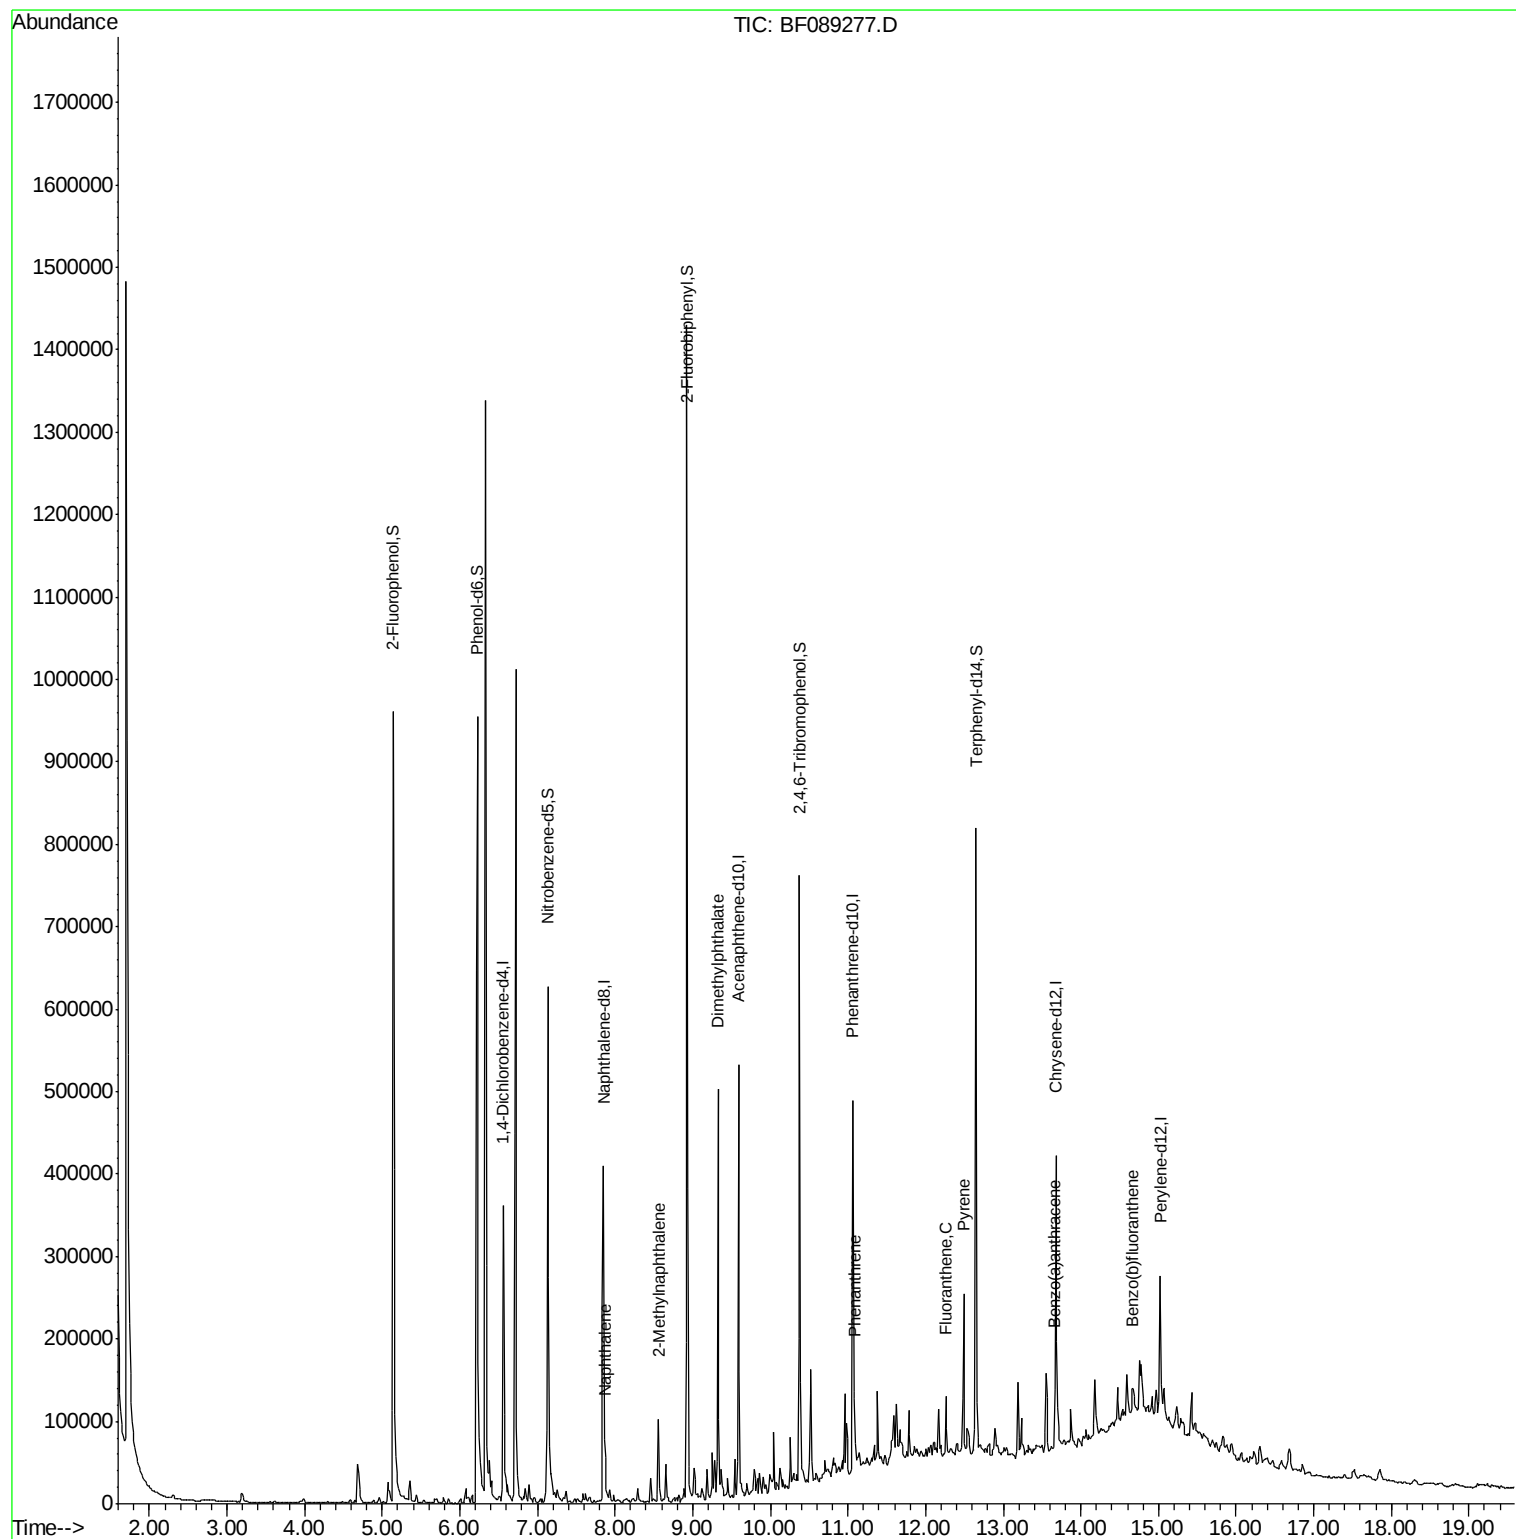

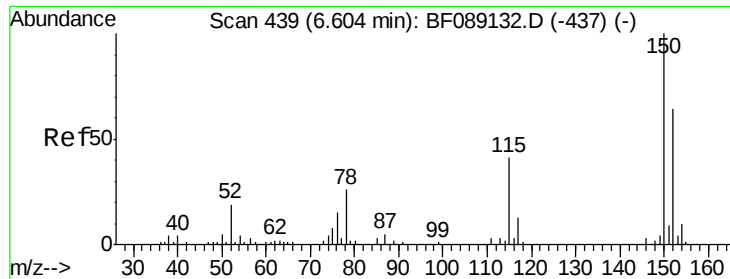

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.56 min Scan# 435

Delta R.T. -0.01 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-0.2-2.0


Tot Ion:152 Resp: 63044

Ion Ratio Lower Upper

152 100

150 156.7 125.1 187.7




115 68.4 51.1 76.7

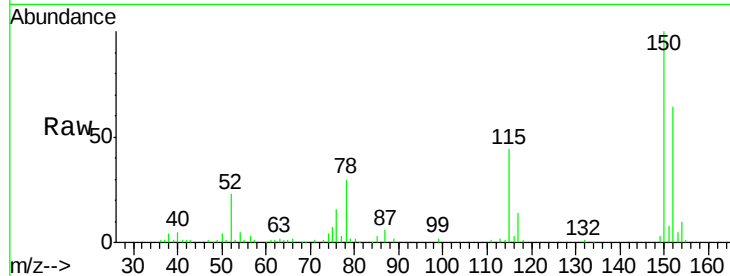

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

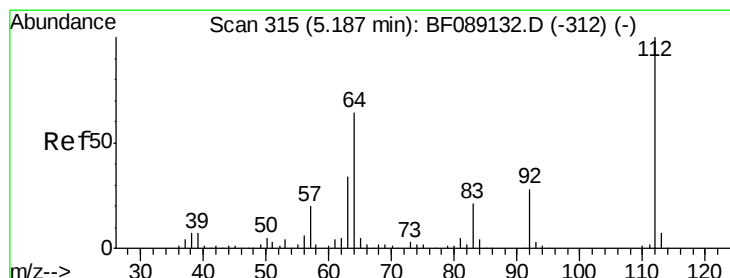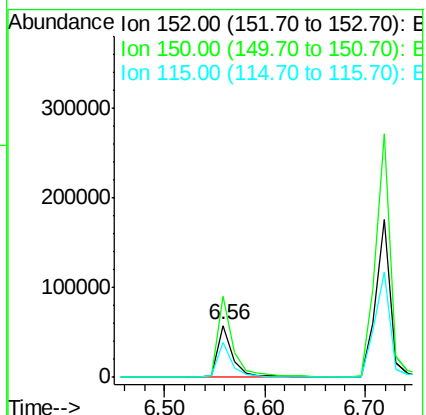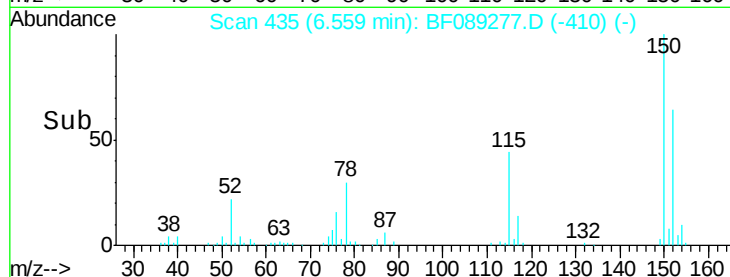

#5

2-Fluorophenol

Concen: 86.19 ng

RT: 5.14 min Scan# 311

Delta R.T. -0.00 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12


Tgt Ion:112 Resp: 357282

Ion Ratio Lower Upper

112 100

64 61.9 51.0 76.4



63 33.8 27.3 40.9

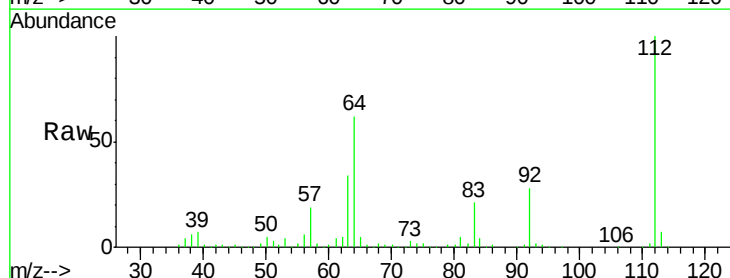


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

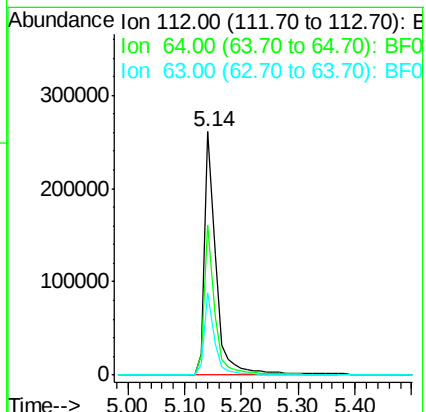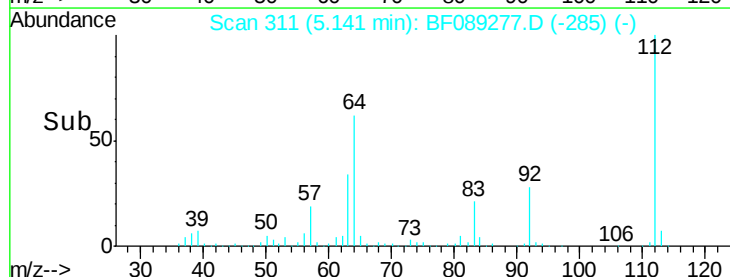

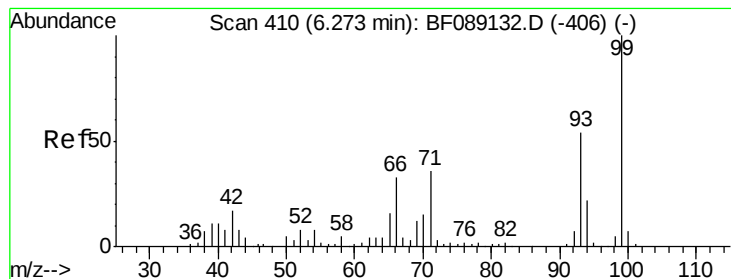

#7

Phenol-d6

Concen: 95.67 ng

RT: 6.23 min Scan# 406

Delta R.T. -0.00 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-0.2-2.0





Tot Ion: 99 Resp: 511397

Ion Ratio Lower Upper

99 100

42 15.2 13.5 20.3

71 34.7 28.9 43.3

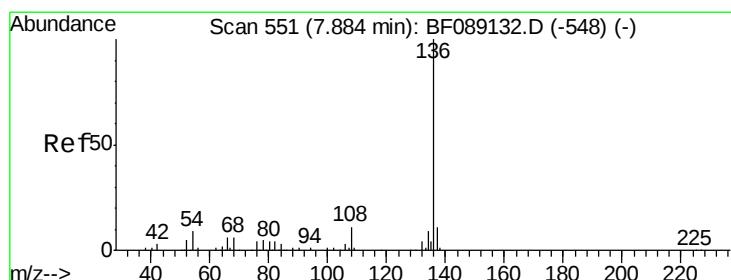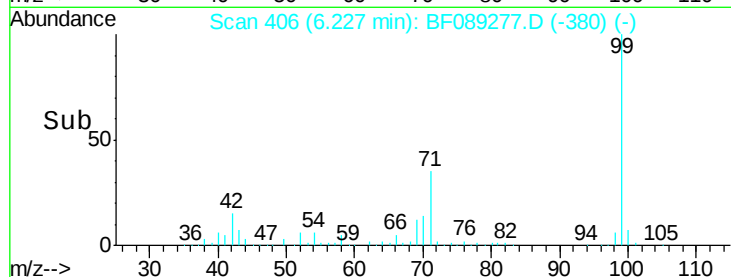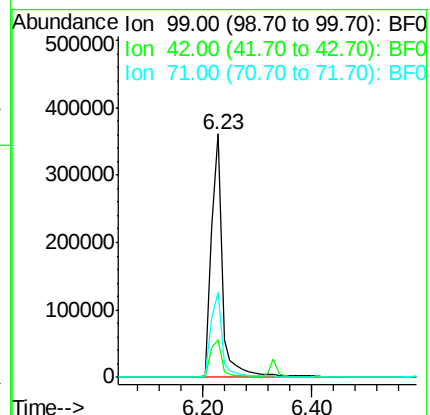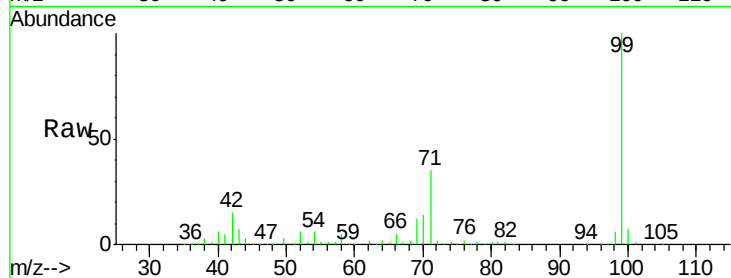

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.85 min Scan# 548

Delta R.T. -0.00 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12

Tgt Ion: 136 Resp: 237074




Ion Ratio Lower Upper


136 100

137 10.5 8.8 13.2

54 5.6 7.0 10.4#

68 4.6 5.0 7.6#

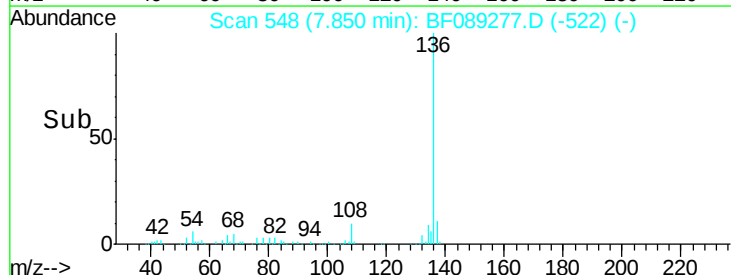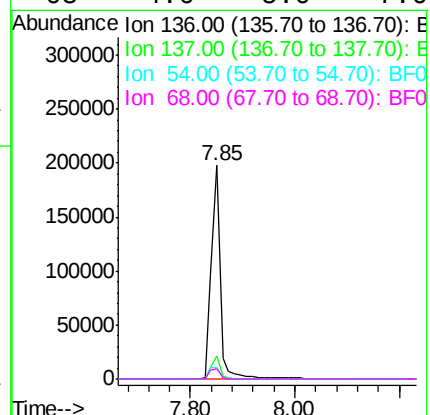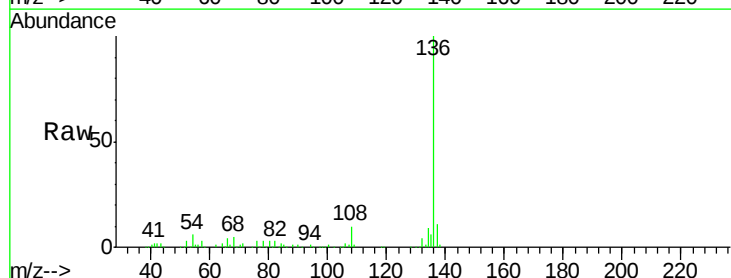

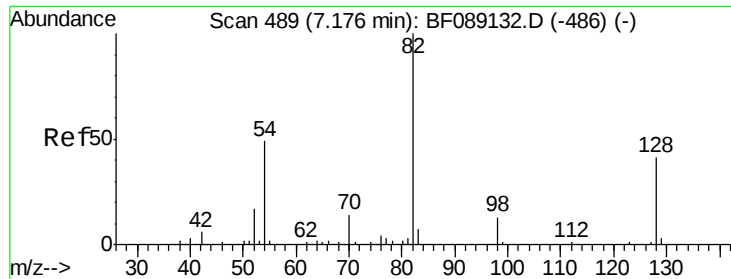

#23

Nitrobenzene-d5

Concen: 65.59 ng

RT: 7.13 min Scan# 485

Delta R.T. -0.01 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-0.2-2.0


Tot Ion: 82 Resp: 292668

Ion Ratio Lower Upper




82 100

128 38.7 33.0 49.6

54 49.1 39.0 58.4

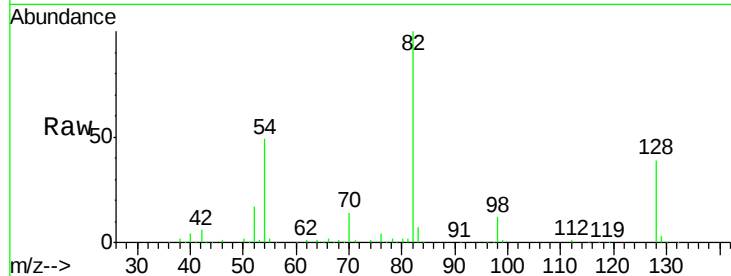

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

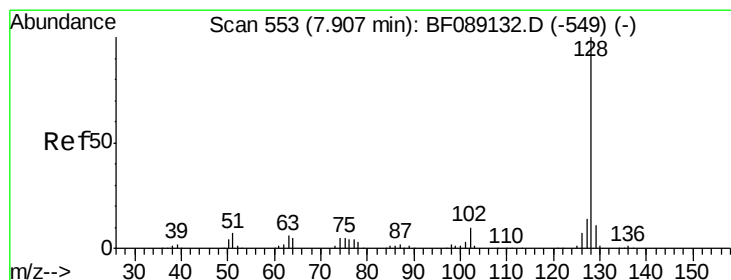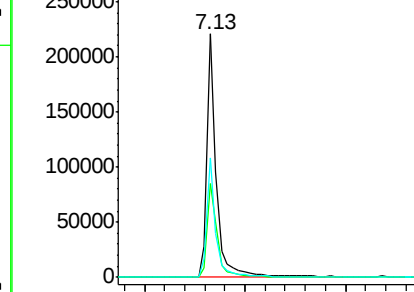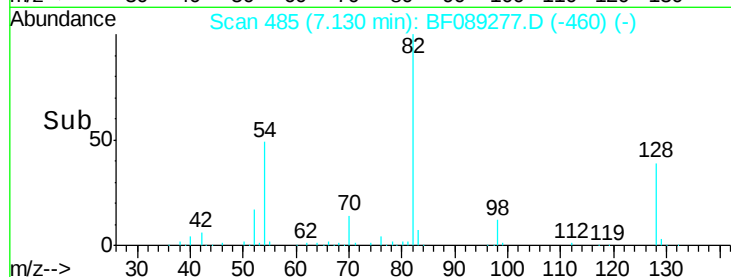

#31

Naphthalene

Concen: 2.15 ng

RT: 7.87 min Scan# 550

Delta R.T. -0.00 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12


Tgt Ion: 128 Resp: 27546

Ion Ratio Lower Upper



128 100


129 11.6 8.9 13.3

127 12.8 10.8 16.2

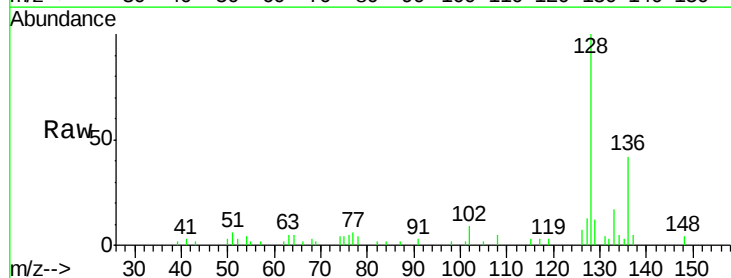

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E



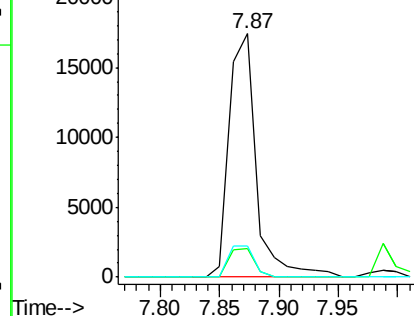
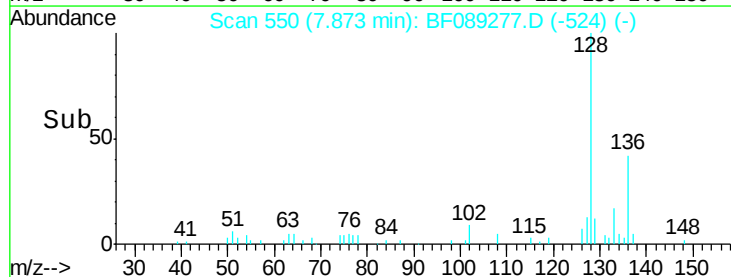


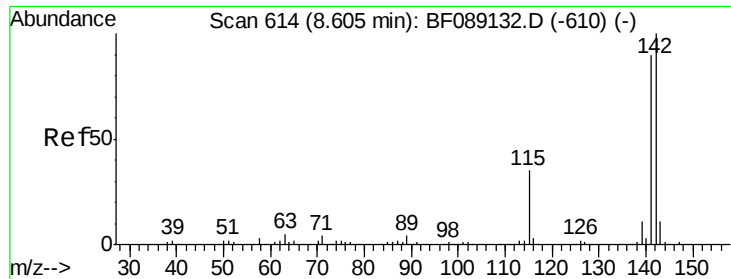

#37
 2-Methylnaphthalene
 Concen: 3.57 ng
 RT: 8.56 min Scan# 610
 Delta R.T. -0.01 min
 Lab File: BF089277.D
 Acq: 25 Jul 2016 14:12




Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-0.2-2.0


Tot Ion:142 Resp: 29141
 Ion Ratio Lower Upper
 142 100
 141 87.4 71.6 107.4
 115 37.8 27.6 41.4

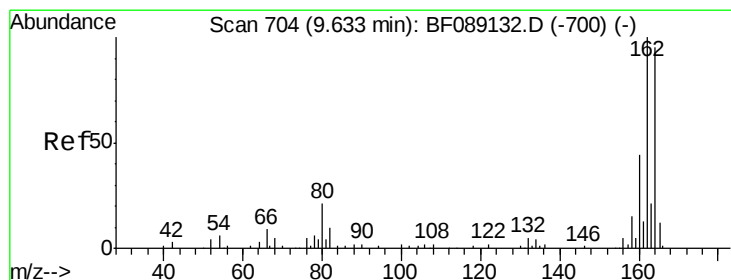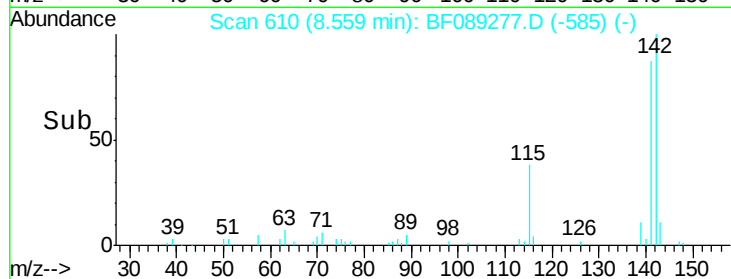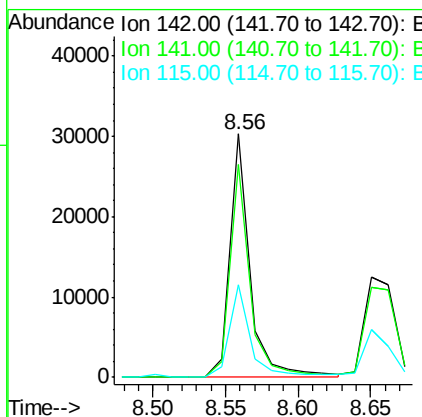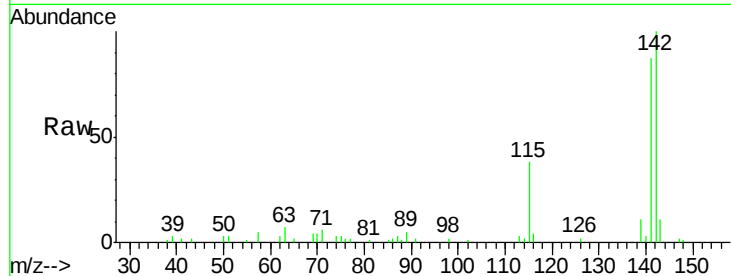

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.59 min Scan# 700
 Delta R.T. -0.01 min
 Lab File: BF089277.D
 Acq: 25 Jul 2016 14:12

Tgt Ion:164 Resp: 100586
 Ion Ratio Lower Upper
 164 100
 162 105.7 84.1 126.1
 160 46.9 37.1 55.7

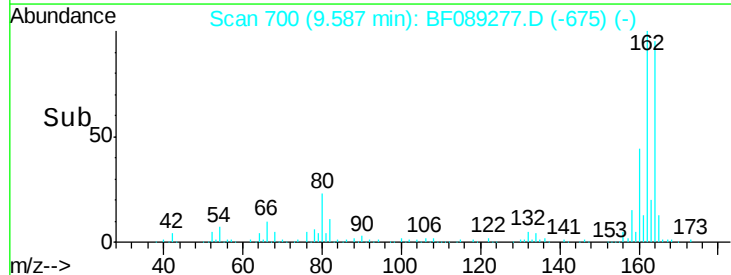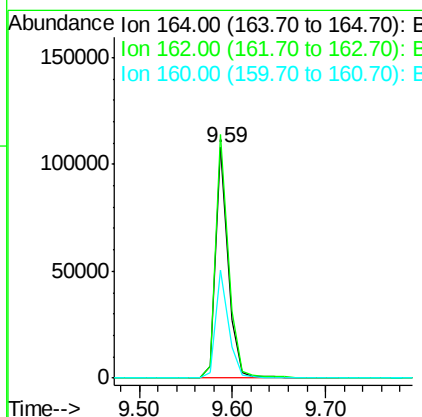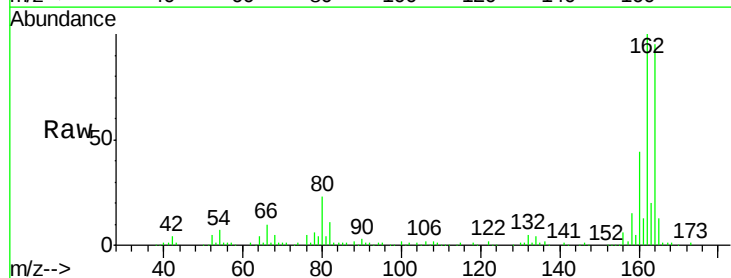


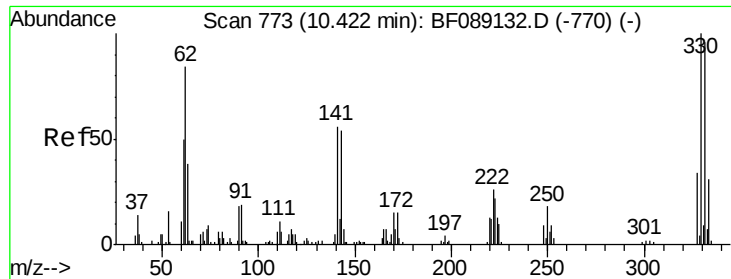




#41
 2,4,6-Tribromophenol
 Concen: 78.32 ng
 RT: 10.38 min Scan# 769
 Delta R.T. -0.01 min
 Lab File: BF089277.D
 Acq: 25 Jul 2016 14:12

Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-0.2-2.0

Tot Ion:330 Resp: 70928
 Ion Ratio Lower Upper
 330 100
 332 96.8 77.2 115.8
 141 57.0 42.2 63.2

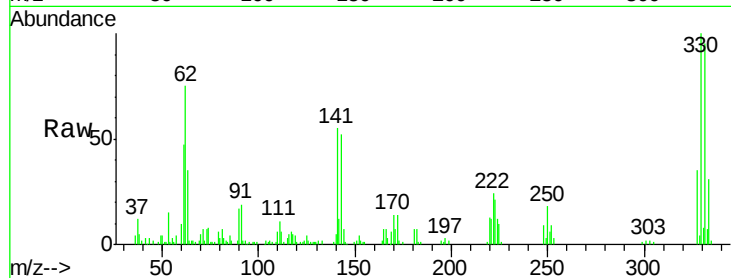


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

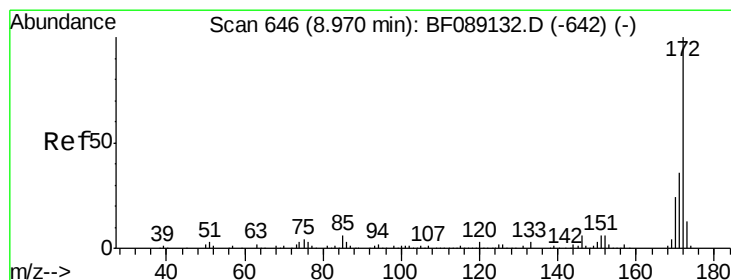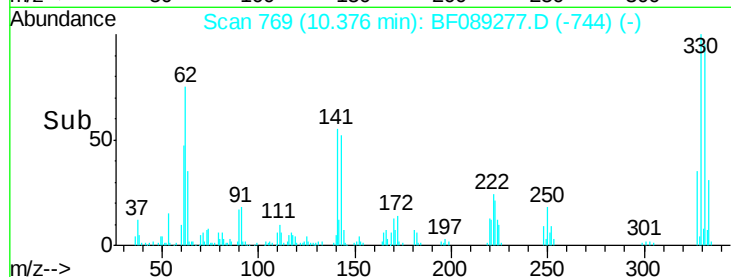
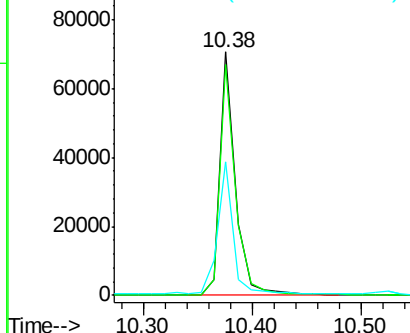



#44
 2-Fluorobiphenyl
 Concen: 66.49 ng
 RT: 8.92 min Scan# 642
 Delta R.T. -0.01 min
 Lab File: BF089277.D
 Acq: 25 Jul 2016 14:12

Tgt Ion:172 Resp: 485375
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.2 43.8
 170 23.6 19.1 28.7

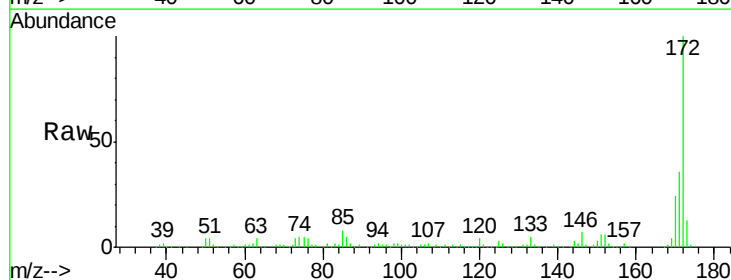

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



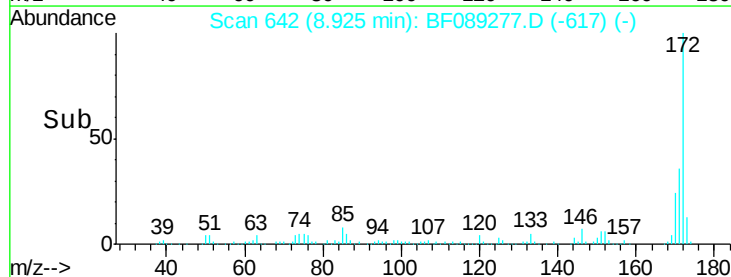
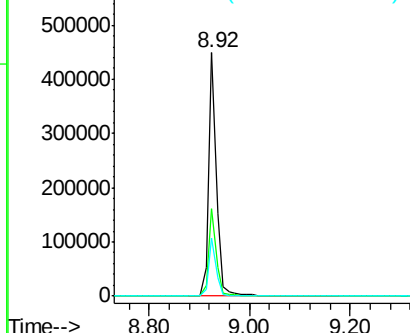


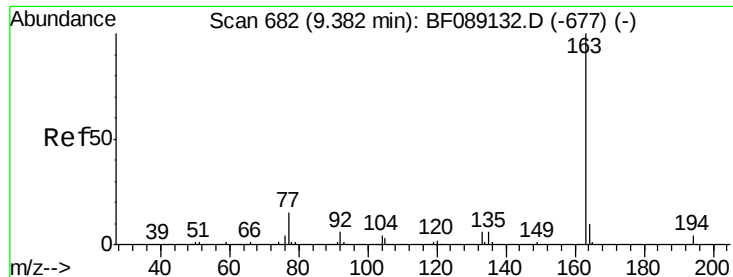

#49
Dimethylphthalate
Concen: 23.68 ng
RT: 9.32 min Scan# 677
Delta R.T. -0.02 min
Lab File: BF089277.D
Acq: 25 Jul 2016 14:12




Instrument :
BNA_F
ClientSampleId :
KSB-14-0.2-2.0


Tot Ion:163 Resp: 182782
Ion Ratio Lower Upper
163 100
194 3.1 2.9 4.3
164 10.0 7.6 11.4

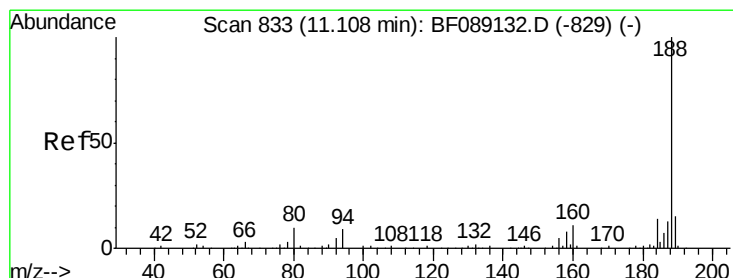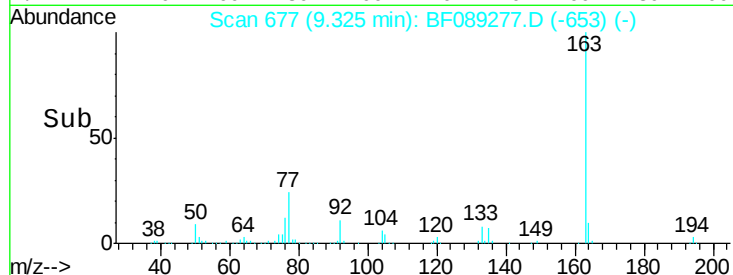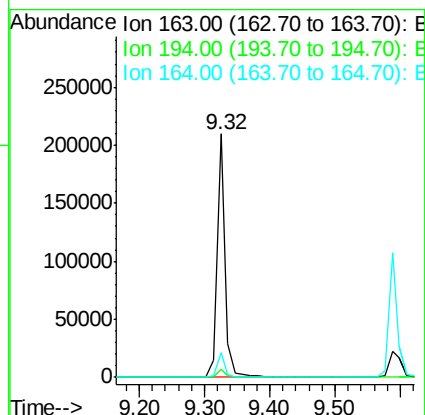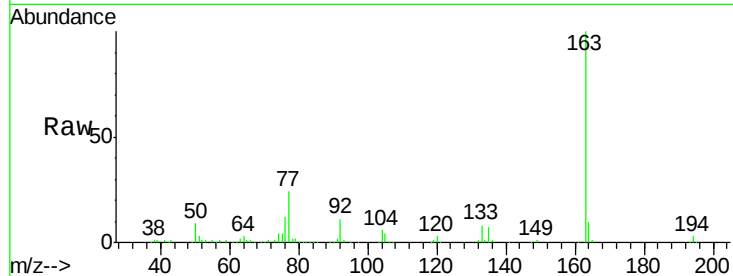

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.06 min Scan# 829
Delta R.T. -0.01 min
Lab File: BF089277.D
Acq: 25 Jul 2016 14:12

Tgt Ion:188 Resp: 169618
Ion Ratio Lower Upper
188 100
94 9.6 7.0 10.4
80 10.4 7.7 11.5

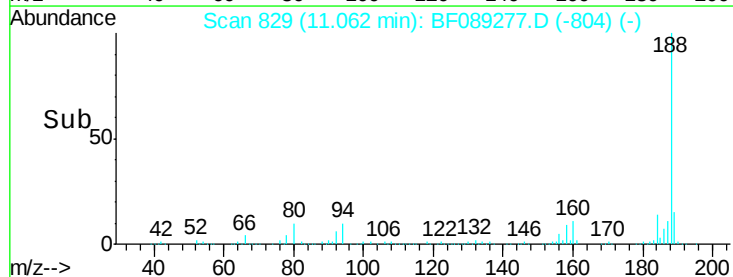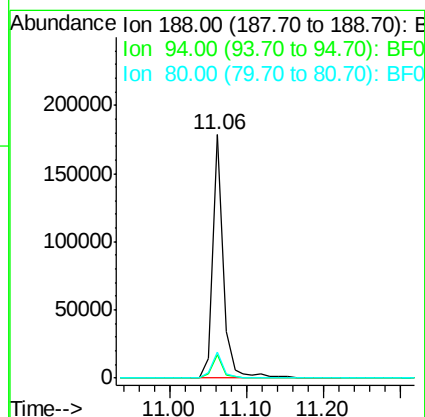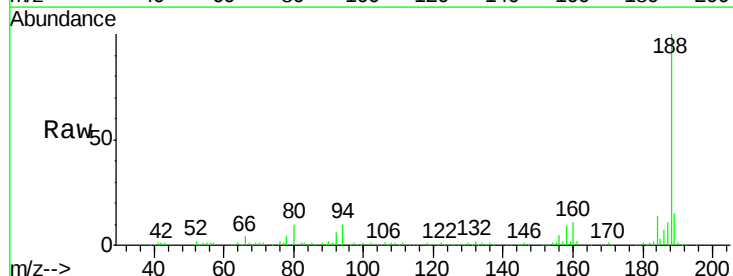

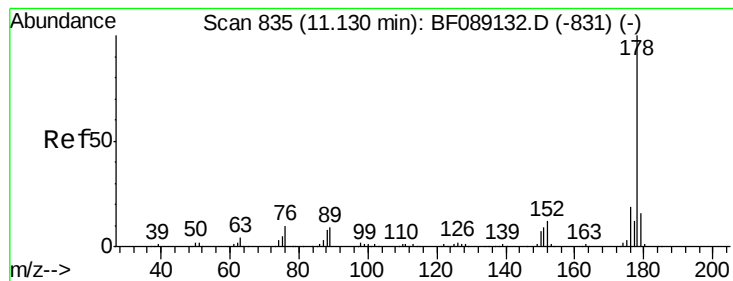

#70

Phenanthrene

Concen: 3.00 ng

RT: 11.08 min Scan# 831

Delta R.T. -0.01 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-0.2-2.0


Tot Ion:178 Resp: 27887

Ion Ratio Lower Upper

178 100

176 19.4 15.6 23.4




179 16.8 12.4 18.6

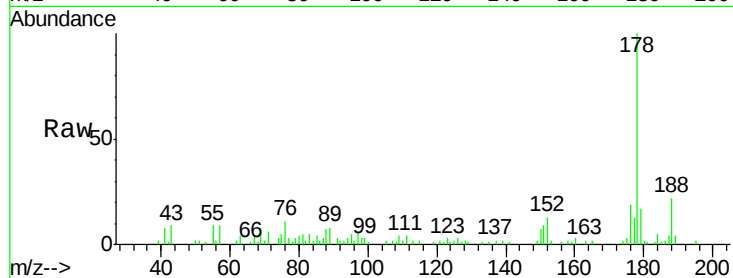

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

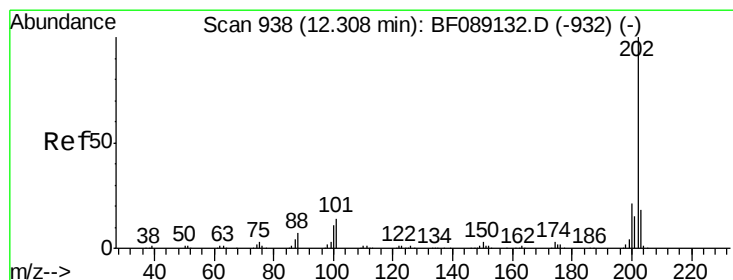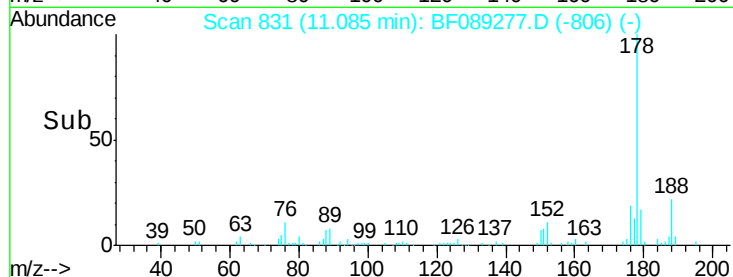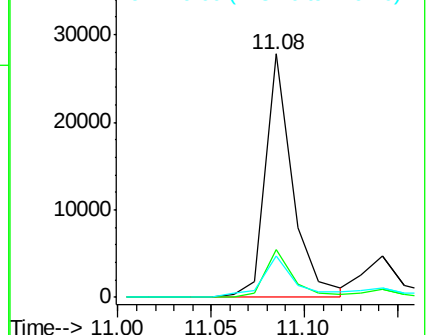

#74

Fluoranthene

Concen: 2.99 ng

RT: 12.26 min Scan# 934

Delta R.T. -0.01 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12


Tgt Ion:202 Resp: 29257

Ion Ratio Lower Upper

202 100

101 14.0 0.0 34.0



203 19.2 0.0 37.8

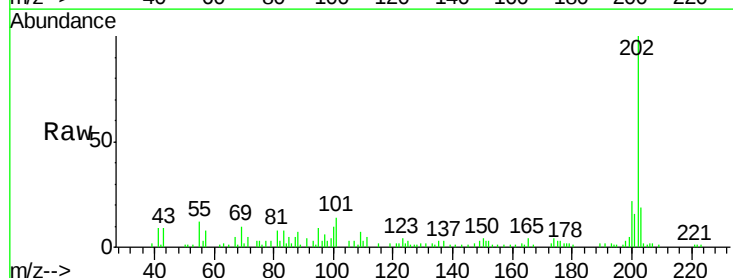


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

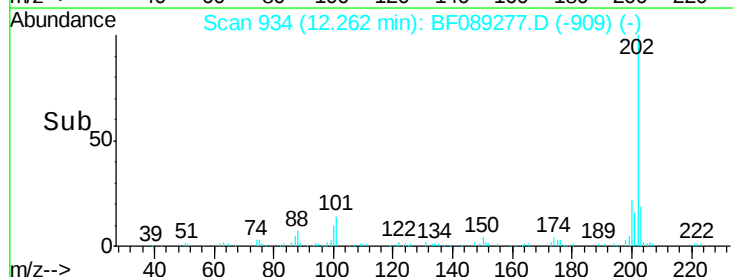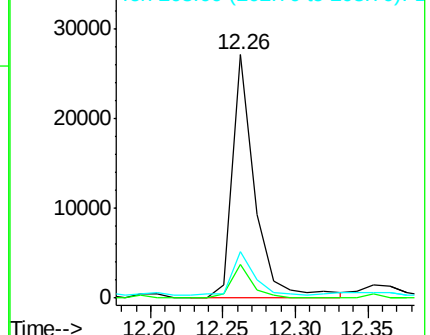

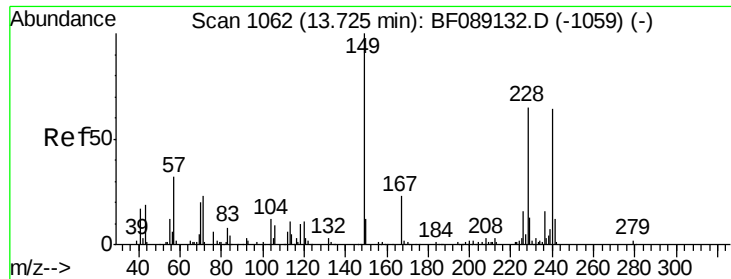

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.68 min Scan# 1058

Delta R.T. -0.01 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-0.2-2.0


Tot Ion:240 Resp: 118301

Ion Ratio Lower Upper

240 100

120 14.4 13.6 20.4




236 25.1 20.5 30.7

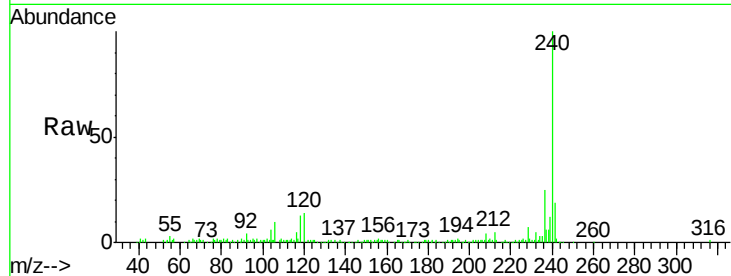

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

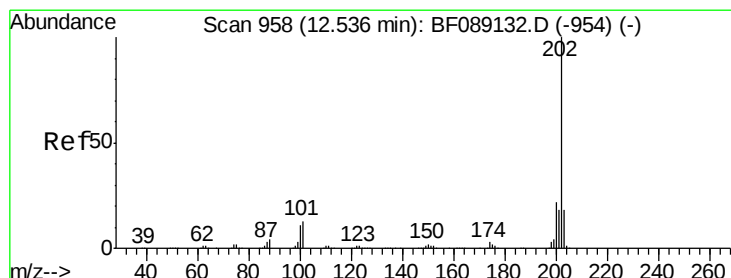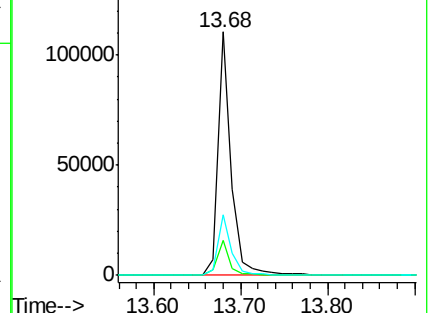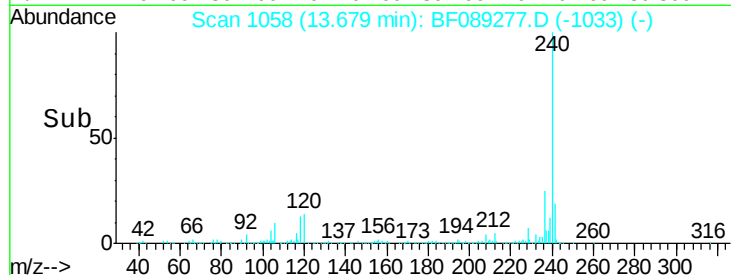

#77

Pyrene

Concen: 2.66 ng

RT: 12.49 min Scan# 954

Delta R.T. -0.00 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12


Tgt Ion:202 Resp: 25980

Ion Ratio Lower Upper

202 100

200 20.8 17.4 26.0



203 19.5 14.2 21.2

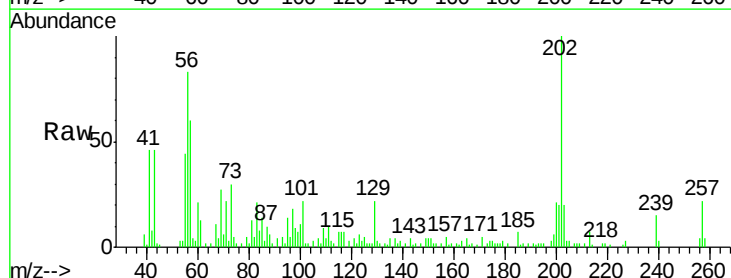


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



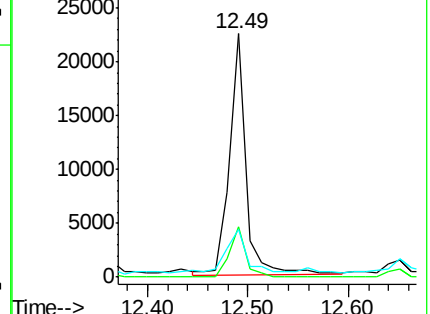
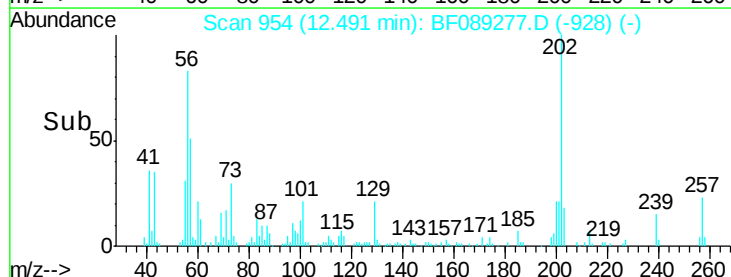


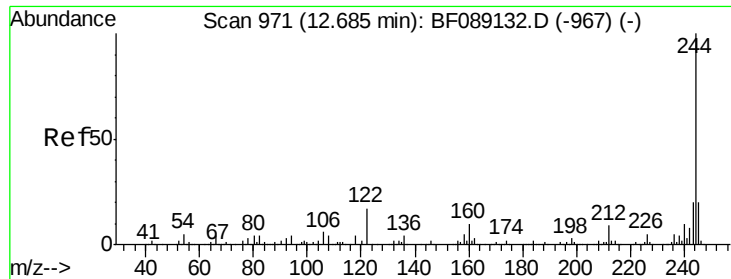

#78
 Terphenyl-d14
 Concen: 59.09 ng
 RT: 12.65 min Scan# 968
 Delta R.T. -0.00 min
 Lab File: BF089277.D
 Acq: 25 Jul 2016 14:12




Instrument :
 BNA_F
 ClientSampleId :
 KSB-14-0.2-2.0


Tot Ion:244 Resp: 322274
 Ion Ratio Lower Upper
 244 100
 212 7.3 7.0 10.4
 122 8.2 13.8 20.8#

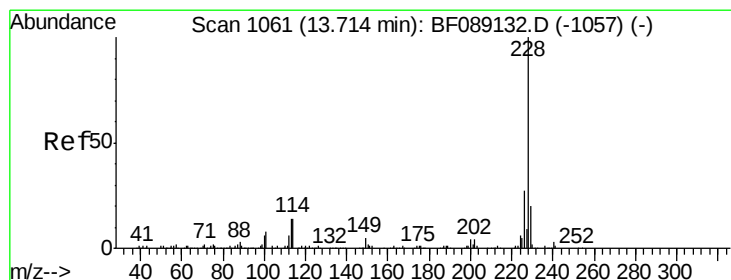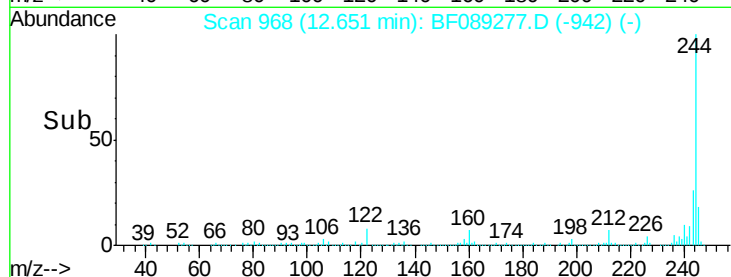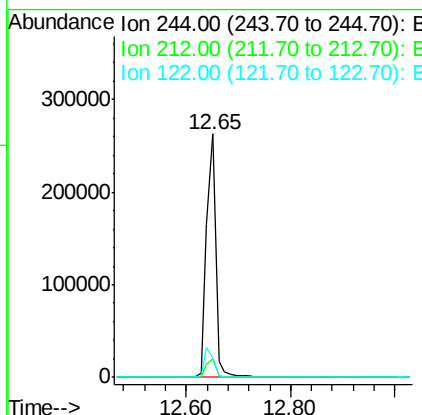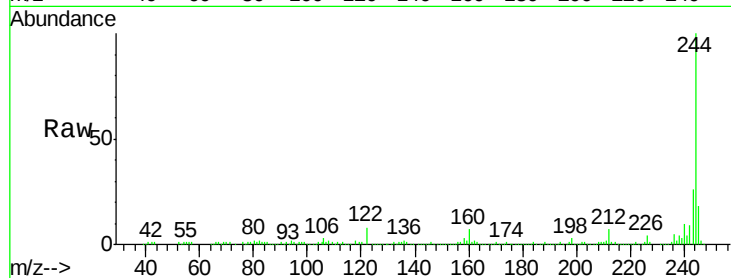

#80
 Benzo(a)anthracene
 Concen: 2.16 ng
 RT: 13.67 min Scan# 1057
 Delta R.T. -0.01 min
 Lab File: BF089277.D
 Acq: 25 Jul 2016 14:12

Tgt Ion:228 Resp: 16251
 Ion Ratio Lower Upper
 228 100
 226 36.7 21.8 32.8#
 229 28.0 15.8 23.8#

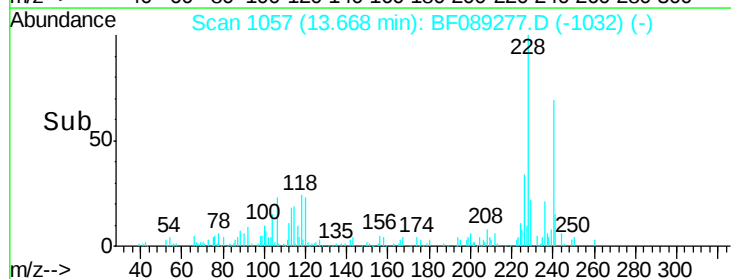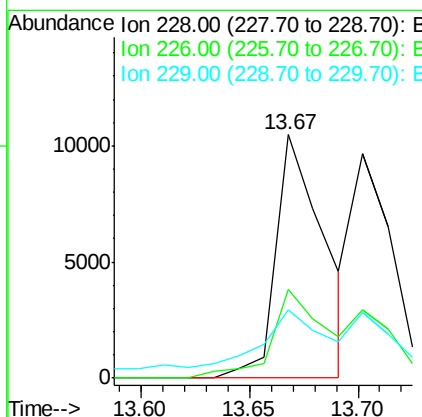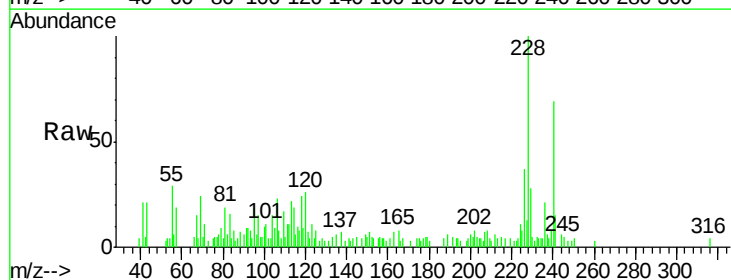

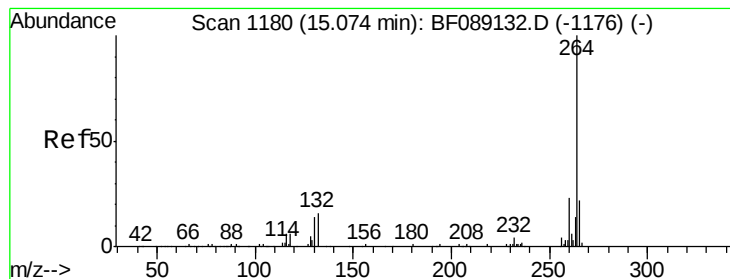

#86

Pervlene-d12

Concen: 20.00 ng

RT: 15.03 min Scan# 1176

Delta R.T. -0.00 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12

Instrument :

BNA_F

ClientSampleId :

KSB-14-0.2-2.0


Tot Ion:264 Resp: 95697

Ion Ratio Lower Upper

264 100

260 22.6 18.5 27.7




265 21.6 17.3 25.9

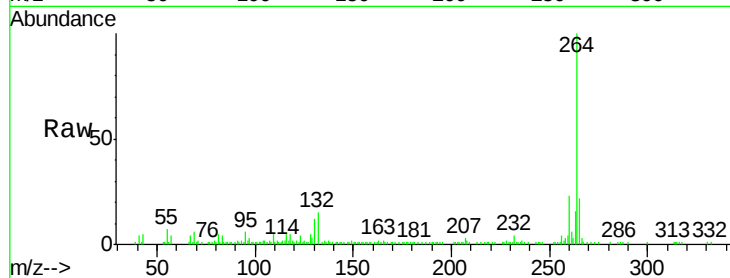

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

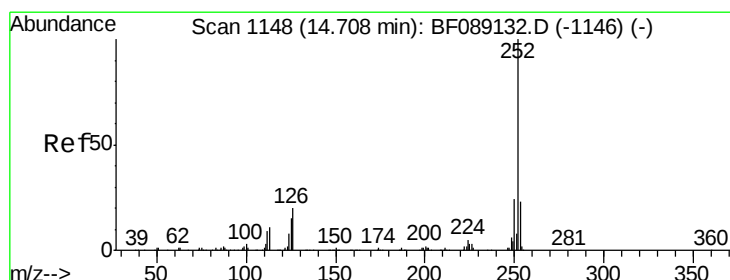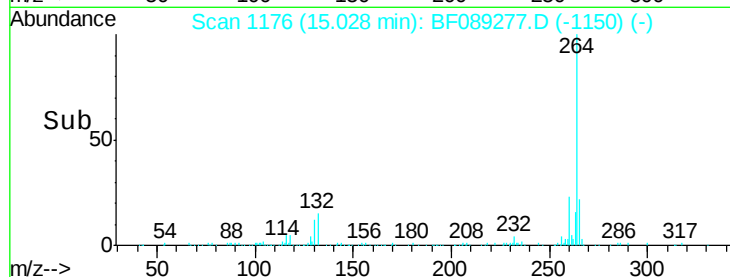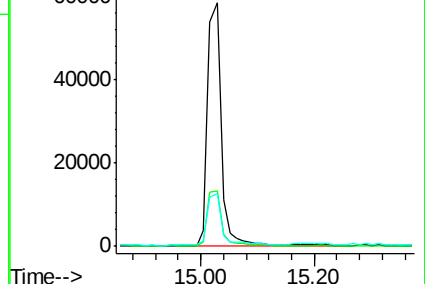

#87

Benzo(b)fluoranthene

Concen: 2.25 ng m

RT: 14.67 min Scan# 1145

Delta R.T. -0.00 min

Lab File: BF089277.D

Acq: 25 Jul 2016 14:12


Tgt Ion:252 Resp: 15604

Ion Ratio Lower Upper

252 100

253 26.4 18.2 27.2

125 22.8 11.9 17.9#

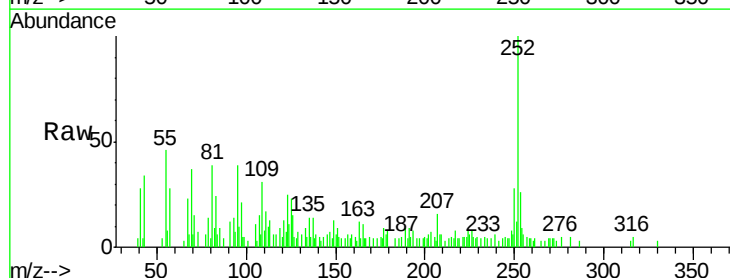

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

