


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072516\
 Data File : BF089269.D
 Acq On : 25 Jul 2016 10:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 25 16:56:43 2016

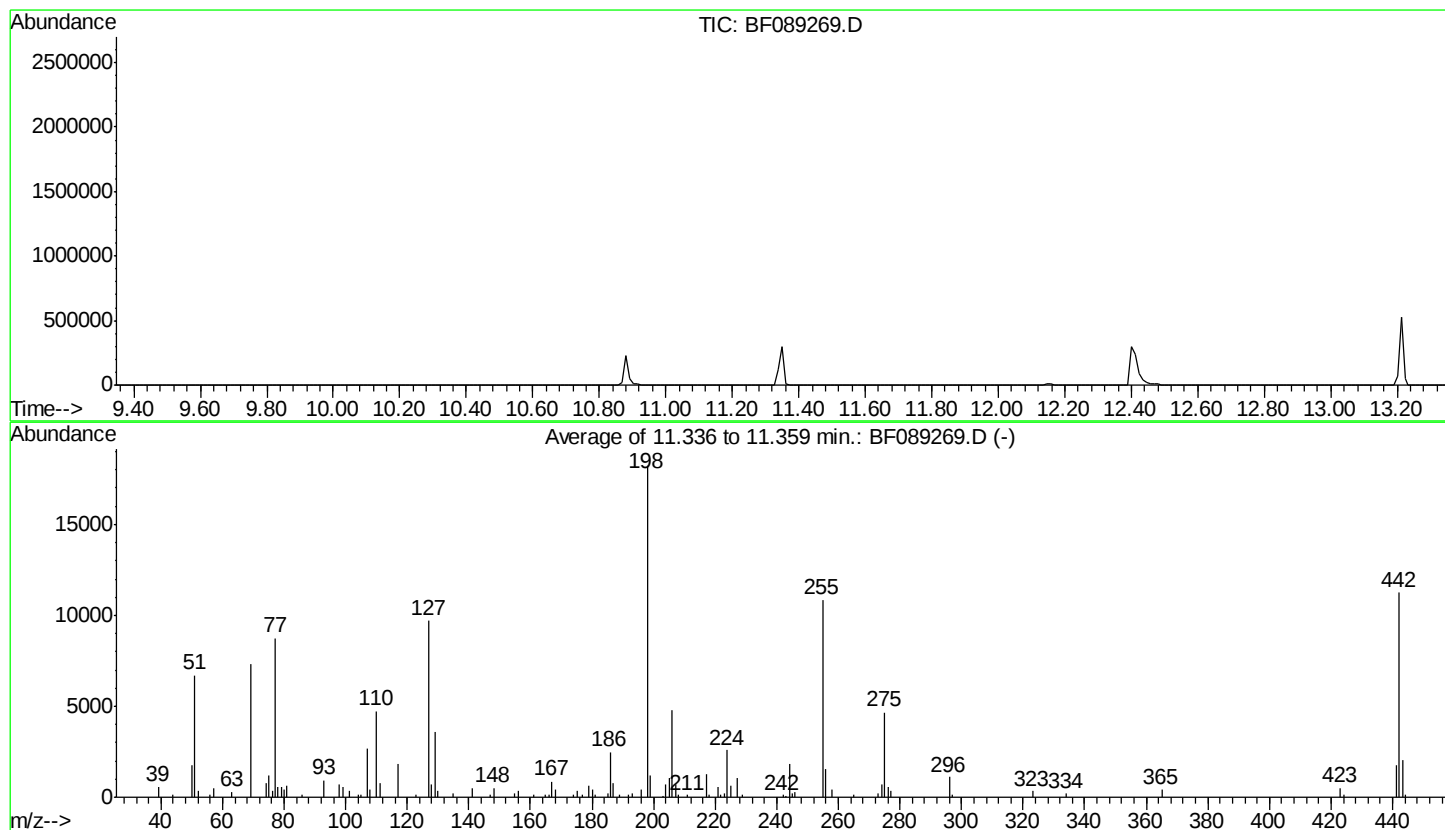

AutoFind: Scans 853, 854, 855; Background Corrected with Scan 850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	6692	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.3	7347	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	9709	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18231	PASS
199	198	5	9	6.4	1175	PASS
275	198	10	60	25.7	4678	PASS
365	198	1	100	2.3	418	PASS
441	442	0.01	24	15.7	1760	PASS
442	198	50	100	61.6	11238	PASS
443	442	15	24	18.3	2060	PASS