


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072516\
 Data File : BF089294.D
 Acq On : 26 Jul 2016 00:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 25 16:56:43 2016

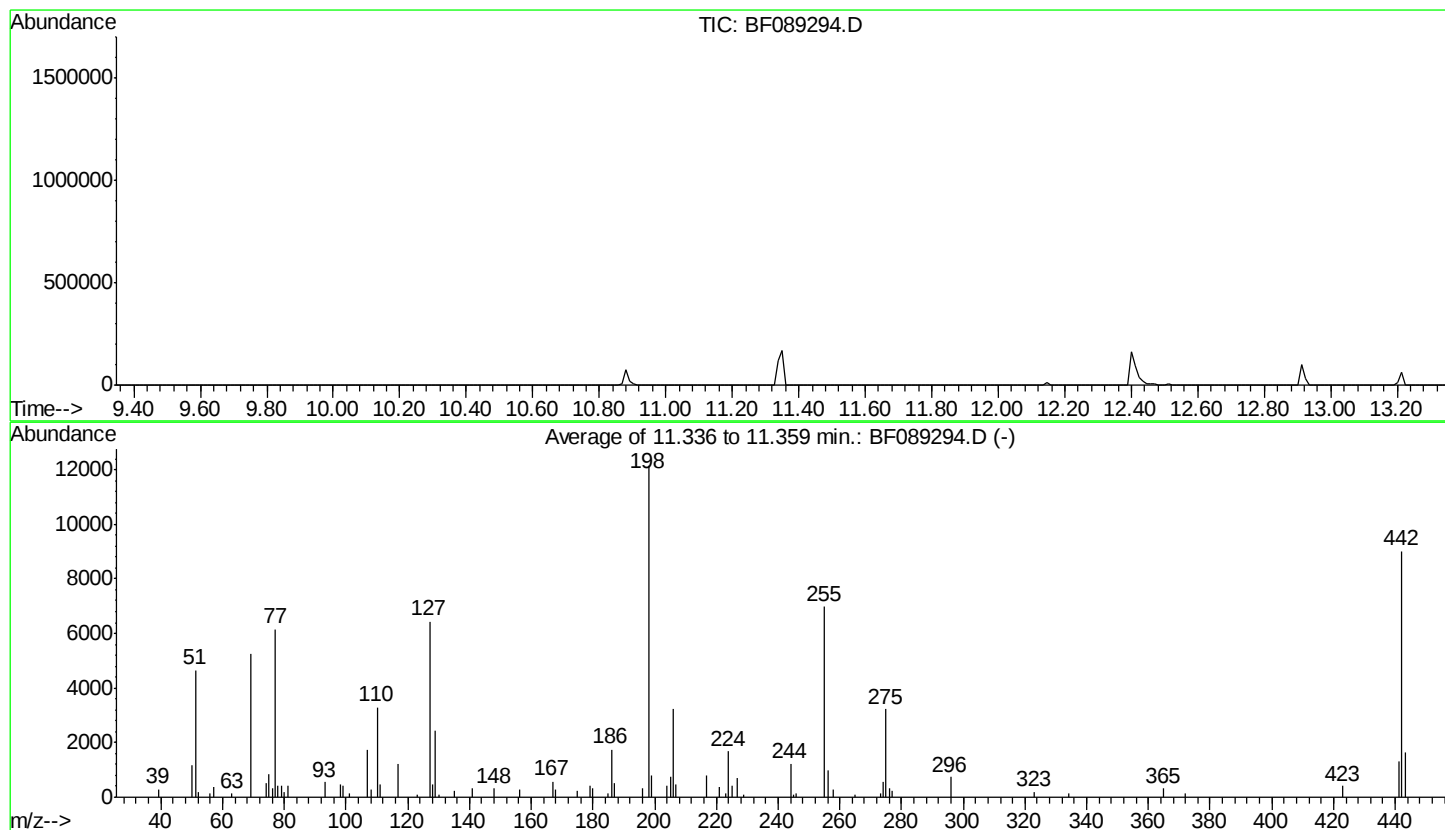

AutoFind: Scans 853, 854, 855; Background Corrected with Scan 850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	4661	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.1	5231	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.9	6429	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12144	PASS
199	198	5	9	6.5	792	PASS
275	198	10	60	26.5	3216	PASS
365	198	1	100	2.6	321	PASS
441	442	0.01	24	14.3	1291	PASS
442	198	50	100	74.3	9024	PASS
443	442	15	24	18.1	1637	PASS