
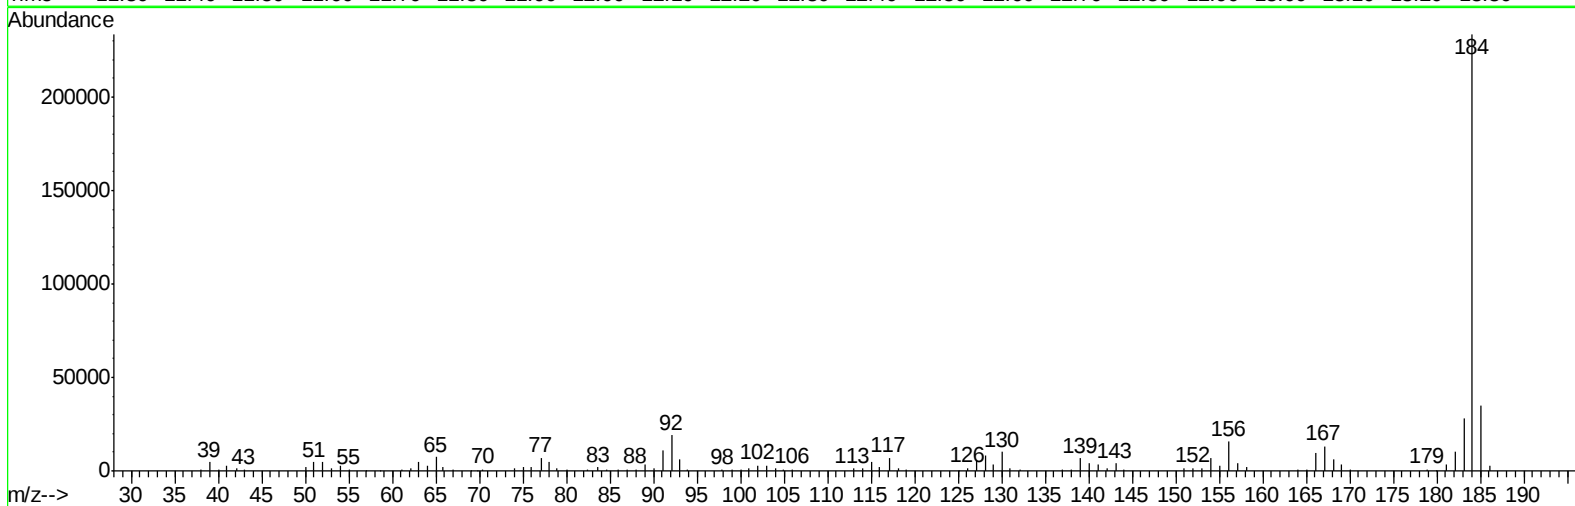


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072517\
 Data File : BF097051.D
 Acq On : 26 Jul 2017 2:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 07:15:51 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 14:11:51 2017
 Response via : Initial Calibration

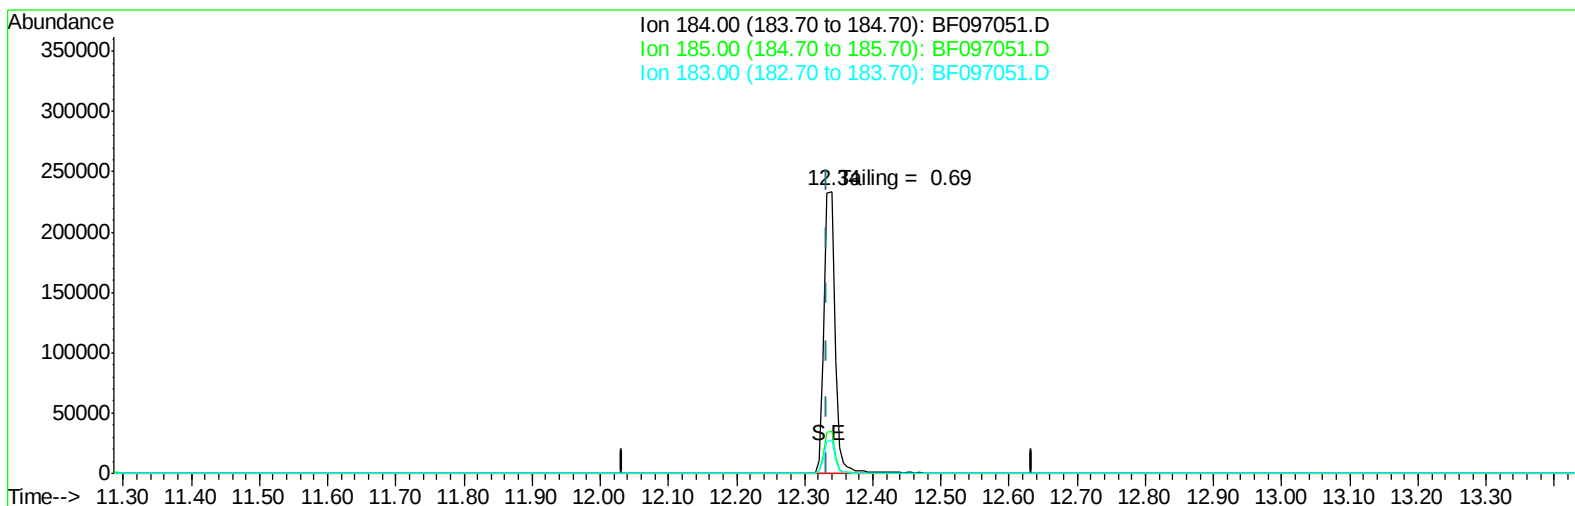

TIC: BF097051.D

(76) Benzidine



12.339min (+0.006) 0.00ng

response 253912

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.97#
183.00	12.20	11.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072517\
Data File : BF097051.D
Acq On : 26 Jul 2017 2:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 07:15:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

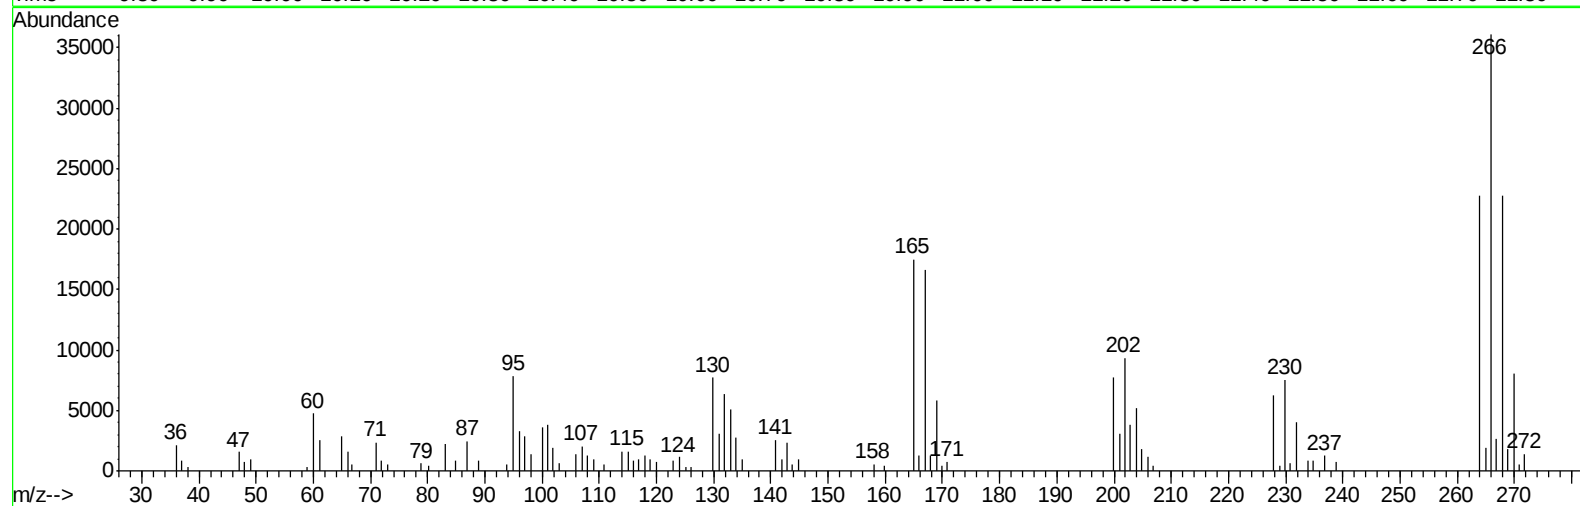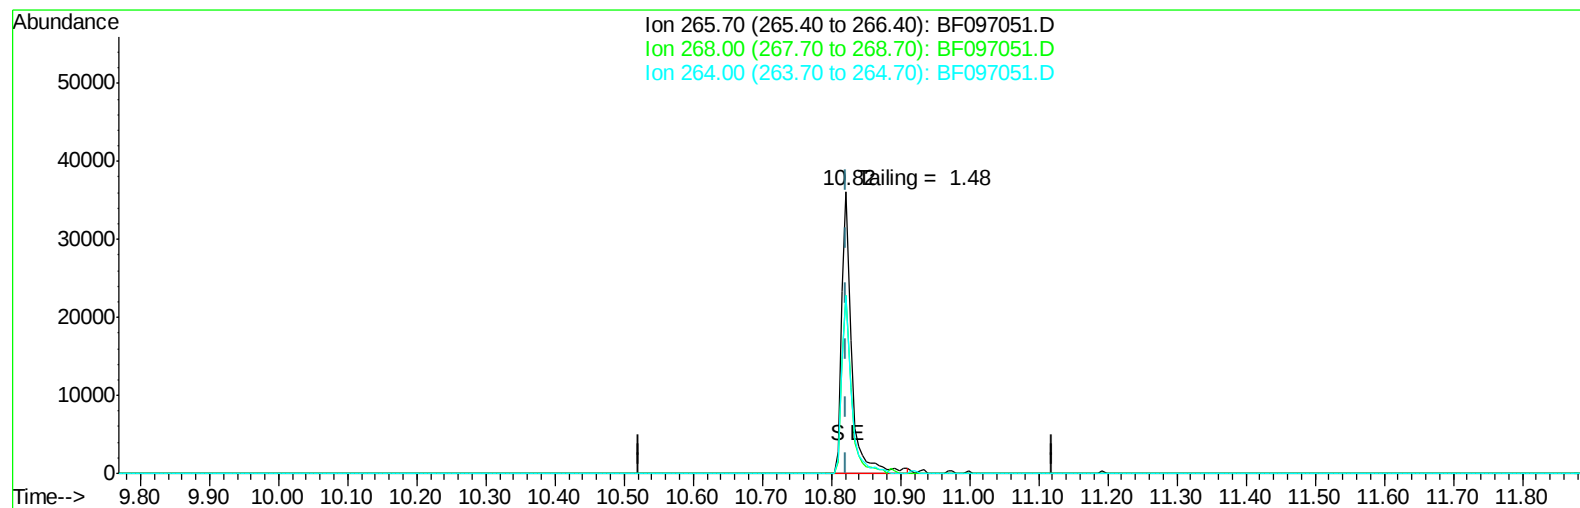

TIC: BF097051.D

(69) Pentachlorophenol (C)

10.822min (+0.001) 0.00ng

response 34377

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.00
264.00	64.60	63.02
0.00	0.00	0.00