


Instrument :
BNA_F
ClientSampleId :

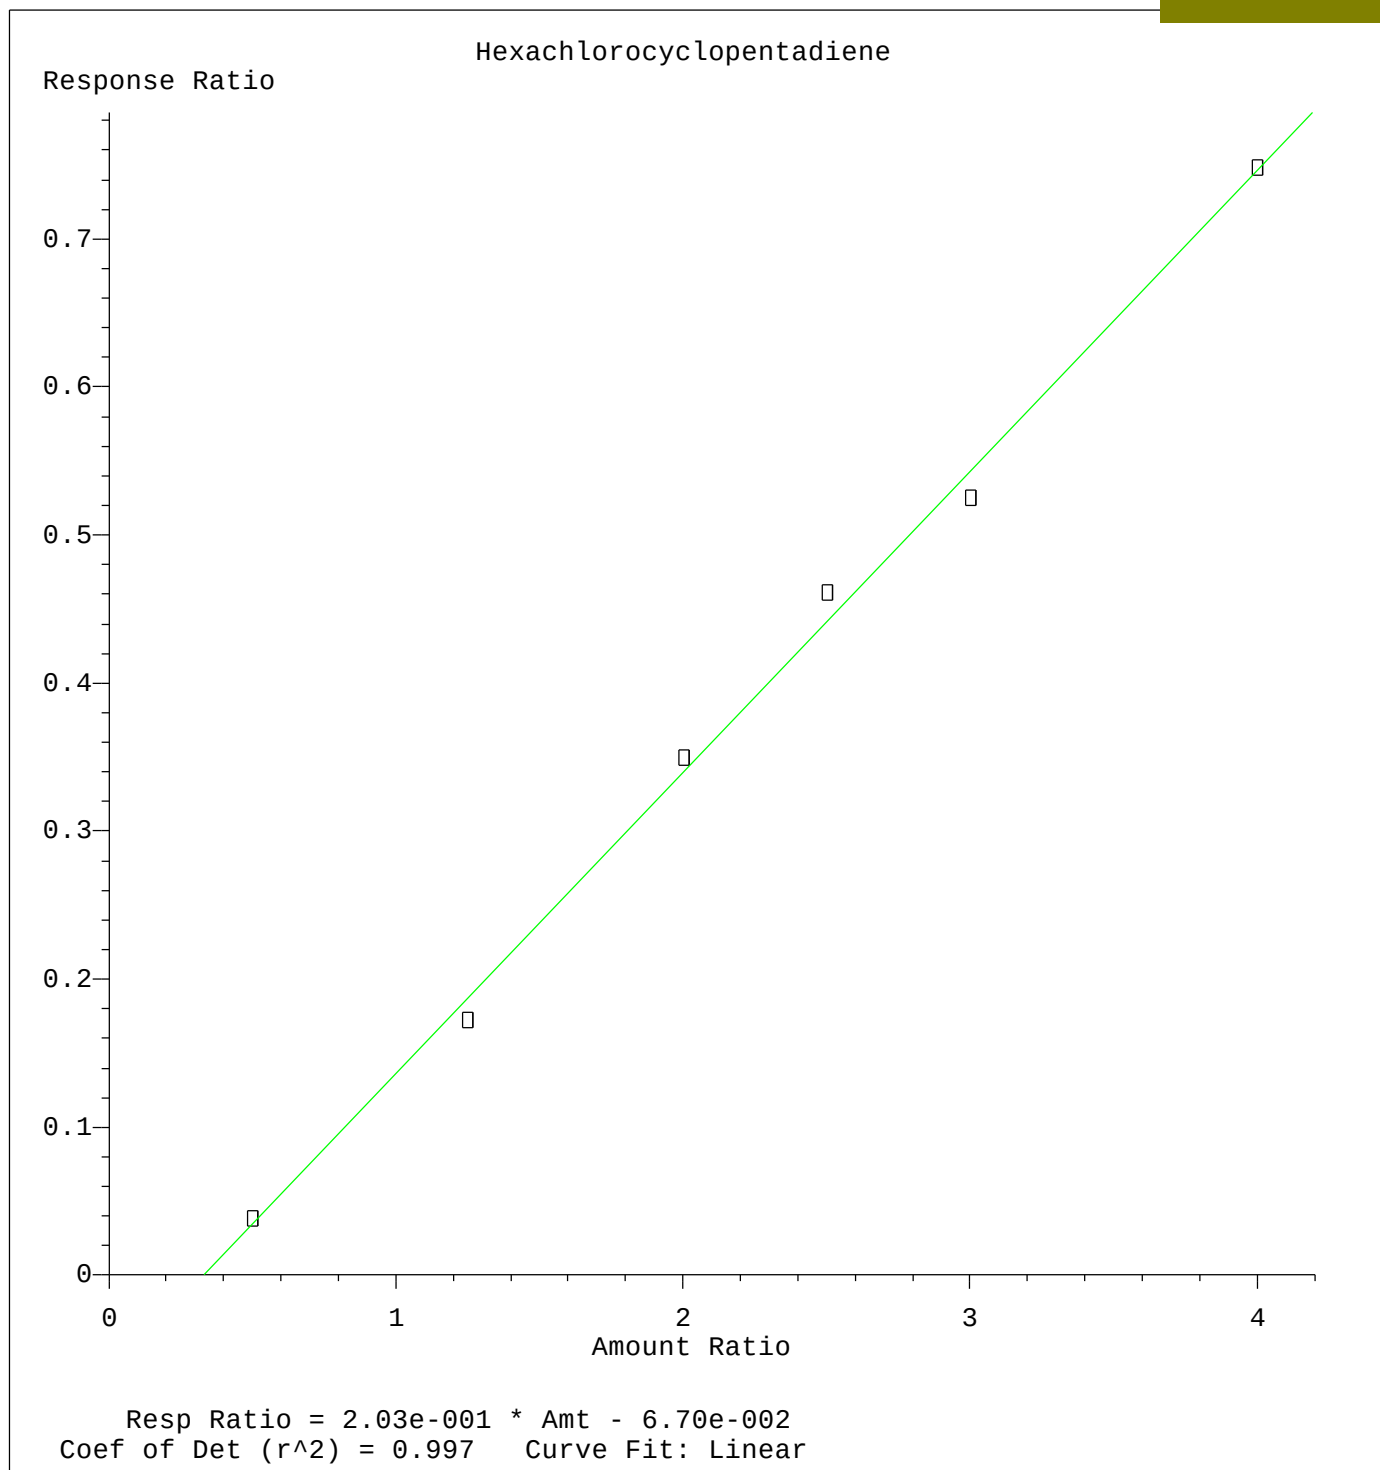

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Calibration Table Last Updated: Tue Jul 25 14:11:51 2017