

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072517\
 Data File : BF097055.D
 Acq On : 26 Jul 2017 4:16
 Operator : SJ/JU
 Sample : I4305-02 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-N5-WSW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.069	367	371	374	rBV	12845	16179	1.43%	0.110%
2	4.634	463	467	473	rBV	59451	73410	6.47%	0.498%
3	5.098	542	546	562	rBV	621728	695989	61.32%	4.723%
4	6.157	722	726	737	rBV	802809	765324	67.43%	5.194%
5	6.269	742	745	753	rBV	866870	739412	65.15%	5.018%
6	6.498	780	784	793	rBV	1047755	949475	83.66%	6.443%
7	6.651	807	810	811	rBV	622073	534045	47.05%	3.624%
8	6.669	811	813	823	rVB	845340	697153	61.42%	4.731%
9	7.063	876	880	886	rBV	501817	422858	37.26%	2.870%
10	7.122	888	890	893	rVB	19279	14933	1.32%	0.101%
11	7.781	998	1002	1010	rBV	1391962	1134976	100.00%	7.702%
12	8.057	1046	1049	1057	rBV	68429	67478	5.95%	0.458%
13	8.228	1072	1078	1082	rVB	22446	20581	1.81%	0.140%
14	8.398	1102	1107	1109	rBV	22268	19778	1.74%	0.134%
15	8.857	1181	1185	1188	rBV	871556	698009	61.50%	4.737%
16	8.957	1195	1202	1207	rVB2	31556	41821	3.68%	0.284%
17	9.028	1210	1214	1218	rVV	23657	21855	1.93%	0.148%
18	9.257	1251	1253	1255	rBV	49899	36326	3.20%	0.247%
19	9.463	1281	1288	1289	rBV4	10360	21507	1.89%	0.146%
20	9.486	1289	1292	1294	rVV	32563	29854	2.63%	0.203%
21	9.528	1294	1299	1303	rVV	1161842	1005547	88.60%	6.824%
22	9.581	1305	1308	1313	rVB4	9294	15155	1.34%	0.103%
23	9.957	1369	1372	1374	rBV	87561	68122	6.00%	0.462%
24	9.980	1374	1376	1380	rVB	38319	29854	2.63%	0.203%
25	10.310	1429	1432	1438	rBV	321897	280862	24.75%	1.906%
26	10.451	1452	1456	1466	rBV	47693	56442	4.97%	0.383%
27	10.898	1530	1532	1535	rVB	36308	26432	2.33%	0.179%
28	10.998	1545	1549	1552	rBV	871691	760720	67.03%	5.163%
29	11.022	1552	1553	1557	rVB	39506	26092	2.30%	0.177%
30	11.322	1602	1604	1609	rVB2	21445	23715	2.09%	0.161%
31	11.557	1641	1644	1646	rBV	19252	16688	1.47%	0.113%
32	11.727	1669	1673	1681	rBV	85907	96118	8.47%	0.652%
33	12.116	1735	1739	1741	rBV2	26861	26227	2.31%	0.178%
34	12.204	1751	1754	1757	rBV	60049	53095	4.68%	0.360%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072517\
Data File : BF097055.D
Acq On : 26 Jul 2017 4:16
Operator : SJ/JU
Sample : I4305-02 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-N5-WSW

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.257	1758	1763	1768	rVV6	22645	42757	3.77%	0.290%
36	12.345	1773	1778	1781	rBV4	23406	33328	2.94%	0.226%
37	12.427	1788	1792	1796	rBV	951752	814089	71.73%	5.525%
38	12.486	1798	1802	1803	rVV	56887	55177	4.86%	0.374%
39	12.504	1803	1805	1809	rVB	206763	166257	14.65%	1.128%
40	12.580	1814	1818	1823	rBV	588572	478953	42.20%	3.250%
41	12.663	1825	1832	1835	rBV7	16879	37481	3.30%	0.254%
42	12.839	1859	1862	1864	rBV	51382	41940	3.70%	0.285%
43	12.863	1864	1866	1870	rVB4	12966	13807	1.22%	0.094%
44	13.133	1908	1912	1915	rBV	720371	633737	55.84%	4.301%
45	13.180	1915	1920	1922	rVV2	123834	166609	14.68%	1.131%
46	13.198	1922	1923	1928	rVB	96217	80945	7.13%	0.549%
47	13.292	1937	1939	1942	rBV4	24676	25153	2.22%	0.171%
48	13.339	1944	1947	1951	rVV	45171	54214	4.78%	0.368%
49	13.392	1954	1956	1959	rVB	35781	32377	2.85%	0.220%
50	13.474	1968	1970	1971	rBV2	20938	17823	1.57%	0.121%
51	13.504	1971	1975	1979	rVB	141694	152626	13.45%	1.036%
52	13.621	1991	1995	1998	rBV	745233	767856	67.65%	5.211%
53	13.645	1998	1999	2002	rVB	41614	30639	2.70%	0.208%
54	13.821	2025	2029	2033	rBV	172119	173008	15.24%	1.174%
55	14.127	2077	2081	2084	rBV	123838	124615	10.98%	0.846%
56	14.415	2127	2130	2133	rVB	157569	147094	12.96%	0.998%
57	14.710	2176	2180	2183	rBV	111639	113980	10.04%	0.774%
58	14.921	2214	2216	2219	rVB	21205	14487	1.28%	0.098%
59	14.974	2221	2225	2229	rBV	514099	575511	50.71%	3.906%
60	15.027	2230	2234	2242	rVB	120278	159711	14.07%	1.084%
61	15.386	2291	2295	2300	rBV	78687	109381	9.64%	0.742%
62	15.798	2362	2365	2370	rVB2	51196	82214	7.24%	0.558%
63	16.286	2445	2448	2452	rVB3	31635	40376	3.56%	0.274%
64	16.674	2510	2514	2521	rVB10	31890	63251	5.57%	0.429%


Sum of corrected areas: 14735428

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072517\
Data File : BF097055.D
Acq On : 26 Jul 2017 4:16
Operator : SJ/JU
Sample : I4305-02 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-N5-WSW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

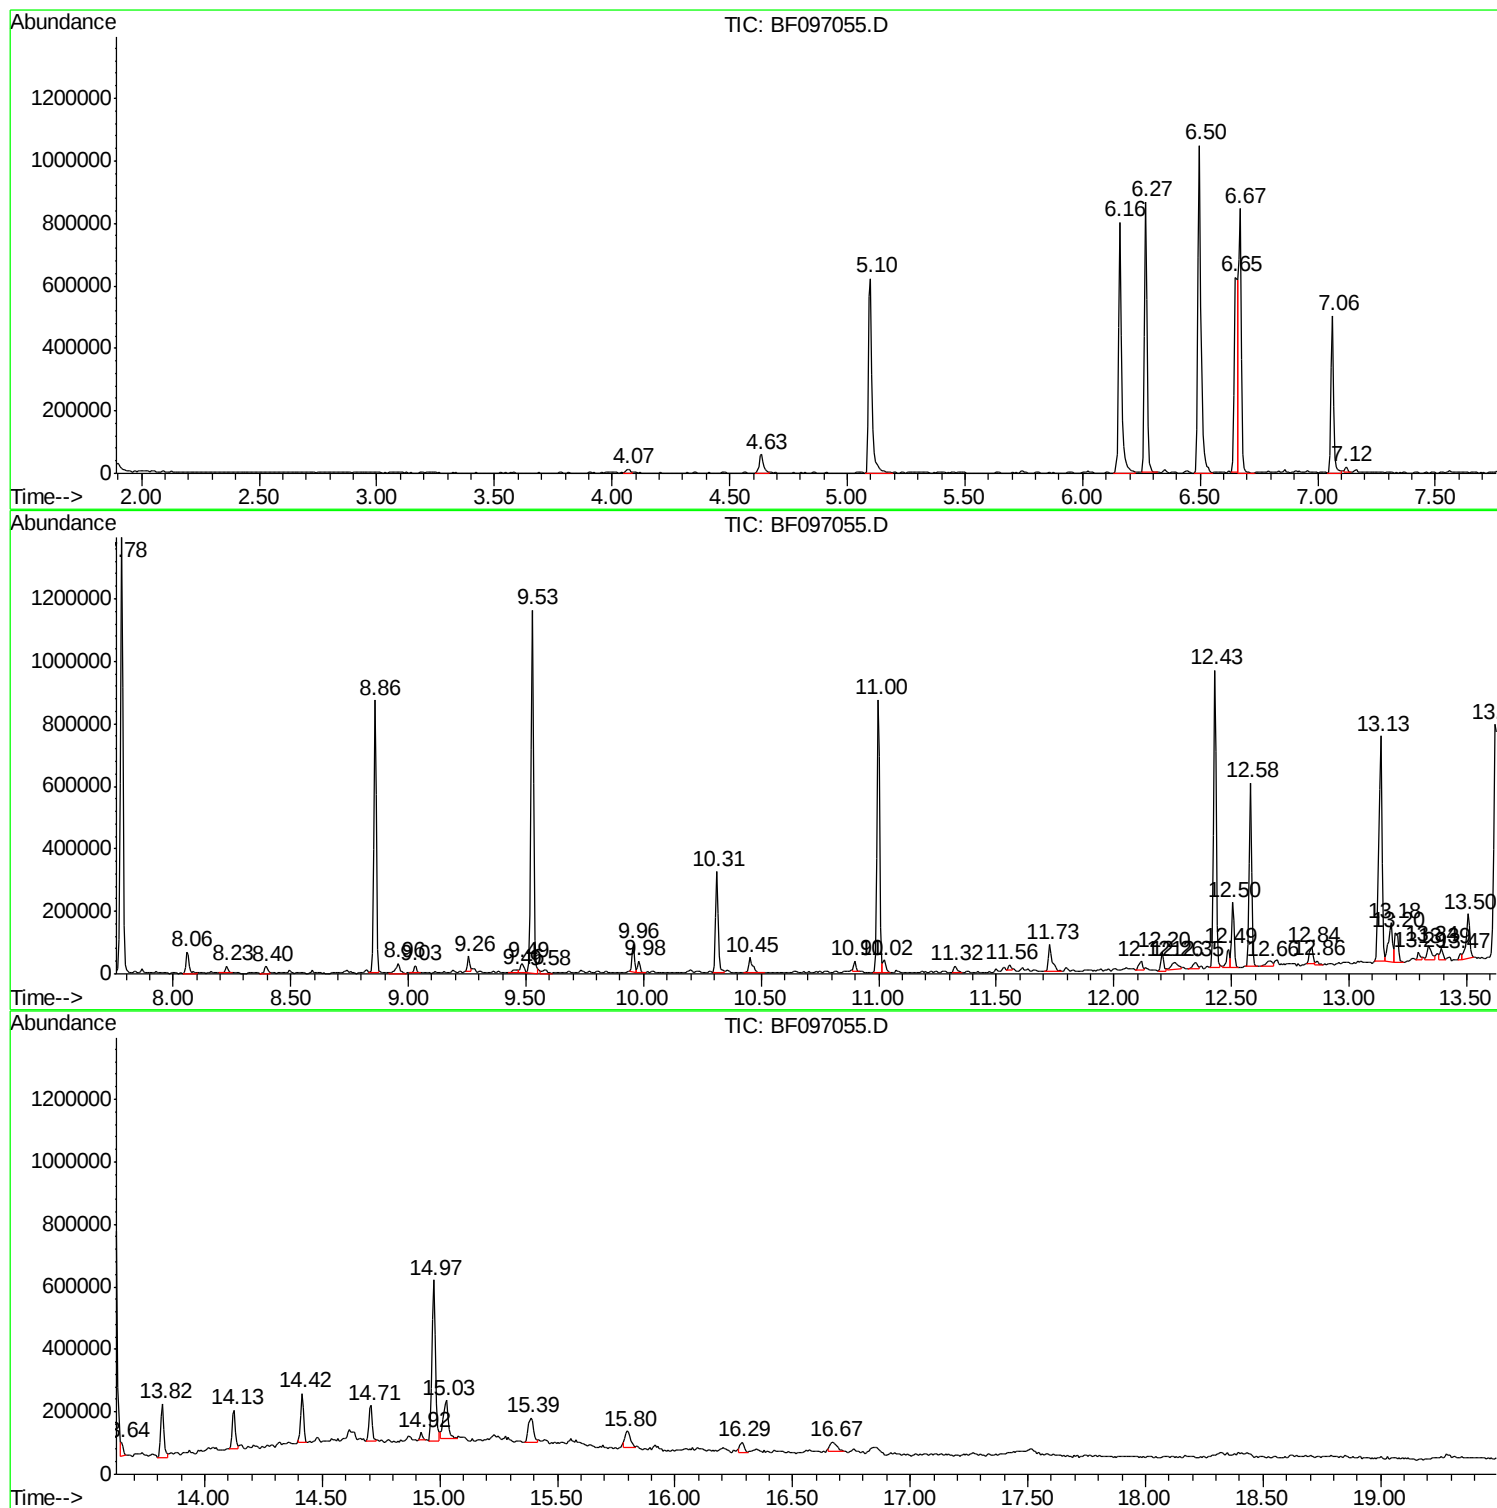

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF072517\
Data_File : BF097055.D
Acq_On : 26 Jul 2017 4:166
Operator : SJ/JUU
Sample : I4305-02_5XX
Misc :
ALS_Vial : 29 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-N5-WSW

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
