


Data Path : Z:\HPCHEM1\BNA F\Data\BF072517\
 Data File : BF097025.D
 Acq On : 25 Jul 2017 13:28
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 25 14:11:51 2017

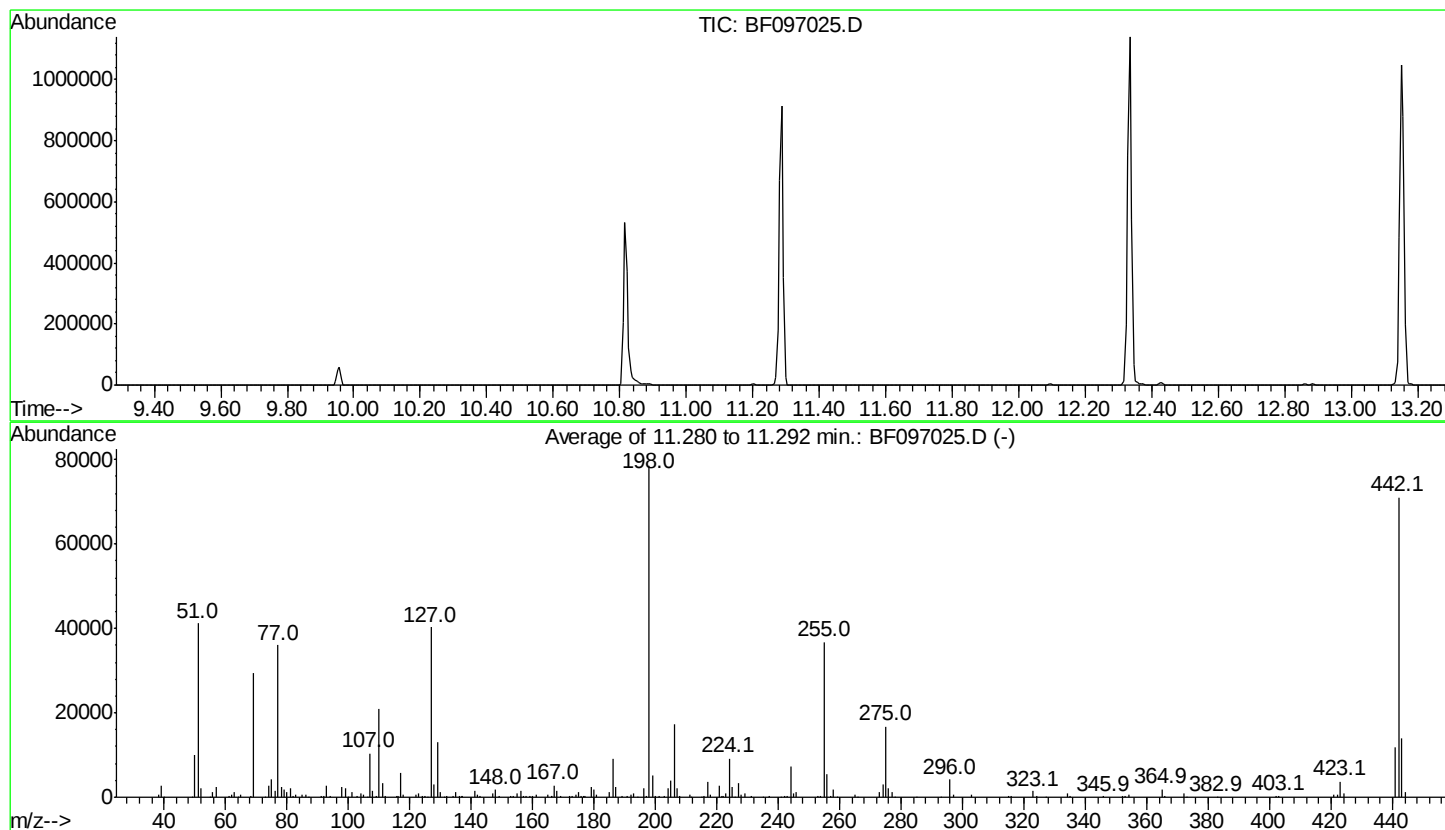

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	41207	PASS
68	69	0.00	2	1.2	341	PASS
69	198	0.00	100	37.4	29409	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	40256	PASS
197	198	0.00	2	0.5	384	PASS
198	198	100	100	100.0	78586	PASS
199	198	5	9	6.5	5141	PASS
275	198	10	60	21.4	16795	PASS
365	198	1	100	2.5	1960	PASS
441	442	0.01	24	16.4	11693	PASS
442	198	50	100	90.5	71125	PASS
443	442	15	24	19.8	14048	PASS