
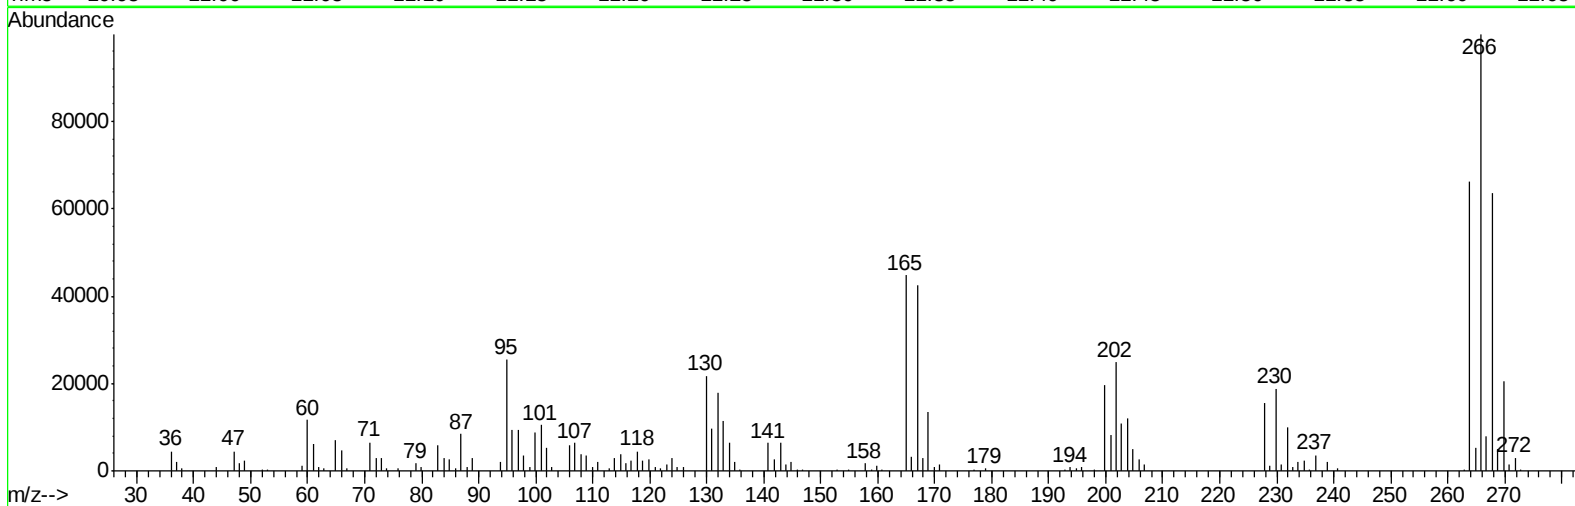


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072519\
Data File : BF115752.D
Acq On : 25 Jul 2019 11:07
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 09:03:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 13:16:07 2019
Response via : Initial Calibration

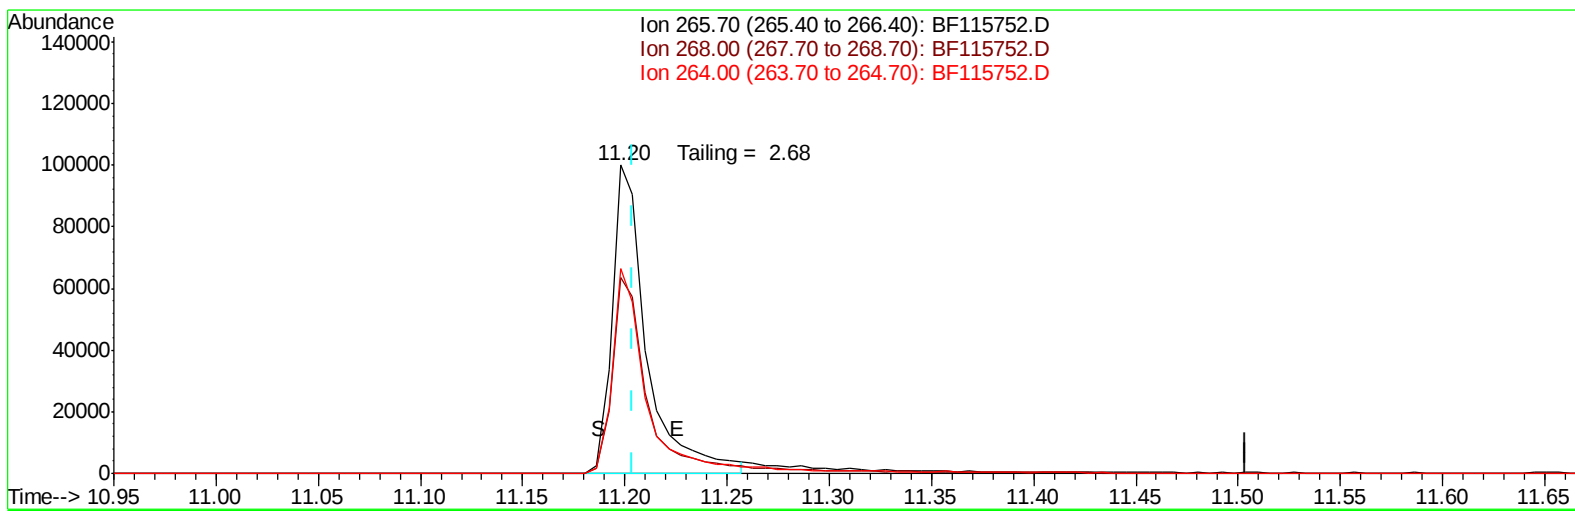

TIC: BF115752.D

(70) Pentachlorophenol (C)



11.198min (-0.006) 26900.60ng

response 126254

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.72
264.00	62.50	66.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072519\
Data File : BF115752.D
Acq On : 25 Jul 2019 11:07
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 09:03:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 13:16:07 2019
Response via : Initial Calibration

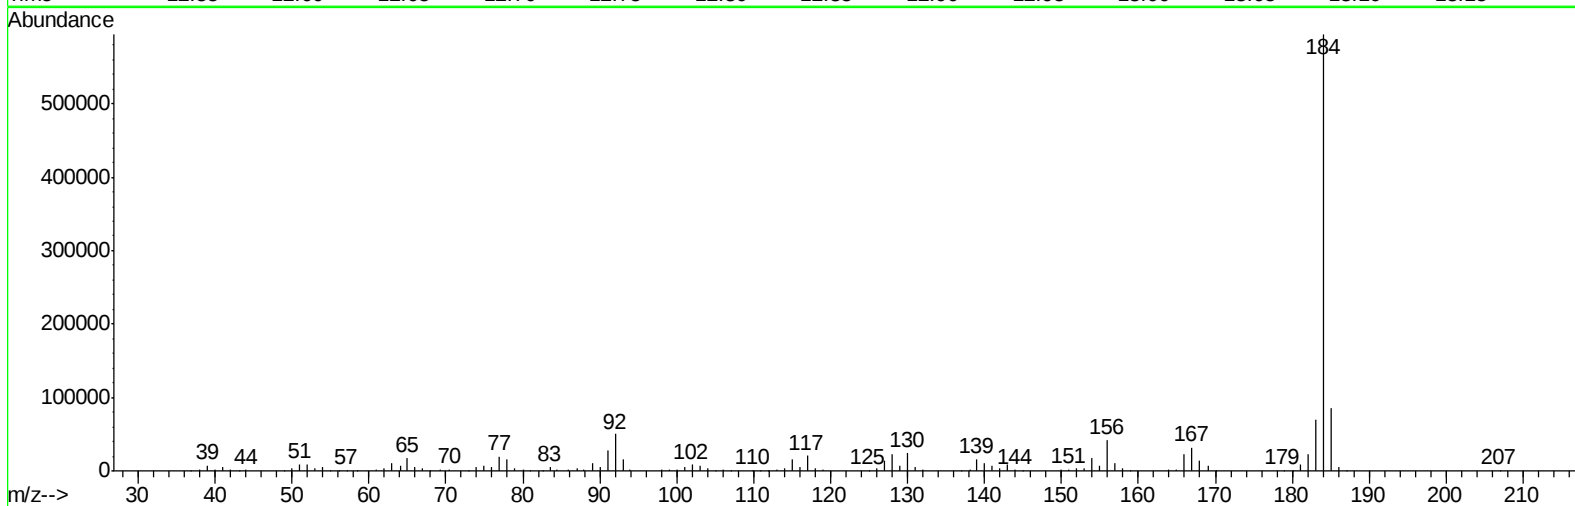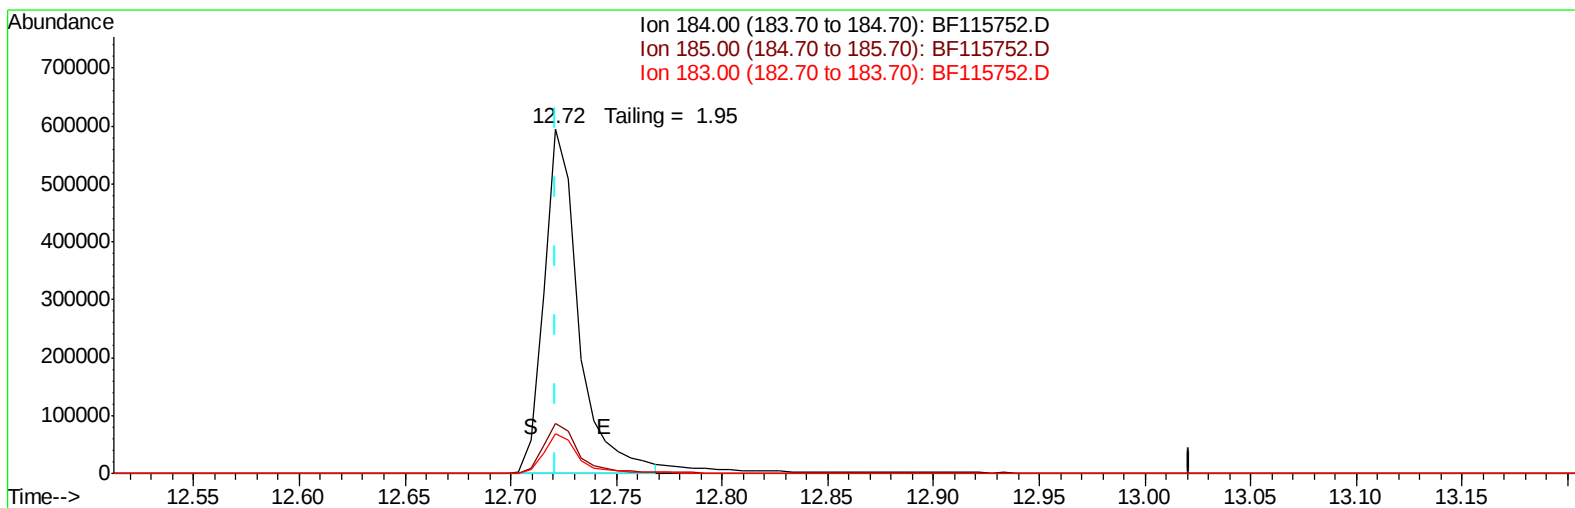

TIC: BF115752.D

(77) Benzidine

12.721min (-0.000) 0.00ng

response 710469

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.50
183.00	11.50	11.69
0.00	0.00	0.00