
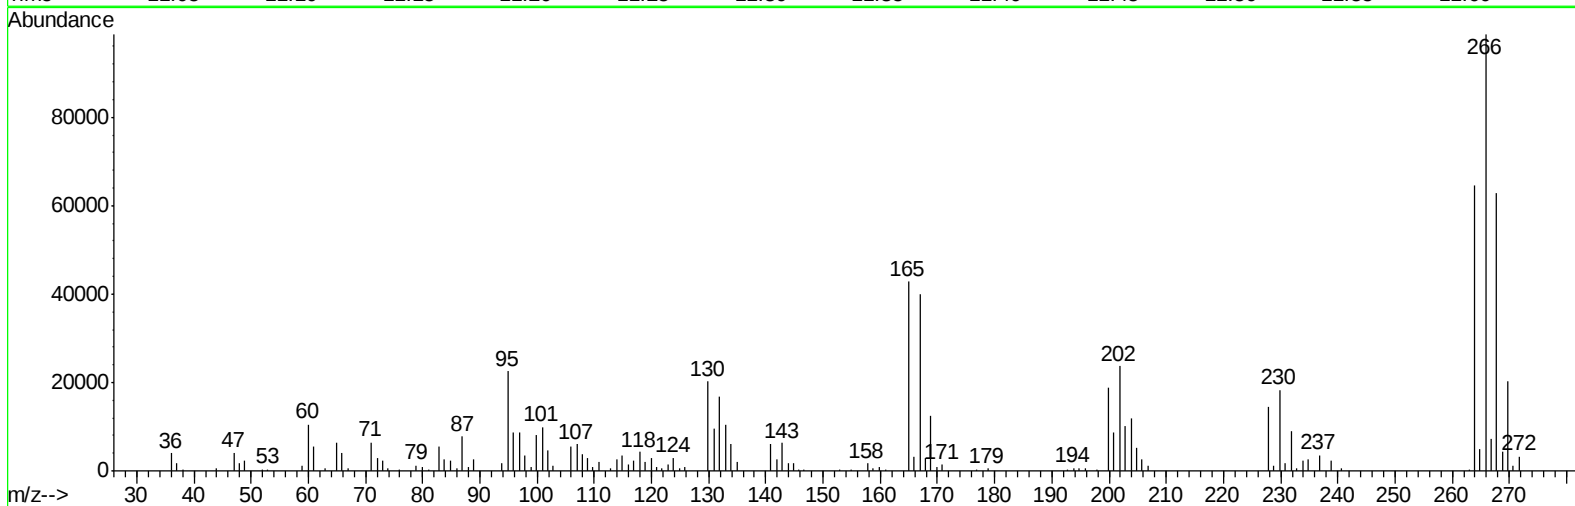


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072519\  
Data File : BF115758.D  
Acq On : 25 Jul 2019 14:55  
Operator : HP/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 09:11:32 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 25 13:16:07 2019  
Response via : Initial Calibration

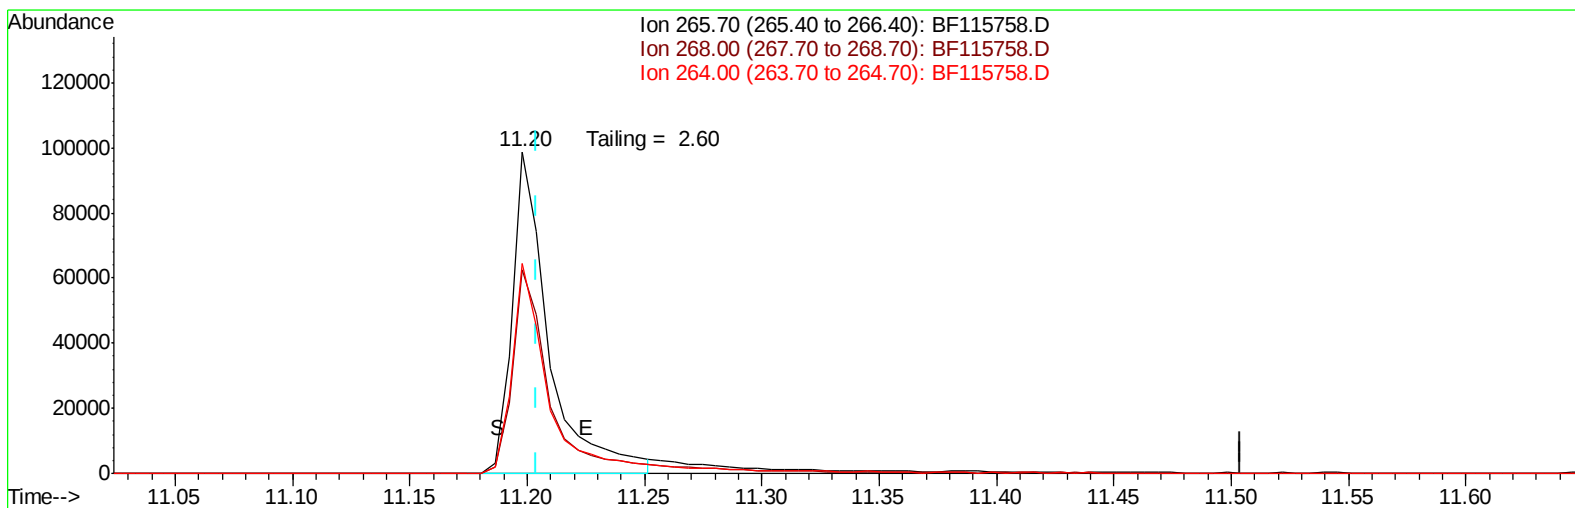

TIC: BF115758.D

(70) Pentachlorophenol (C)



11.198min (-0.006) 138455.91ng

response 118250

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.00 | 63.54 |
| 264.00 | 62.50 | 65.28 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072519\  
Data File : BF115758.D  
Acq On : 25 Jul 2019 14:55  
Operator : HP/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 09:11:32 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 25 13:16:07 2019  
Response via : Initial Calibration

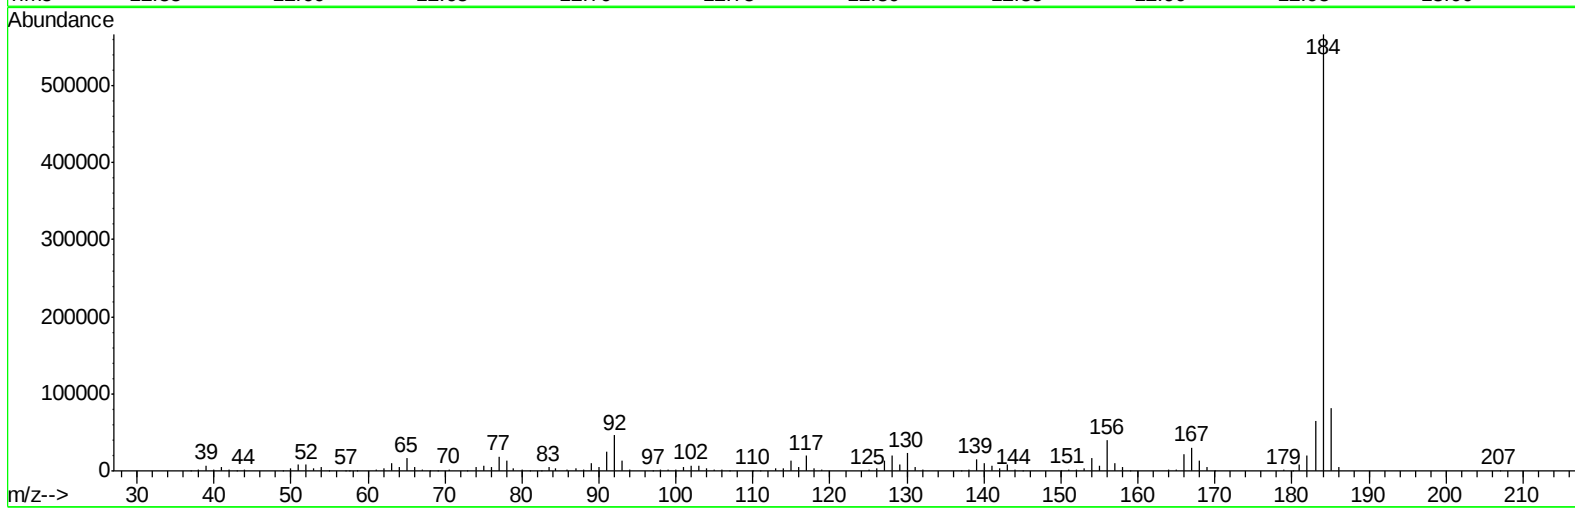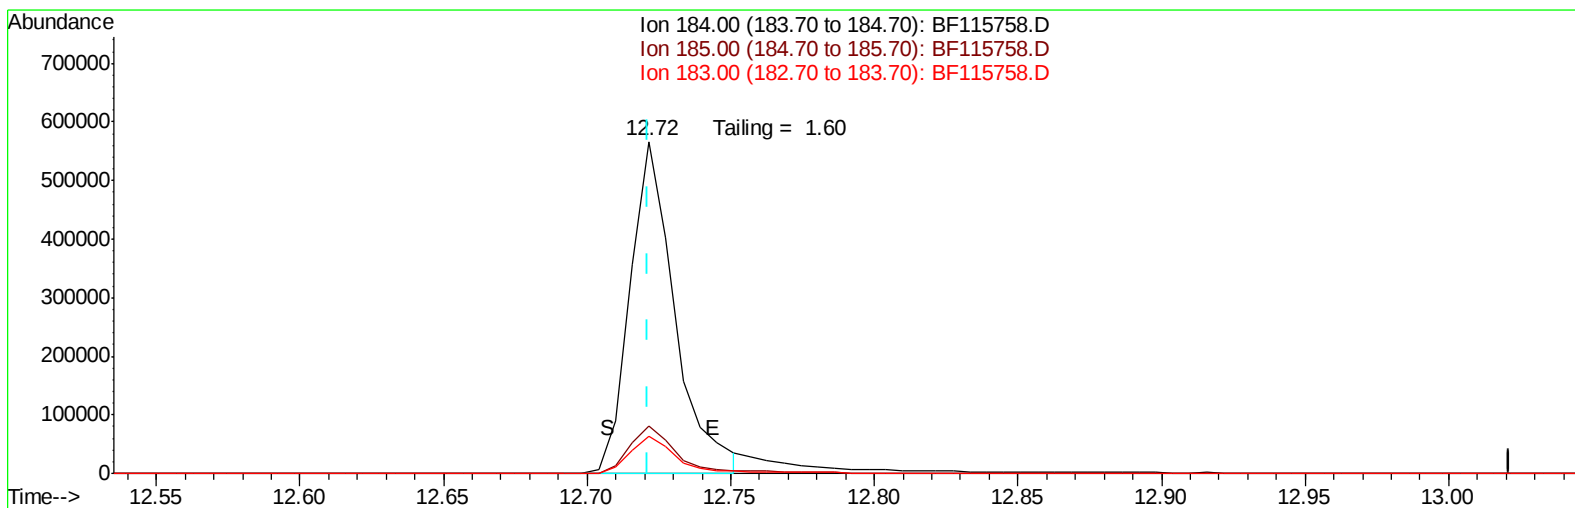

TIC: BF115758.D

(77) Benzidine

12.722min (+0.000) 0.00ng

response 670616

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.60 | 14.38 |
| 183.00 | 11.50 | 11.36 |
| 0.00   | 0.00  | 0.00  |