


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072519\
 Data File : BF115752.D
 Acq On : 25 Jul 2019 11:07
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 25 13:16:07 2019

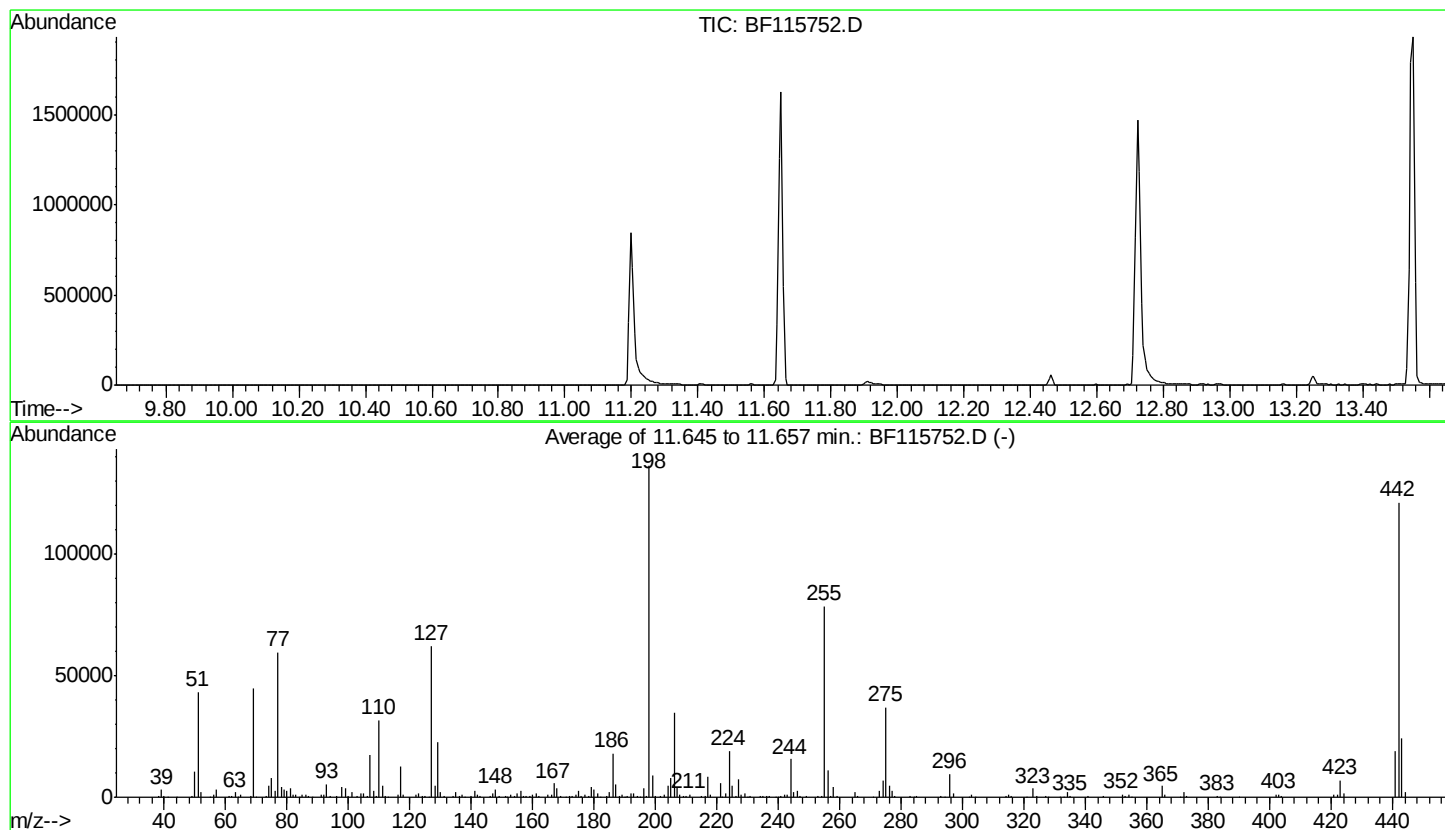

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	43282	PASS
68	69	0.00	2	1.5	662	PASS
69	198	0.00	100	32.7	44551	PASS
70	69	0.00	2	0.5	213	PASS
127	198	10	80	45.6	62120	PASS
197	198	0.00	2	0.6	771	PASS
198	198	100	100	100.0	136106	PASS
199	198	5	9	6.7	9187	PASS
275	198	10	60	27.2	37040	PASS
365	198	1	100	3.4	4688	PASS
441	198	0.01	100	14.1	19134	PASS
442	198	50	100	88.9	121008	PASS
443	442	15	24	19.8	23963	PASS