


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072519\
 Data File : BF115758.D
 Acq On : 25 Jul 2019 14:55
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 25 13:16:07 2019

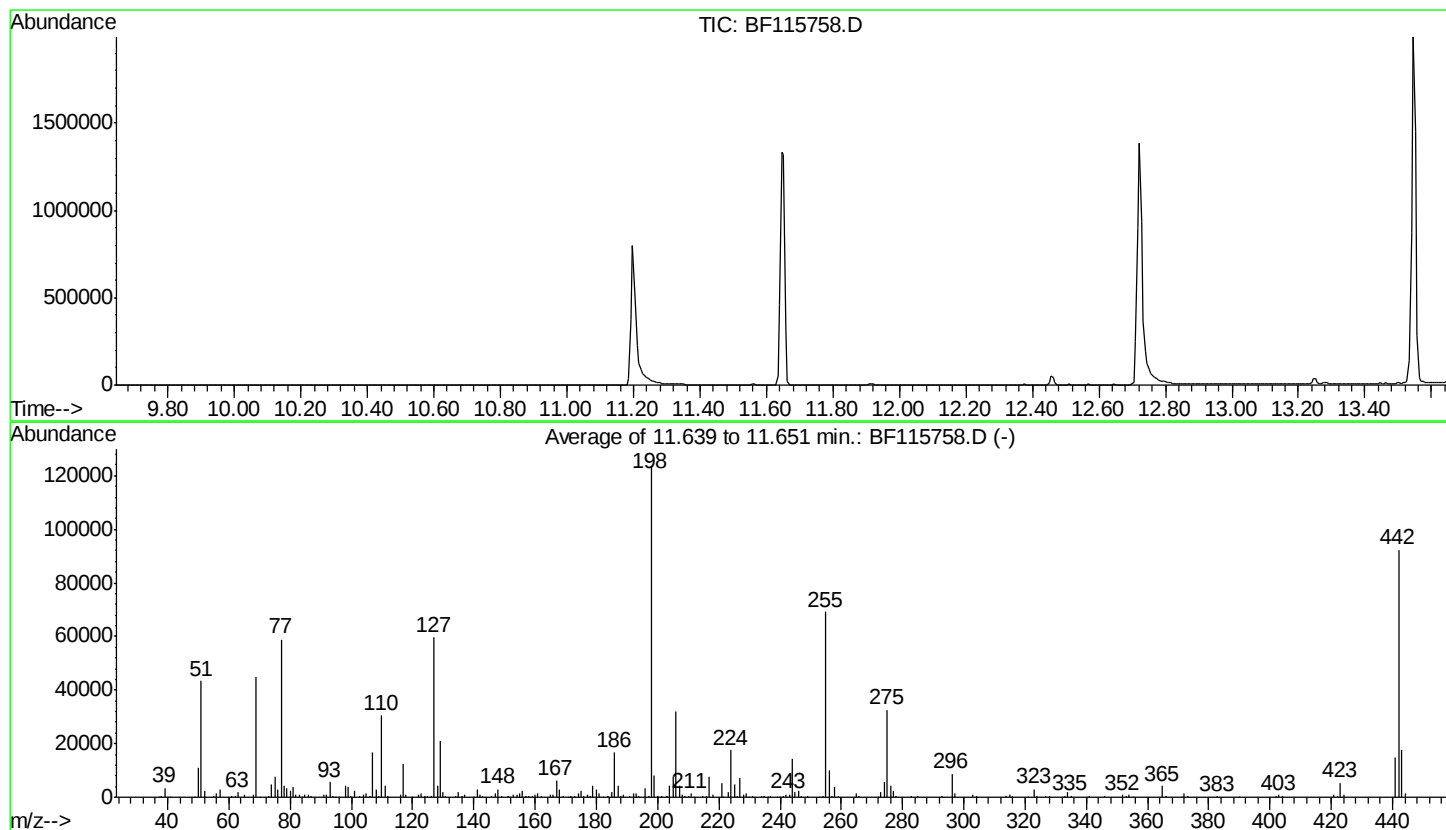

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	43418	PASS
68	69	0.00	2	1.7	775	PASS
69	198	0.00	100	36.3	44952	PASS
70	69	0.00	2	0.4	169	PASS
127	198	10	80	48.1	59496	PASS
197	198	0.00	2	0.6	718	PASS
198	198	100	100	100.0	123744	PASS
199	198	5	9	6.7	8264	PASS
275	198	10	60	26.3	32563	PASS
365	198	1	100	3.3	4132	PASS
441	198	0.01	100	11.9	14669	PASS
442	198	50	100	74.7	92386	PASS
443	442	15	24	18.9	17503	PASS