

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072522\  
 Data File : BF129339.D  
 Acq On : 25 Jul 2022 18:57  
 Operator : CG\JU  
 Sample : PB146423BL  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB146423BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129339.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.146       | 483           | 486         | 499          | rVB      | 75432          | 109818        | 1.17%           | 0.182%        |
| 2         | 5.510       | 543           | 548         | 551          | rBV      | 6545053        | 7636068       | 81.50%          | 12.655%       |
| 3         | 6.516       | 712           | 719         | 721          | rBV      | 6215326        | 7647503       | 81.62%          | 12.674%       |
| 4         | 6.881       | 777           | 781         | 785          | rBV      | 2152228        | 1744272       | 18.62%          | 2.891%        |
| 5         | 7.445       | 872           | 877         | 880          | rBV      | 4530986        | 5284723       | 56.40%          | 8.758%        |
| 6         | 8.163       | 994           | 999         | 1003         | rBV      | 2580042        | 2385443       | 25.46%          | 3.953%        |
| 7         | 9.245       | 1176          | 1183        | 1186         | rBV      | 8632915        | 9203213       | 98.23%          | 15.252%       |
| 8         | 9.922       | 1292          | 1298        | 1302         | rBV      | 3159791        | 2732706       | 29.17%          | 4.529%        |
| 9         | 10.716      | 1426          | 1433        | 1436         | rBV      | 5718205        | 5886018       | 62.82%          | 9.755%        |
| 10        | 11.416      | 1547          | 1552        | 1555         | rBV      | 3088077        | 2775990       | 29.63%          | 4.601%        |
| 11        | 13.004      | 1817          | 1822        | 1825         | rBV      | 8583616        | 9369424       | 100.00%         | 15.528%       |
| 12        | 14.057      | 1997          | 2001        | 2005         | rBV      | 2723917        | 2348991       | 25.07%          | 3.893%        |
| 13        | 14.821      | 2127          | 2131        | 2136         | rBV      | 111984         | 103987        | 1.11%           | 0.172%        |
| 14        | 15.168      | 2186          | 2190        | 2197         | rVB      | 135493         | 158900        | 1.70%           | 0.263%        |
| 15        | 15.551      | 2248          | 2255        | 2270         | rBV      | 1743708        | 2266327       | 24.19%          | 3.756%        |
| 16        | 15.998      | 2326          | 2331        | 2338         | rBV      | 152728         | 218819        | 2.34%           | 0.363%        |
| 17        | 16.515      | 2414          | 2419        | 2428         | rVB      | 116926         | 211021        | 2.25%           | 0.350%        |
| 18        | 17.127      | 2517          | 2523        | 2532         | rVB2     | 64713          | 139173        | 1.49%           | 0.231%        |
| 19        | 17.845      | 2638          | 2645        | 2655         | rBV2     | 44721          | 118433        | 1.26%           | 0.196%        |




Sum of corrected areas: 60340829

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072522\  
Data File : BF129339.D  
Acq On : 25 Jul 2022 18:57  
Operator : CG\JU  
Sample : PB146423BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB146423BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

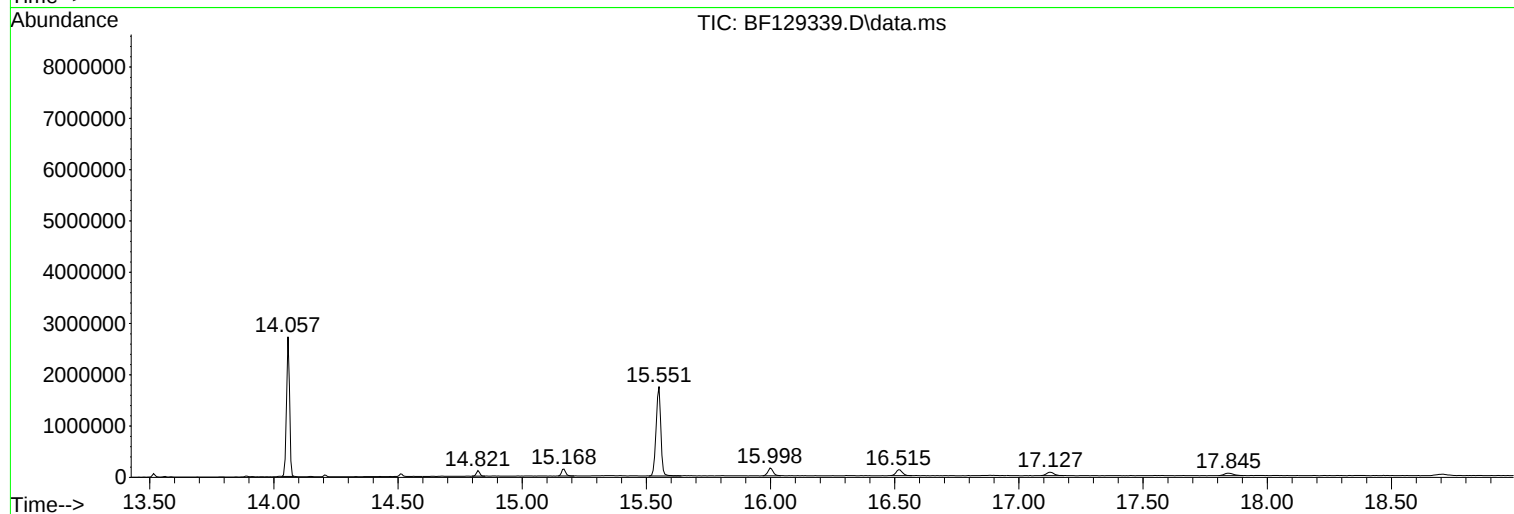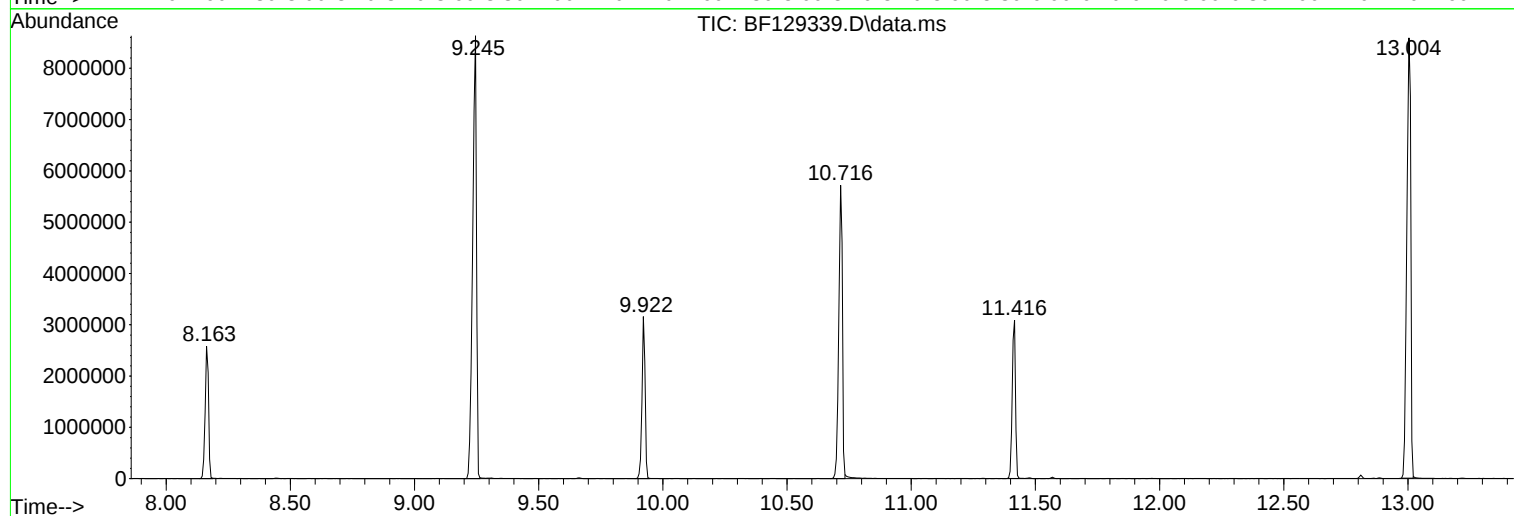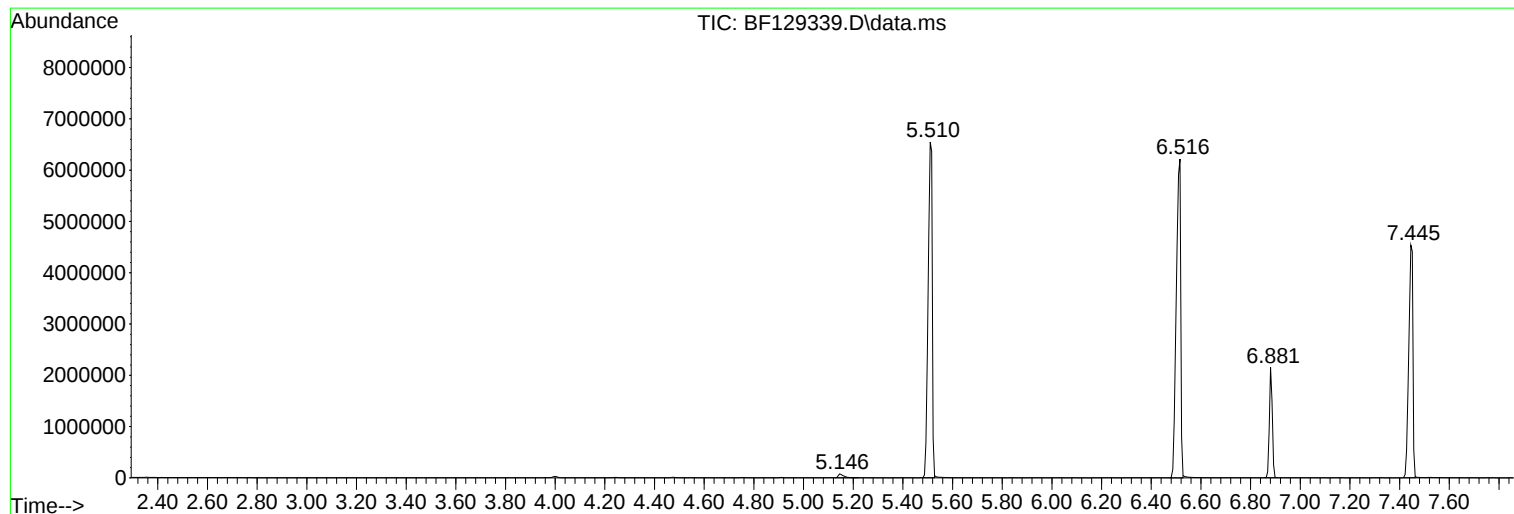

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072522\  
Data File : BF129339.D  
Acq On : 25 Jul 2022 18:57  
Operator : CG\JU  
Sample : PB146423BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB146423BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072522\  
Data File : BF129339.D  
Acq On : 25 Jul 2022 18:57  
Operator : CG\JU  
Sample : PB146423BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB146423BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|