


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072522\
 Data File : BF129328.D
 Acq On : 25 Jul 2022 09:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 25 17:24:17 2022

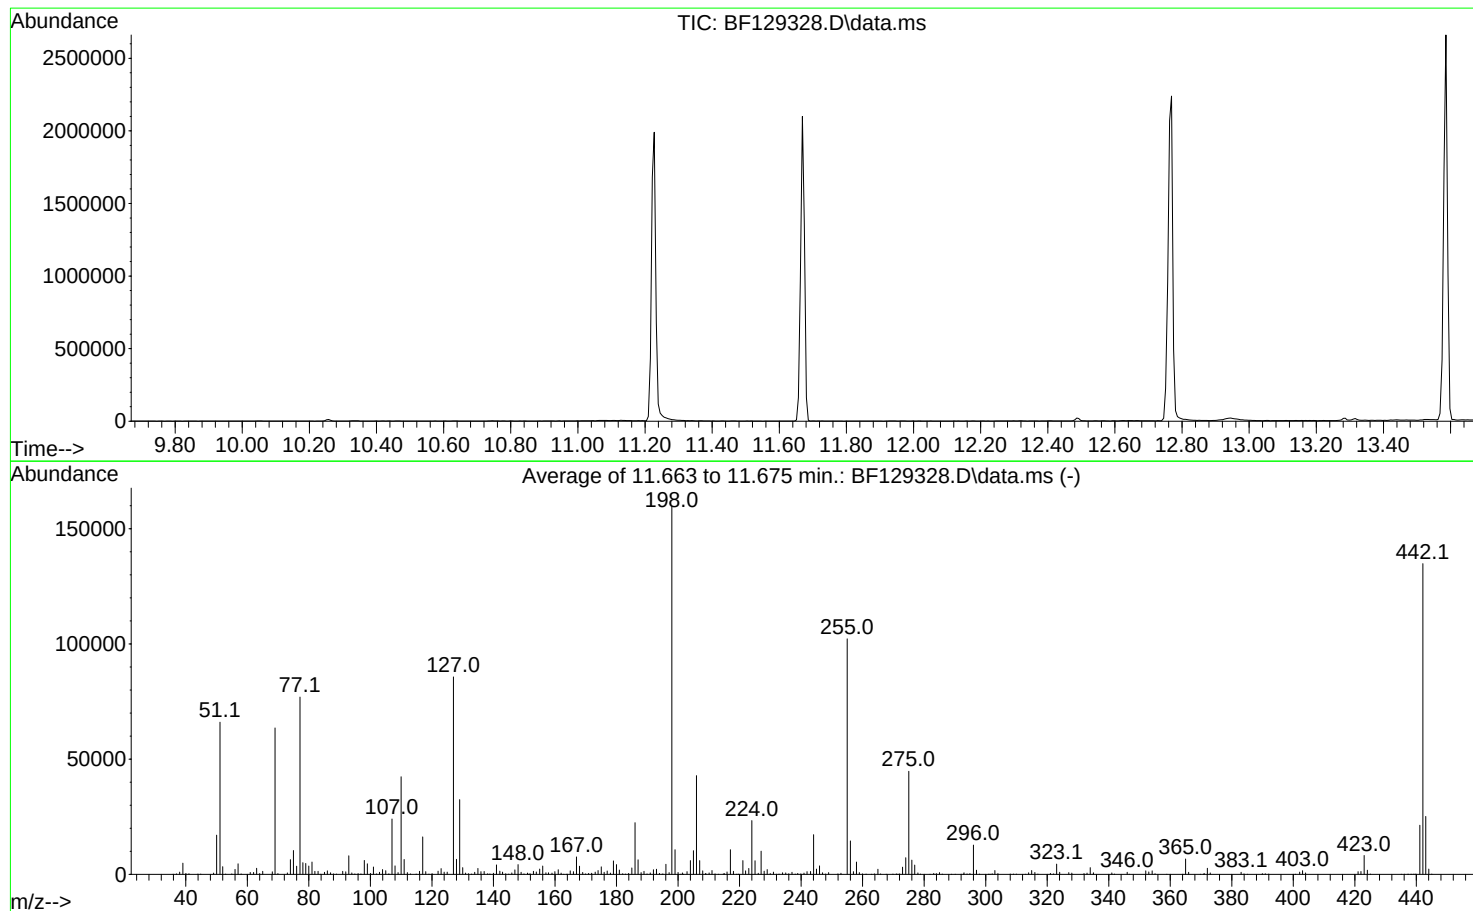


AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	66088	PASS
68	69	0.00	2	1.7	1099	PASS
69	198	0.00	100	39.8	63571	PASS
70	69	0.00	2	0.5	342	PASS
127	198	10	80	53.7	85749	PASS
197	198	0.00	2	0.5	794	PASS
198	198	100	100	100.0	159691	PASS
199	198	5	9	6.7	10672	PASS
275	198	10	60	28.0	44760	PASS
365	198	1	100	4.2	6707	PASS
441	198	0.01	100	13.4	21360	PASS
442	442	50	100	100.0	134883	PASS
443	442	15	24	18.6	25129	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072522\
Data File : BF129328.D
Acq On : 25 Jul 2022 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 16:04:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 16:00:06 2022
Response via : Initial Calibration

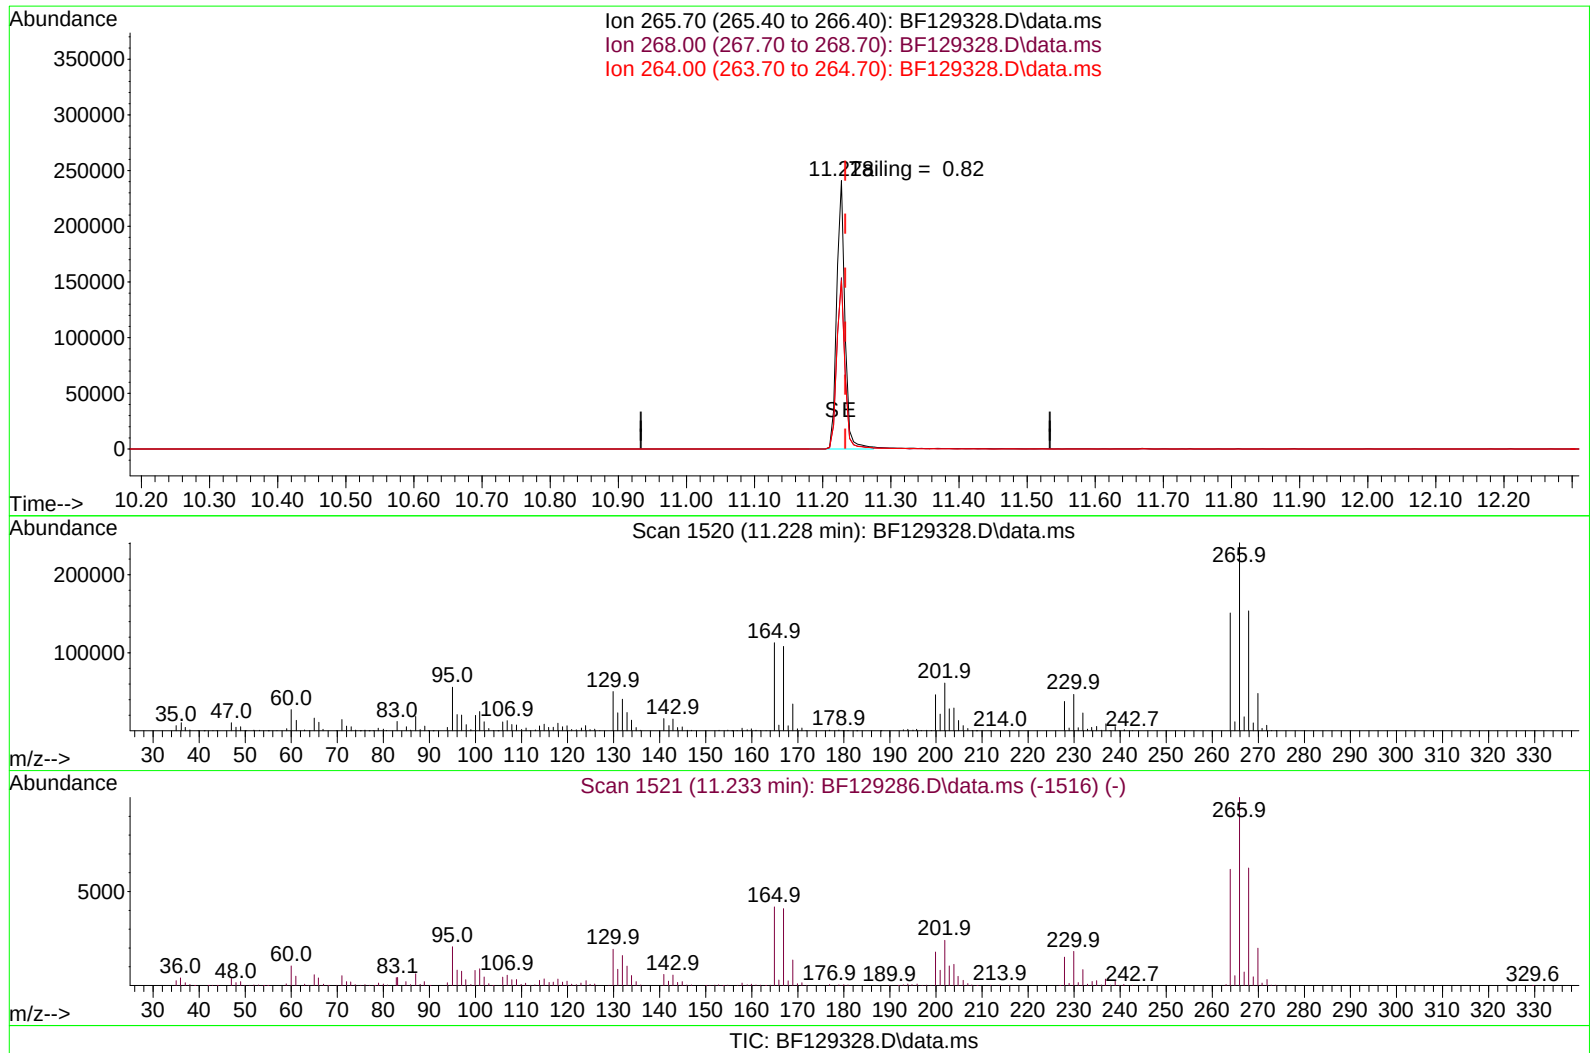

(70) Pentachlorophenol (C)

11.228min (-0.006) 556695.82 ng




response 206160

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.77
264.00	61.80	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072522\
Data File : BF129328.D
Acq On : 25 Jul 2022 09:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 16:04:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 16:00:06 2022
Response via : Initial Calibration

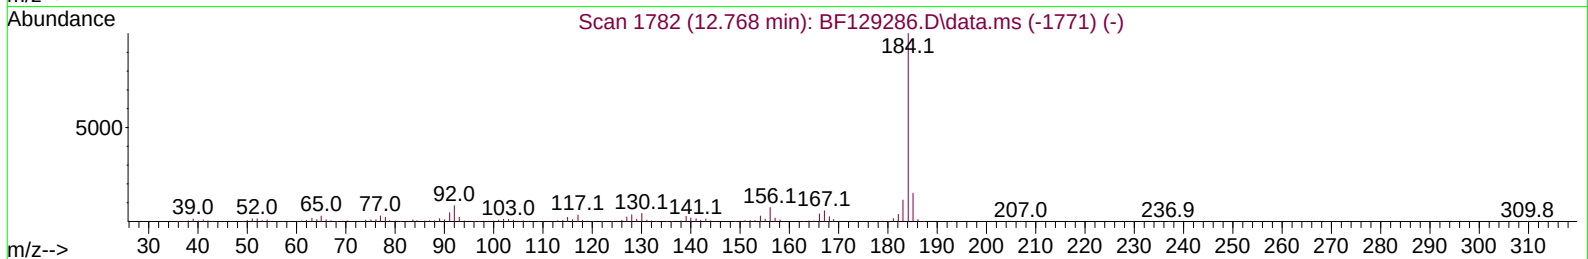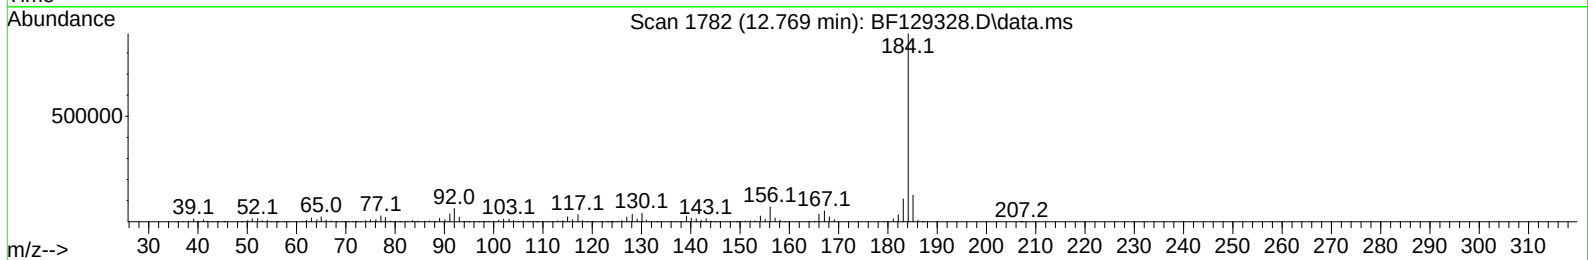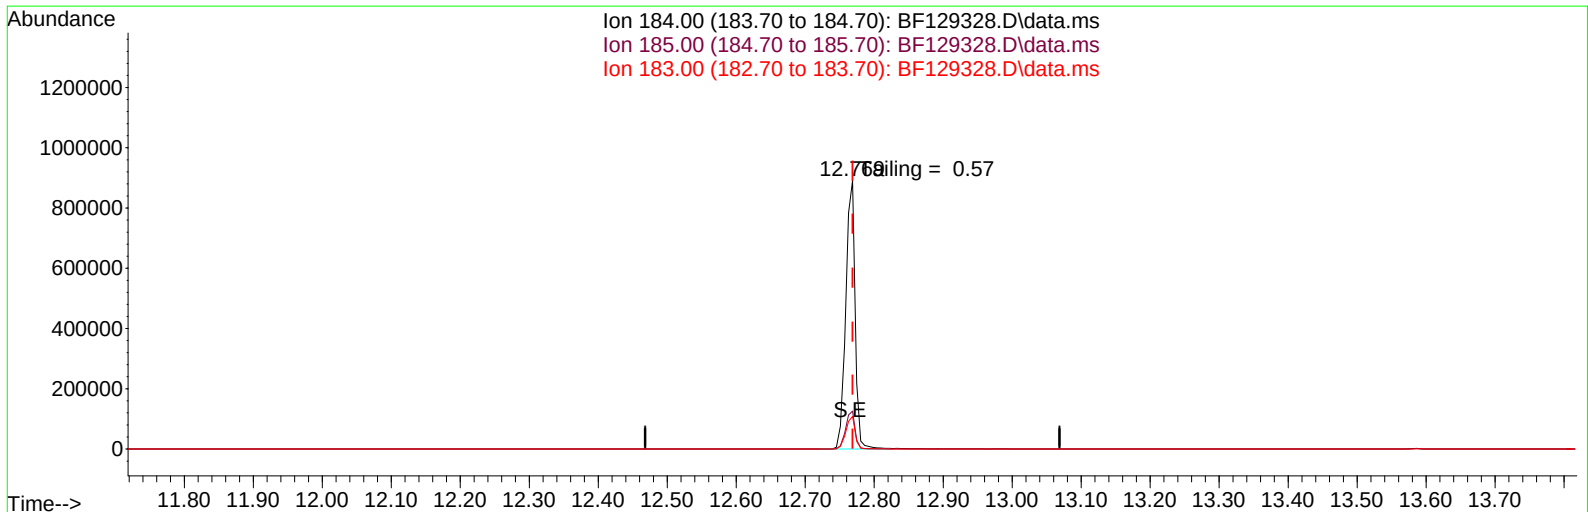

TIC: BF129328.D\data.ms

(77) Benzidine

12.769min (+ 0.000) 3865.28 ng m

response 839354

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.13
183.00	11.60	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/25/2022	BNA_F	<u>BF129328.D</u>
Compound Name	Response	Retention Time
DDT	383704	13.58
DDD	2633	13.28
DDE	205	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2838	386542	0.73

Instrument :
BNA_F
ClientSampleId :
DFTPP