

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
 Data File : BF138665.D
 Acq On : 25 Jul 2024 21:23
 Operator : RC/JU
 Sample : P3343-01 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-A-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.904	303	308	313	rVB	4164	6430	1.26%	0.141%
2	5.057	499	504	513	rVB	14250	19470	3.82%	0.427%
3	5.475	570	575	589	rBV	232047	305434	59.95%	6.695%
4	6.487	742	747	763	rBV	237671	312692	61.37%	6.854%
5	6.851	804	809	814	rBV	361137	441886	86.73%	9.687%
6	7.410	899	904	916	rBV	149928	189225	37.14%	4.148%
7	8.133	1022	1027	1036	rBV	417331	509488	100.00%	11.168%
8	9.204	1204	1209	1218	rBV	217078	266240	52.26%	5.836%
9	9.886	1320	1325	1335	rBV	365387	448882	88.10%	9.840%
10	9.975	1336	1340	1346	rVB5	6116	9299	1.83%	0.204%
11	10.674	1454	1459	1474	rVB	101264	133385	26.18%	2.924%
12	10.792	1474	1479	1487	rVB7	3005	6646	1.30%	0.146%
13	11.369	1572	1577	1587	rBV	336802	480423	94.30%	10.531%
14	11.445	1587	1590	1594	rVB	7597	9474	1.86%	0.208%
15	11.874	1659	1663	1664	rBV2	6745	8684	1.70%	0.190%
16	11.898	1664	1667	1671	rVB2	11441	16186	3.18%	0.355%
17	11.986	1678	1682	1690	rVB3	12384	26123	5.13%	0.573%
18	12.168	1709	1713	1715	rBV2	5902	8451	1.66%	0.185%
19	12.416	1751	1755	1758	rBV	11735	17940	3.52%	0.393%
20	12.510	1768	1771	1773	rBV	8041	8712	1.71%	0.191%
21	12.580	1779	1783	1788	rBV	91460	120385	23.63%	2.639%
22	12.810	1816	1822	1828	rBV	99820	158719	31.15%	3.479%
23	12.951	1841	1846	1854	rVB	210704	284359	55.81%	6.233%
24	13.057	1862	1864	1868	rVB	17447	18682	3.67%	0.410%
25	14.010	2021	2026	2036	rVB2	291564	451110	88.54%	9.889%
26	15.474	2271	2275	2287	rVB	178780	303529	59.58%	6.654%


Sum of corrected areas: 4561854

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138665.D
Acq On : 25 Jul 2024 21:23
Operator : RC/JU
Sample : P3343-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-A-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

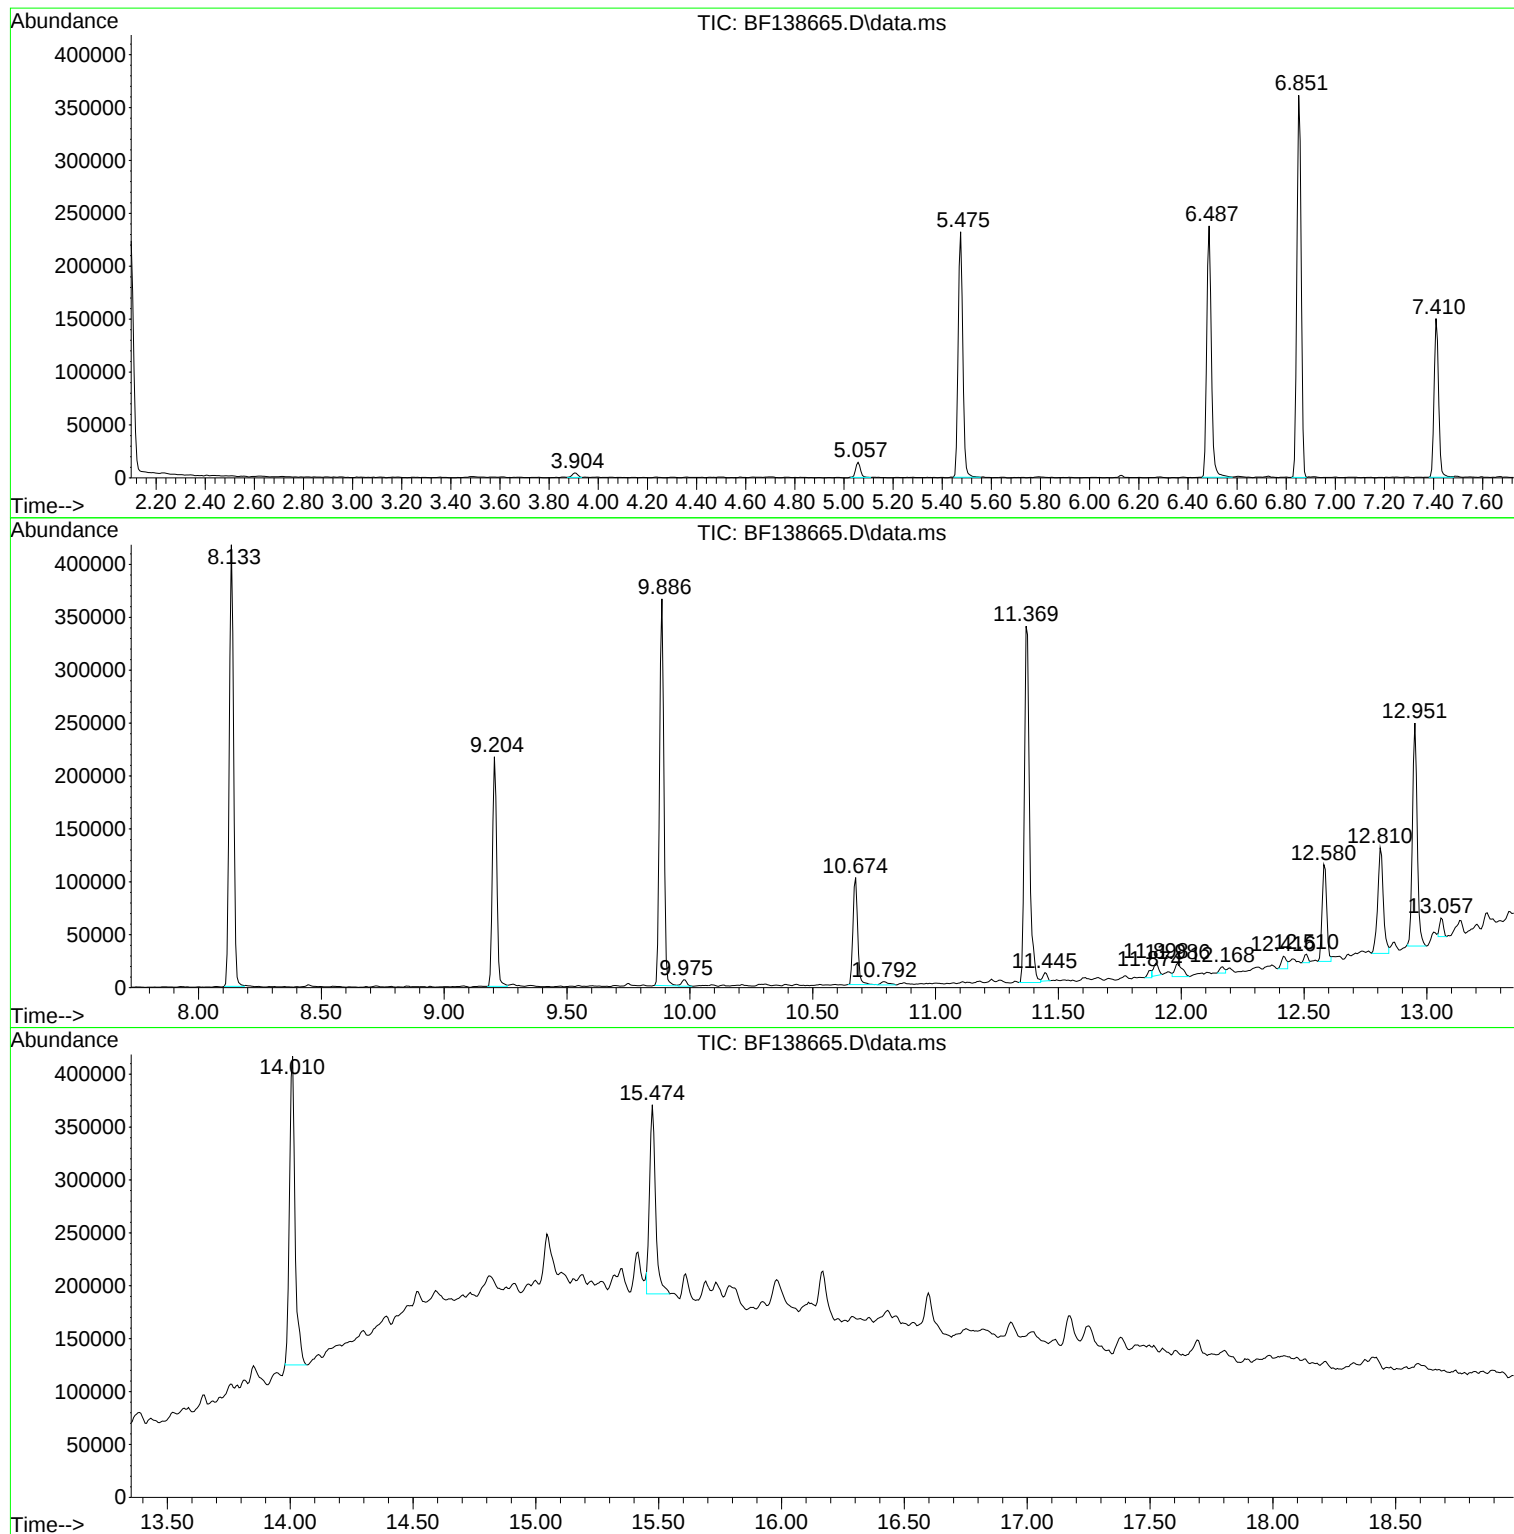

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138665.D
Acq On : 25 Jul 2024 21:23
Operator : RC/JU
Sample : P3343-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-A-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138665.D
Acq On : 25 Jul 2024 21:23
Operator : RC/JU
Sample : P3343-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-A-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------