

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
 Data File : BF138666.D
 Acq On : 25 Jul 2024 21:53
 Operator : RC/JU
 Sample : P3358-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-07242024

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.905	304	308	313	rVB	3148	4890	1.04%	0.147%
2	5.057	499	504	511	rBV	5620	7887	1.68%	0.236%
3	5.475	571	575	584	rBV	85502	116358	24.74%	3.488%
4	6.487	742	747	762	rBV	87673	122109	25.96%	3.660%
5	6.851	804	809	815	rBV	345378	430133	91.45%	12.892%
6	7.410	899	904	912	rBV	55157	73516	15.63%	2.203%
7	8.134	1022	1027	1033	rBV	388552	470360	100.00%	14.098%
8	8.451	1074	1081	1087	rBV3	3389	6356	1.35%	0.191%
9	9.204	1204	1209	1219	rBV	88277	108575	23.08%	3.254%
10	9.281	1219	1222	1229	rVB3	2993	4973	1.06%	0.149%
11	9.810	1305	1312	1318	rBV5	3802	6804	1.45%	0.204%
12	9.886	1320	1325	1330	rVV	347191	418971	89.07%	12.558%
13	9.981	1334	1341	1349	rVV	52309	80697	17.16%	2.419%
14	10.310	1393	1397	1405	rVB2	4719	6025	1.28%	0.181%
15	10.528	1429	1434	1441	rBV2	2969	5414	1.15%	0.162%
16	10.675	1455	1459	1466	rVB	37343	47189	10.03%	1.414%
17	10.786	1473	1478	1487	rVB2	8346	14403	3.06%	0.432%
18	11.233	1550	1554	1556	rBV2	5848	7760	1.65%	0.233%
19	11.257	1556	1558	1564	rVB3	4391	6405	1.36%	0.192%
20	11.369	1572	1577	1588	rBV	320508	442736	94.13%	13.270%
21	11.657	1623	1626	1630	rVB	6226	7668	1.63%	0.230%
22	11.898	1660	1667	1671	rBV6	6461	16426	3.49%	0.492%
23	11.986	1678	1682	1692	rVB9	6054	11995	2.55%	0.360%
24	12.063	1692	1695	1699	rBV2	9235	11220	2.39%	0.336%
25	12.169	1710	1713	1715	rBV4	3936	5019	1.07%	0.150%
26	12.351	1741	1744	1751	rBV9	5460	11660	2.48%	0.349%
27	12.422	1752	1756	1757	rBV4	8227	10593	2.25%	0.318%
28	12.451	1758	1761	1768	rVB3	16117	27925	5.94%	0.837%
29	12.586	1780	1784	1788	rBV	28215	35823	7.62%	1.074%
30	12.816	1818	1823	1829	rBV2	36647	65788	13.99%	1.972%
31	12.951	1842	1846	1855	rBV	98730	130713	27.79%	3.918%
32	14.010	2022	2026	2033	rVB	261078	342145	72.74%	10.255%
33	15.474	2271	2275	2283	rVB	170731	277812	59.06%	8.327%


Sum of corrected areas: 3336348

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138666.D
Acq On : 25 Jul 2024 21:53
Operator : RC/JU
Sample : P3358-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-07242024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

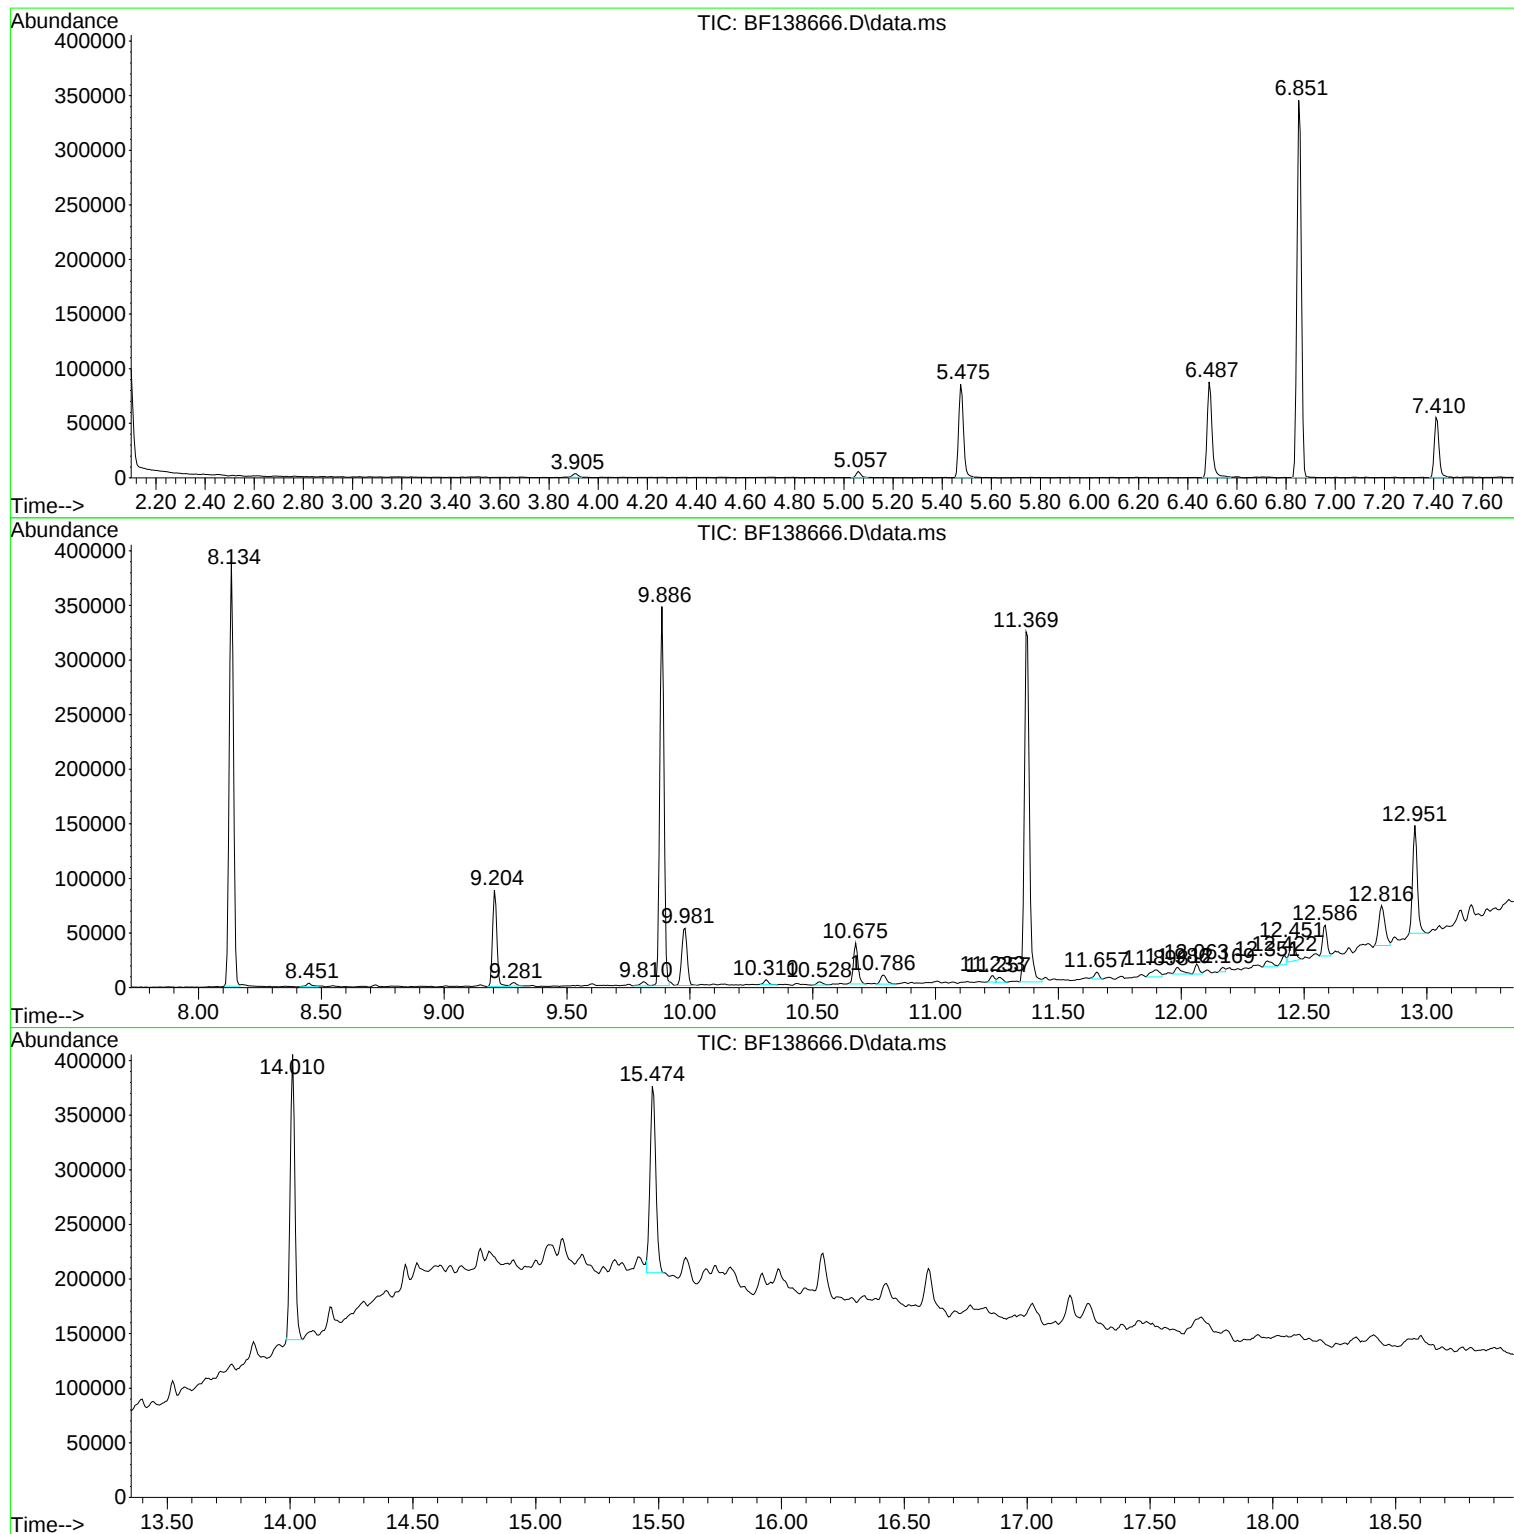

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138666.D
Acq On : 25 Jul 2024 21:53
Operator : RC/JU
Sample : P3358-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-07242024










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown9.981 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.981	3.85 ng	80697	Acenaphthene-d10	9.886

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		3-Octanol, 2,6-dimethyl-, acetate	200	C12H24O2	123232-57-5	27
2		2,4,4-Trimethyl-1-pentanol, chlo...	242	C10H17ClF2O2	1000447-27-2	14
3		3-Hexene-2,5-dione	112	C6H8O2	004436-75-3	11
4		Tetradecane, 1-bromo-	276	C14H29Br	000112-71-0	10
5		Octadecane, 1-bromo-	332	C18H37Br	000112-89-0	10

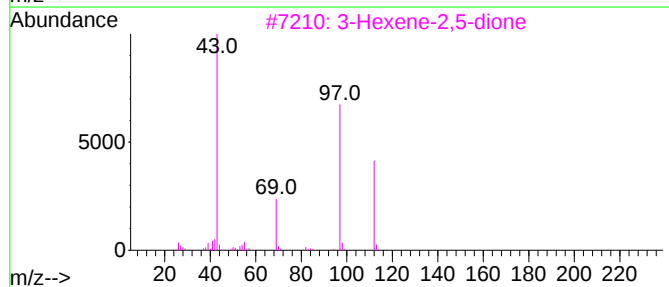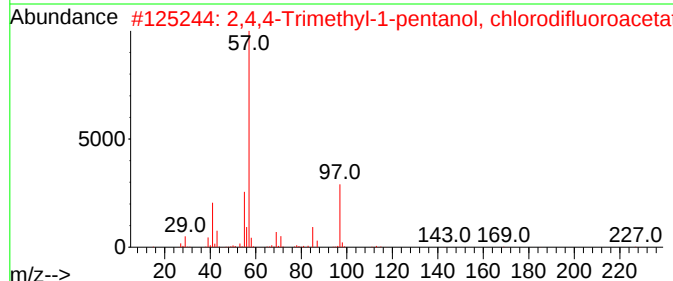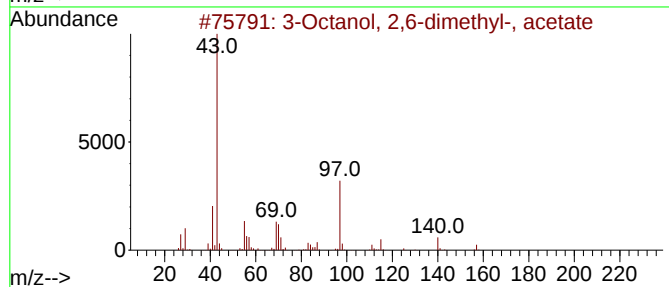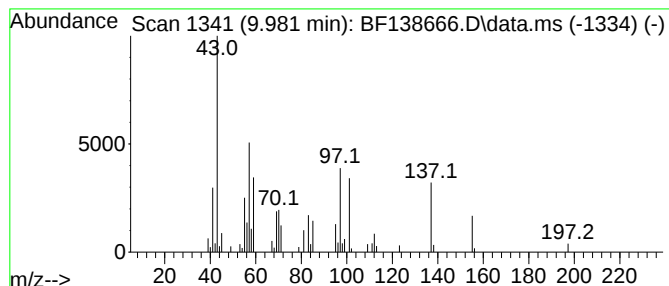

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138666.D
Acq On : 25 Jul 2024 21:53
Operator : RC/JU
Sample : P3358-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-07242024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown9.981	9.981	3.9	ng	80697	3	9.886	418971	20.0