


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138647.D
Acq On : 25 Jul 2024 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

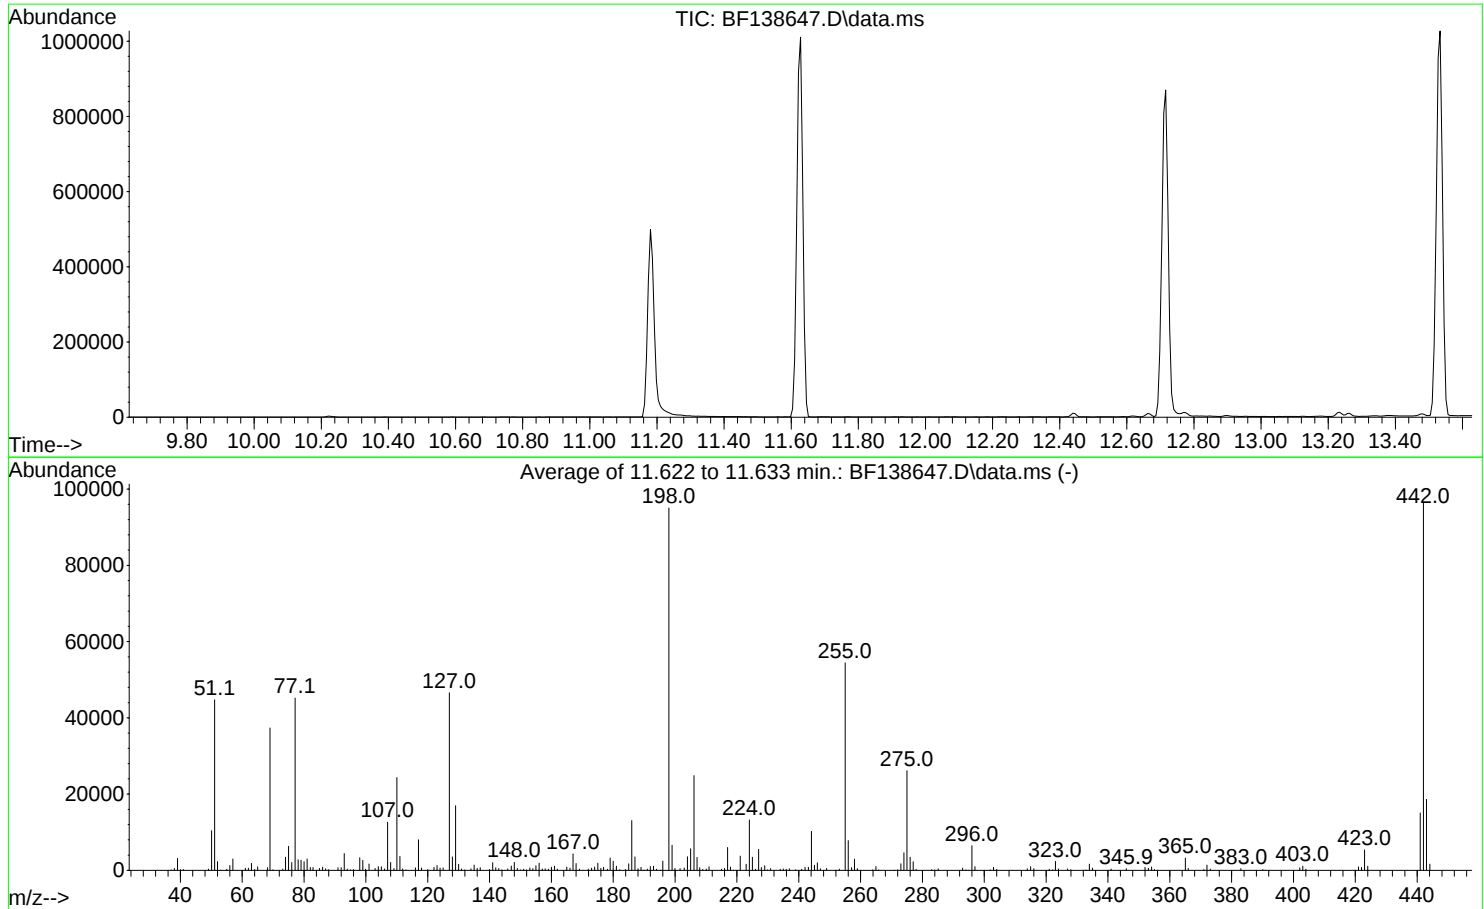




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	44720	PASS
68	69	0.00	2	1.9	719	PASS
69	198	0.00	100	39.3	37336	PASS
70	69	0.00	2	0.4	160	PASS
127	198	10	80	49.0	46560	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95064	PASS
199	198	5	9	6.9	6573	PASS
275	198	10	60	27.5	26157	PASS
365	198	1	100	3.4	3245	PASS
441	198	0.01	100	15.9	15070	PASS
442	442	50	100	100.0	96477	PASS
443	442	15	24	19.3	18652	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138647.D
Acq On : 25 Jul 2024 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 12:39:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

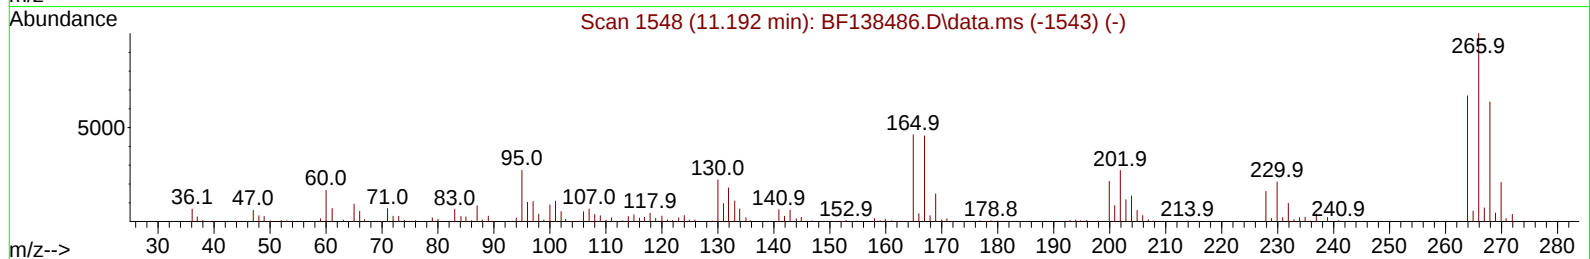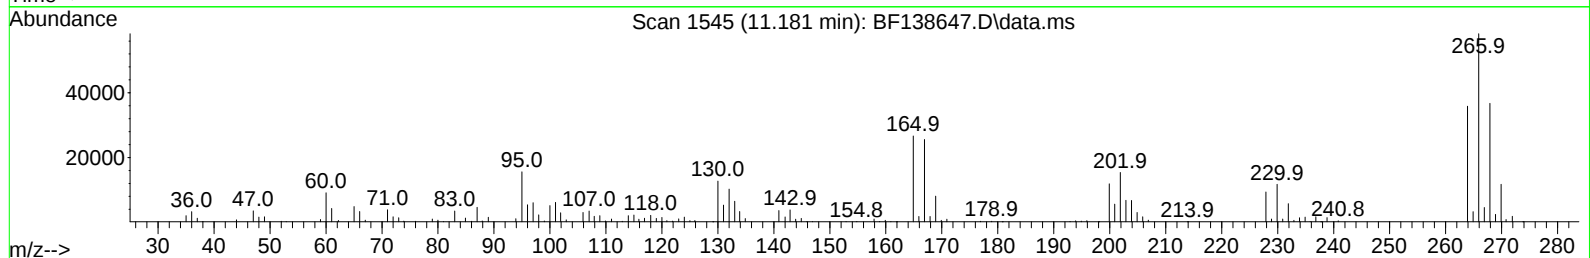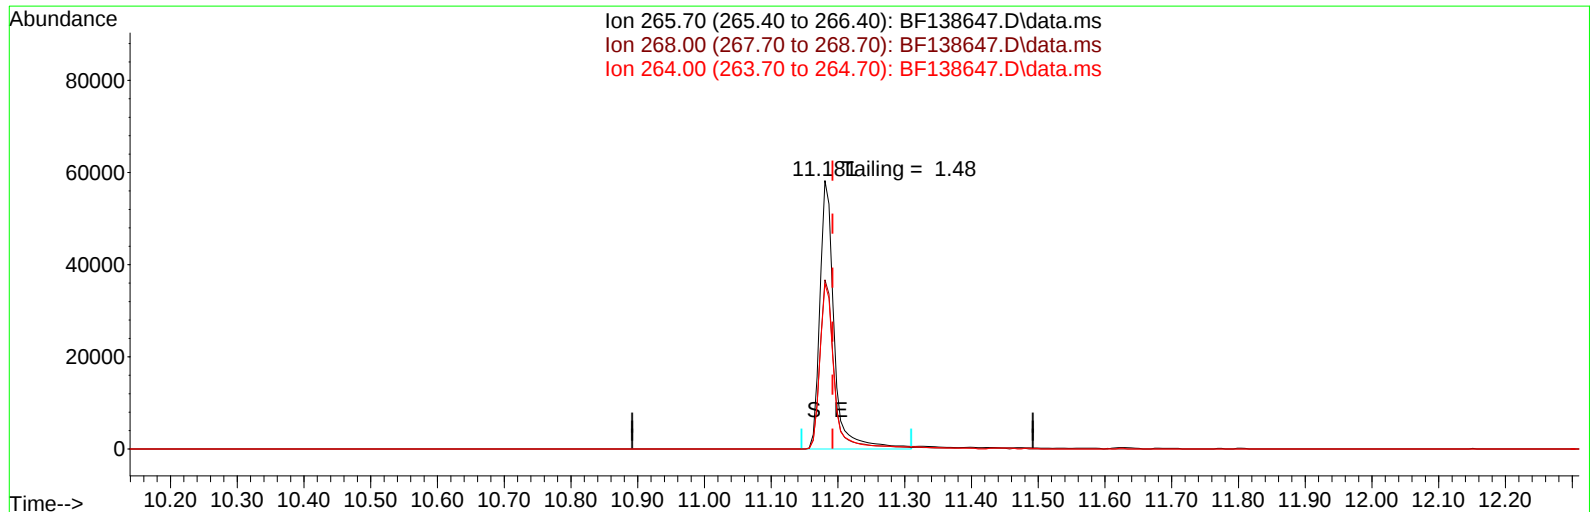

TIC: BF138647.D\data.ms

(70) Pentachlorophenol (C)

11.181min (-0.011) 24927.27 ng




response 86905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.04
264.00	66.90	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072524\
Data File : BF138647.D
Acq On : 25 Jul 2024 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 12:39:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

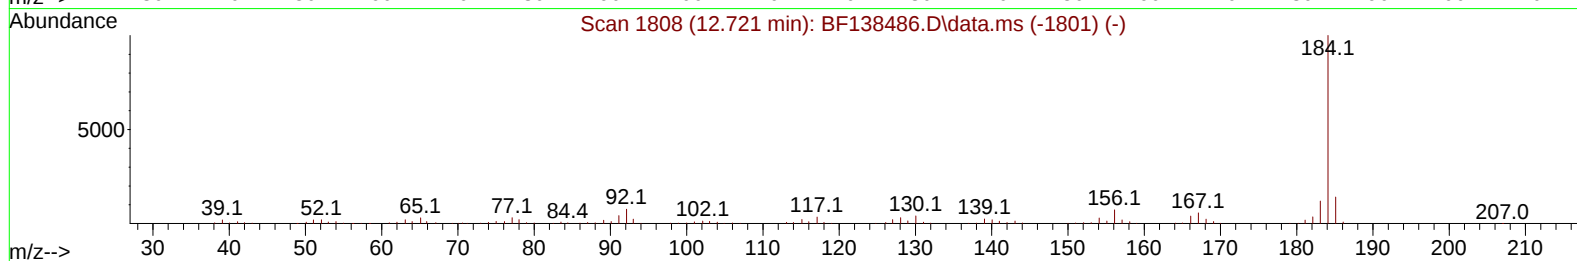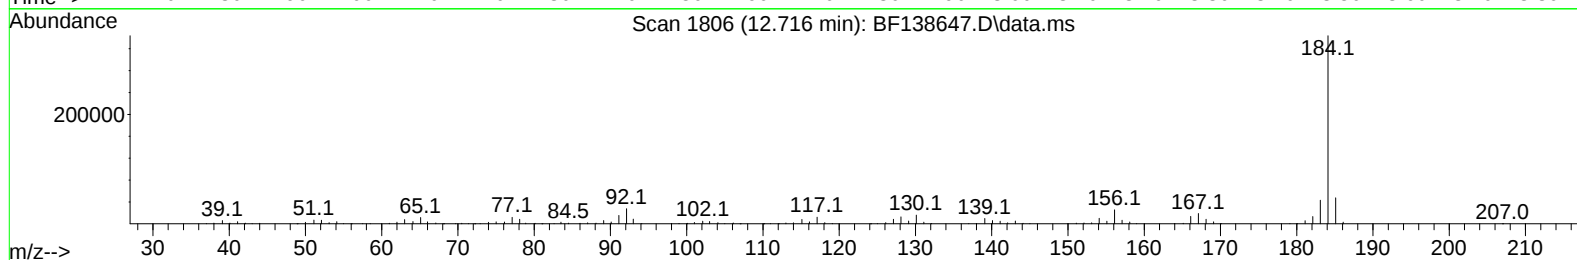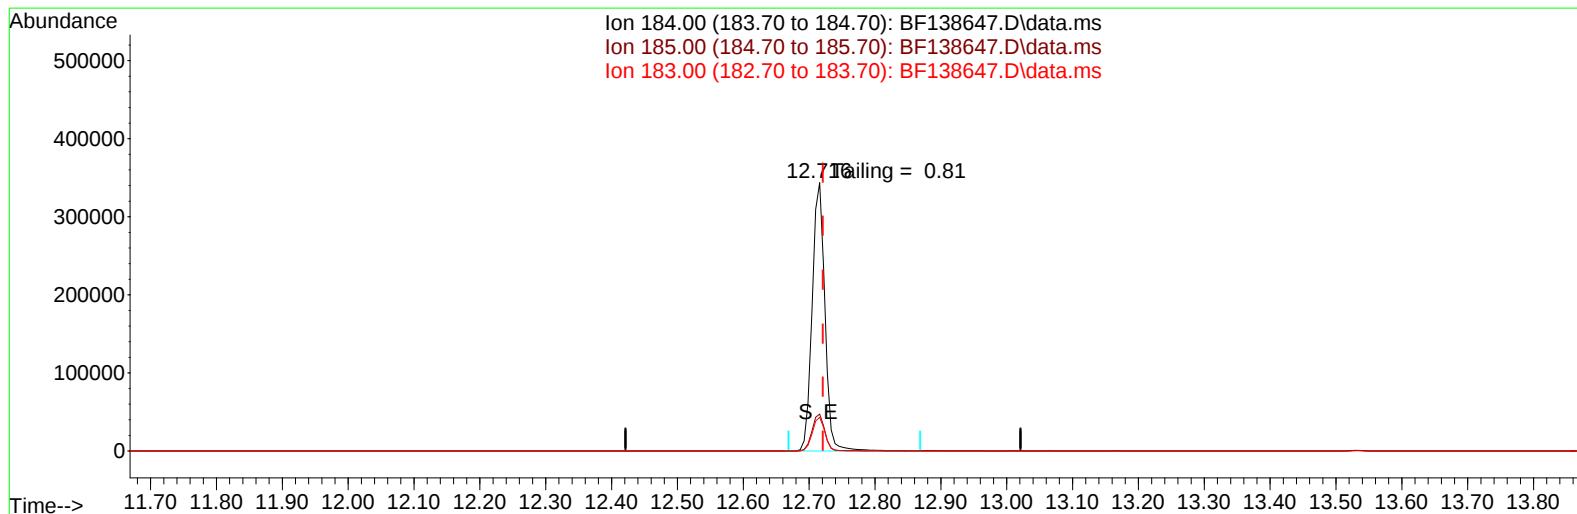

TIC: BF138647.D\data.ms

(77) Benzidine

12.716min (-0.005) 0.00 ng

response 463261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.82
183.00	11.90	12.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/25/2024	BNA_F	<u>BF138647.D</u>
Compound Name	Response	Retention Time
DDT	249642	13.533
DDD	6428	13.233
DDE	1017	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7445	257087	2.90

Instrument :
BNA_F
ClientSampleId :
DFTPP