


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072525\
Data File : BF143245.D
Acq On : 25 Jul 2025 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

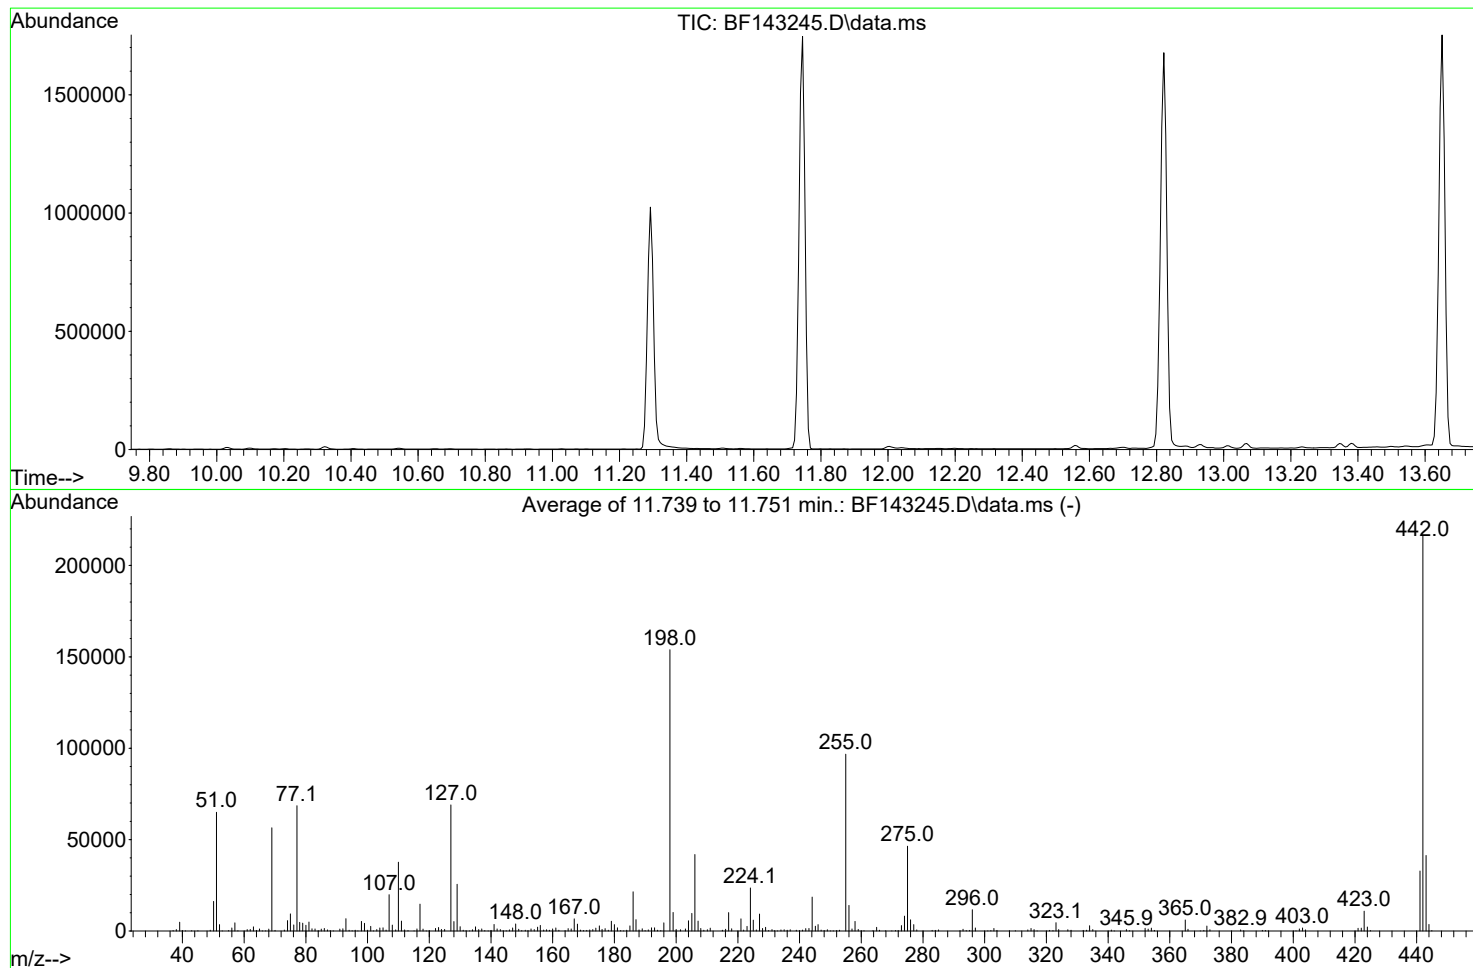

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1083	PASS
69	69	100	100	100.0	56435	PASS
70	69	0.00	2	0.6	337	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153907	PASS
199	198	5	9	6.6	10165	PASS
365	198	1	100	3.9	6025	PASS
441	443	0.01	150	79.5	32861	PASS
442	442	100	100	100.0	216021	PASS
443	442	15	24	19.1	41341	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/25/2025	BNA_F	<u>BF143245.D</u>
Compound Name	Response	Retention Time
DDT	432332	13.651
DDD	9218	13.345
DDE	2347	13.015
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11565	443897	2.61

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072525\
Data File : BF143245.D
Acq On : 25 Jul 2025 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 13:15:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

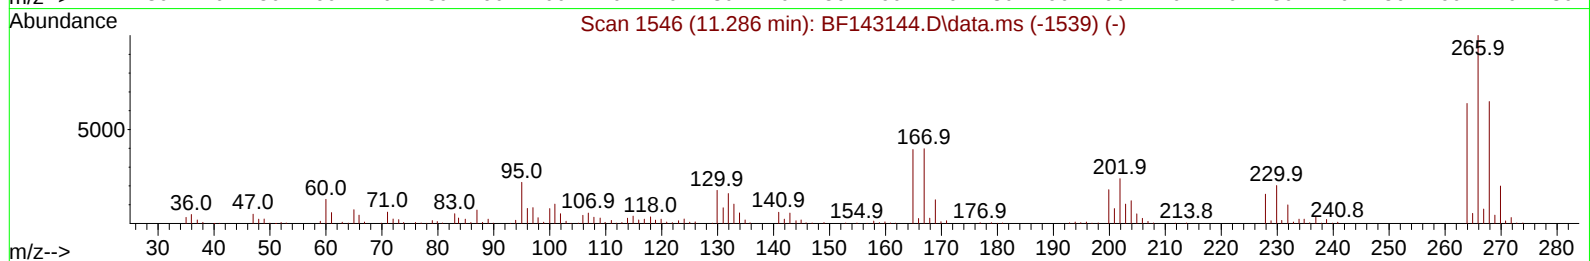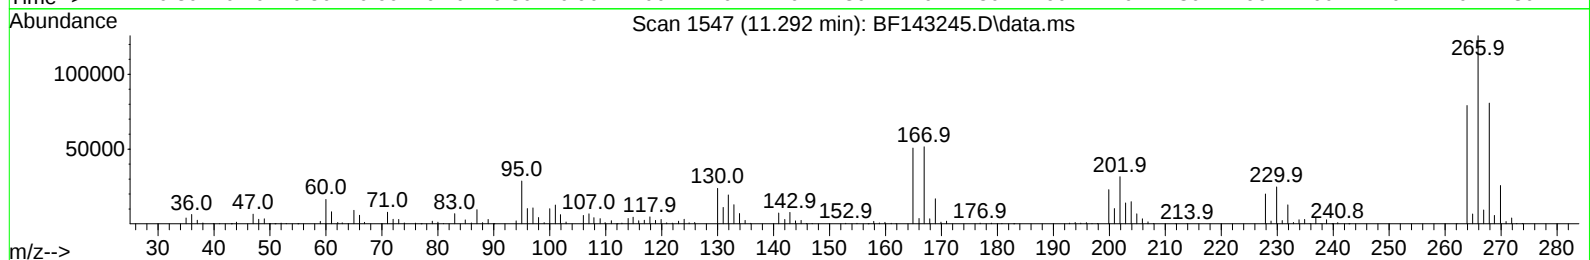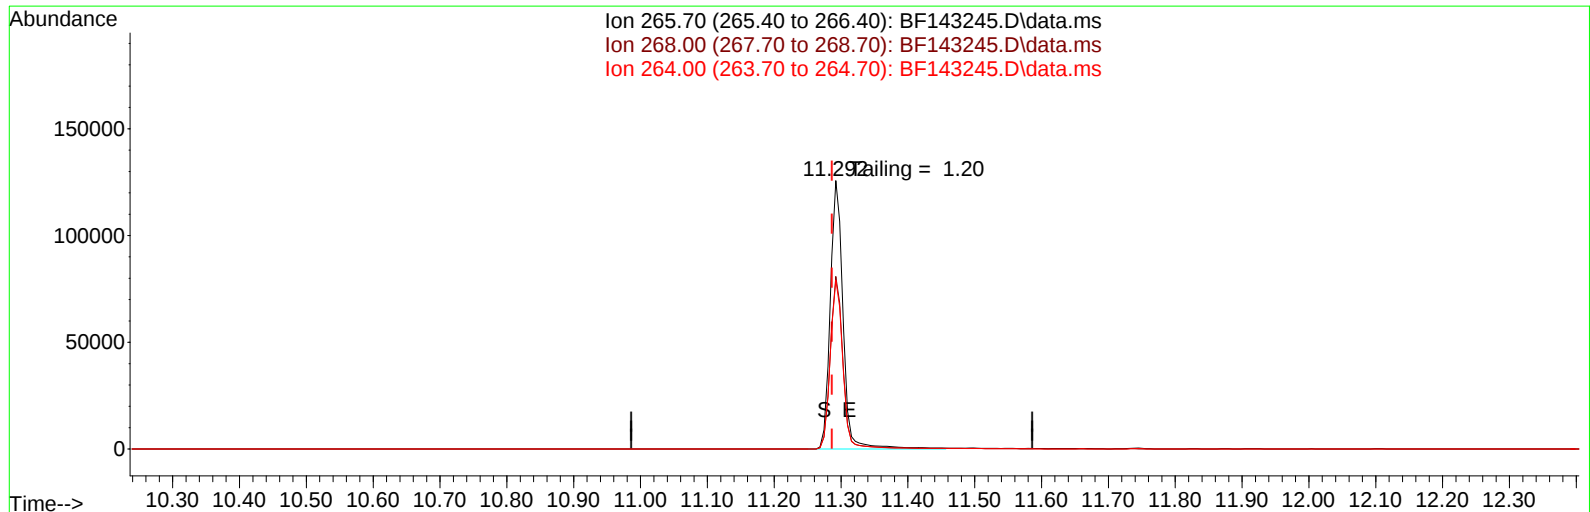

TIC: BF143245.D\data.ms

(70) Pentachlorophenol (C)

11.292min (+ 0.006) 27195.92 ng




response 166943

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.25
264.00	63.80	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072525\
Data File : BF143245.D
Acq On : 25 Jul 2025 11:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 13:15:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

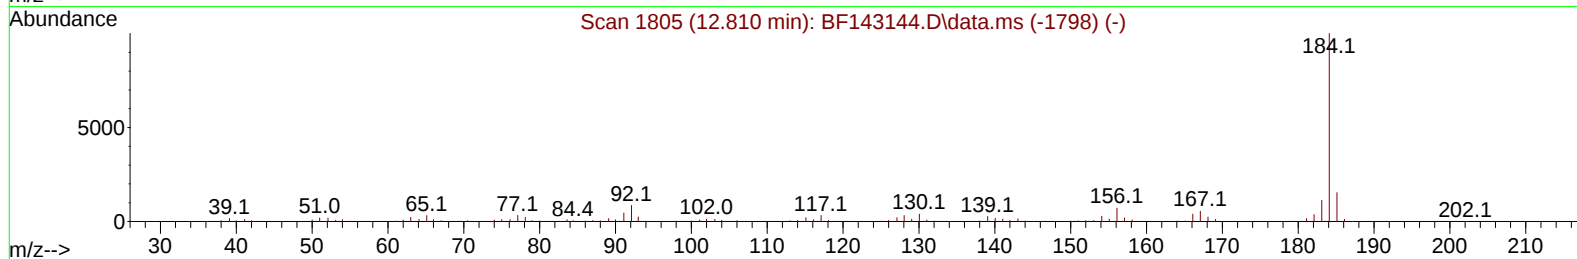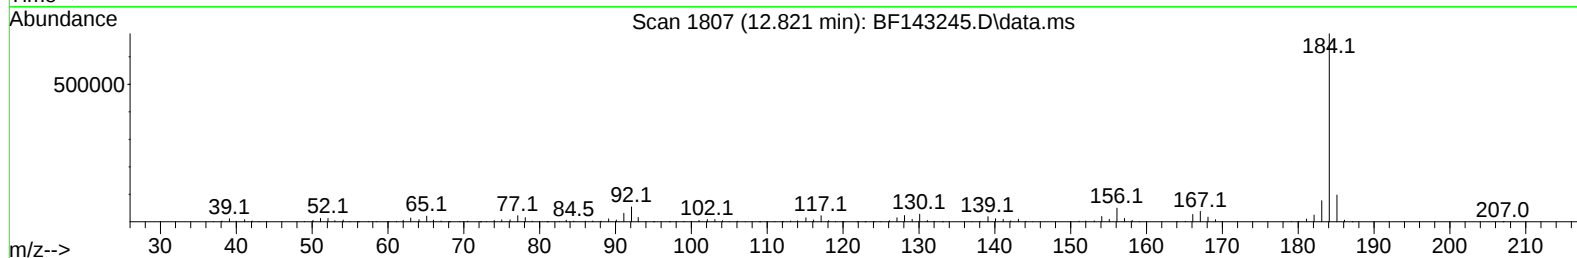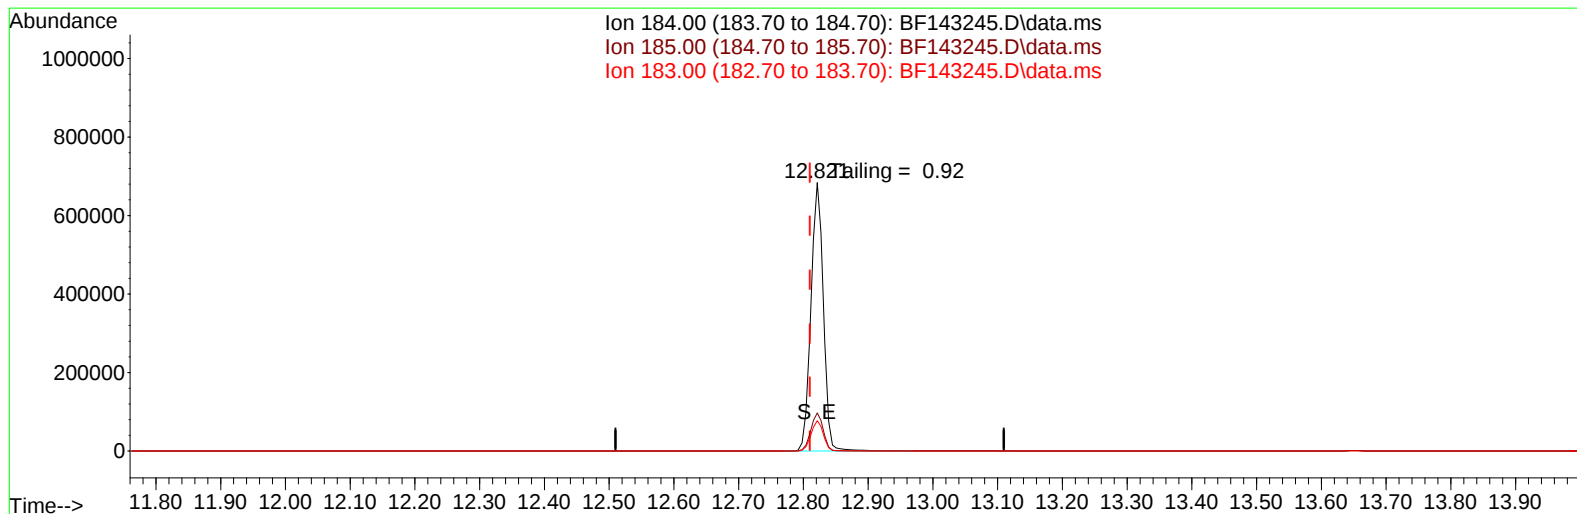

TIC: BF143245.D\data.ms

(77) Benzidine

12.821min (+ 0.011) 0.00 ng

response 918620

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.22
183.00	11.20	11.28
0.00	0.00	0.00