


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072616\
 Data File : BF089303.D
 Acq On : 26 Jul 2016 9:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 25 16:56:43 2016

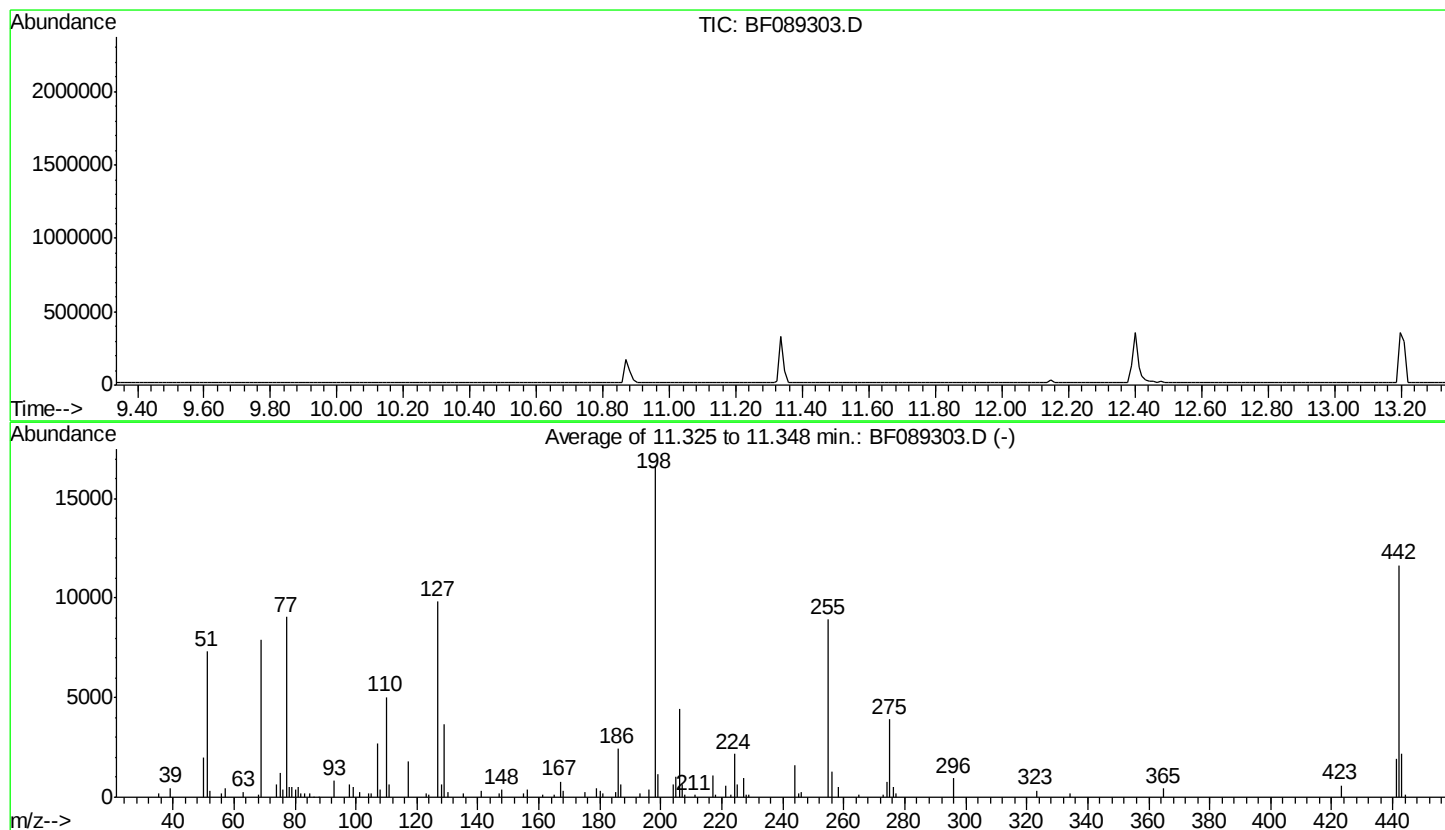

AutoFind: Scans 852, 853, 854; Background Corrected with Scan 849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	7313	PASS
68	69	0.00	2	1.7	134	PASS
69	198	0.00	100	47.4	7886	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.9	9808	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16653	PASS
199	198	5	9	6.8	1137	PASS
275	198	10	60	23.5	3907	PASS
365	198	1	100	2.6	436	PASS
441	442	0.01	24	16.4	1912	PASS
442	198	50	100	70.1	11668	PASS
443	442	15	24	18.8	2188	PASS