

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072617\
 Data File : BF097073.D
 Acq On : 26 Jul 2017 14:12
 Operator : SJ/JU
 Sample : I4443-04 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-M7-NSW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.622	462	465	473	rBV	47726	58468	5.42%	0.611%
2	5.087	541	544	561	rBV	487201	530786	49.23%	5.550%
3	6.151	722	725	736	rBV	609531	606118	56.22%	6.338%
4	6.263	741	744	752	rVB	670795	573096	53.15%	5.993%
5	6.492	779	783	790	rBV	817598	690755	64.07%	7.223%
6	6.645	806	809	819	rBV	393098	391461	36.31%	4.093%
7	7.057	876	879	893	rVB	404935	364739	33.83%	3.814%
8	7.780	997	1002	1005	rBV	981462	972792	90.22%	10.172%
9	8.857	1181	1185	1188	rBV	520131	468118	43.42%	4.895%
10	9.257	1250	1253	1256	rVB	60311	45217	4.19%	0.473%
11	9.522	1293	1298	1302	rBV	1121980	1078197	100.00%	11.275%
12	9.951	1363	1371	1374	rBV	121694	109720	10.18%	1.147%
13	9.980	1374	1376	1379	rVB2	16454	14257	1.32%	0.149%
14	10.310	1428	1432	1437	rBV	391413	365998	33.95%	3.827%
15	10.451	1450	1456	1457	rBV2	14558	16585	1.54%	0.173%
16	10.998	1545	1549	1553	rBV	1210449	1022008	94.79%	10.687%
17	11.551	1641	1643	1647	rBV2	16179	19475	1.81%	0.204%
18	11.739	1670	1675	1680	rVB3	44776	48627	4.51%	0.508%
19	11.851	1691	1694	1698	rVB	32394	30112	2.79%	0.315%
20	12.580	1814	1818	1821	rBV	464643	396502	36.77%	4.146%
21	12.715	1837	1841	1844	rBV4	9580	13319	1.24%	0.139%
22	13.127	1909	1911	1915	rBV5	10456	12922	1.20%	0.135%
23	13.498	1971	1974	1978	rBV3	21008	27358	2.54%	0.286%
24	13.551	1981	1983	1985	rBV2	11460	12796	1.19%	0.134%
25	13.621	1991	1995	1999	rBV	908324	851157	78.94%	8.901%
26	14.127	2078	2081	2086	rBV6	10442	16903	1.57%	0.177%
27	14.786	2190	2193	2194	rBV2	18998	25487	2.36%	0.267%
28	14.974	2220	2225	2231	rBV	589325	633036	58.71%	6.620%
29	15.027	2231	2234	2237	rVB3	14391	16789	1.56%	0.176%
30	15.386	2292	2295	2299	rVB3	15165	19329	1.79%	0.202%
31	15.545	2319	2322	2325	rBV5	12085	18707	1.74%	0.196%
32	16.286	2444	2448	2453	rBV6	21889	39971	3.71%	0.418%
33	16.503	2483	2485	2491	rBV6	6780	11658	1.08%	0.122%
34	16.703	2516	2519	2523	rBV6	11971	18982	1.76%	0.198%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072617\
Data File : BF097073.D
Acq On : 26 Jul 2017 14:12
Operator : SJ/JU
Sample : I4443-04 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-M7-NSW

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	17.074	2579	2582	2586	rBV6	10633	19045	1.77%	0.199%
36	17.427	2638	2642	2643	rBV3	17407	22516	2.09%	0.235%


Sum of corrected areas: 9563006

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072617\
Data File : BF097073.D
Acq On : 26 Jul 2017 14:12
Operator : SJ/JU
Sample : I4443-04 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-M7-NSW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

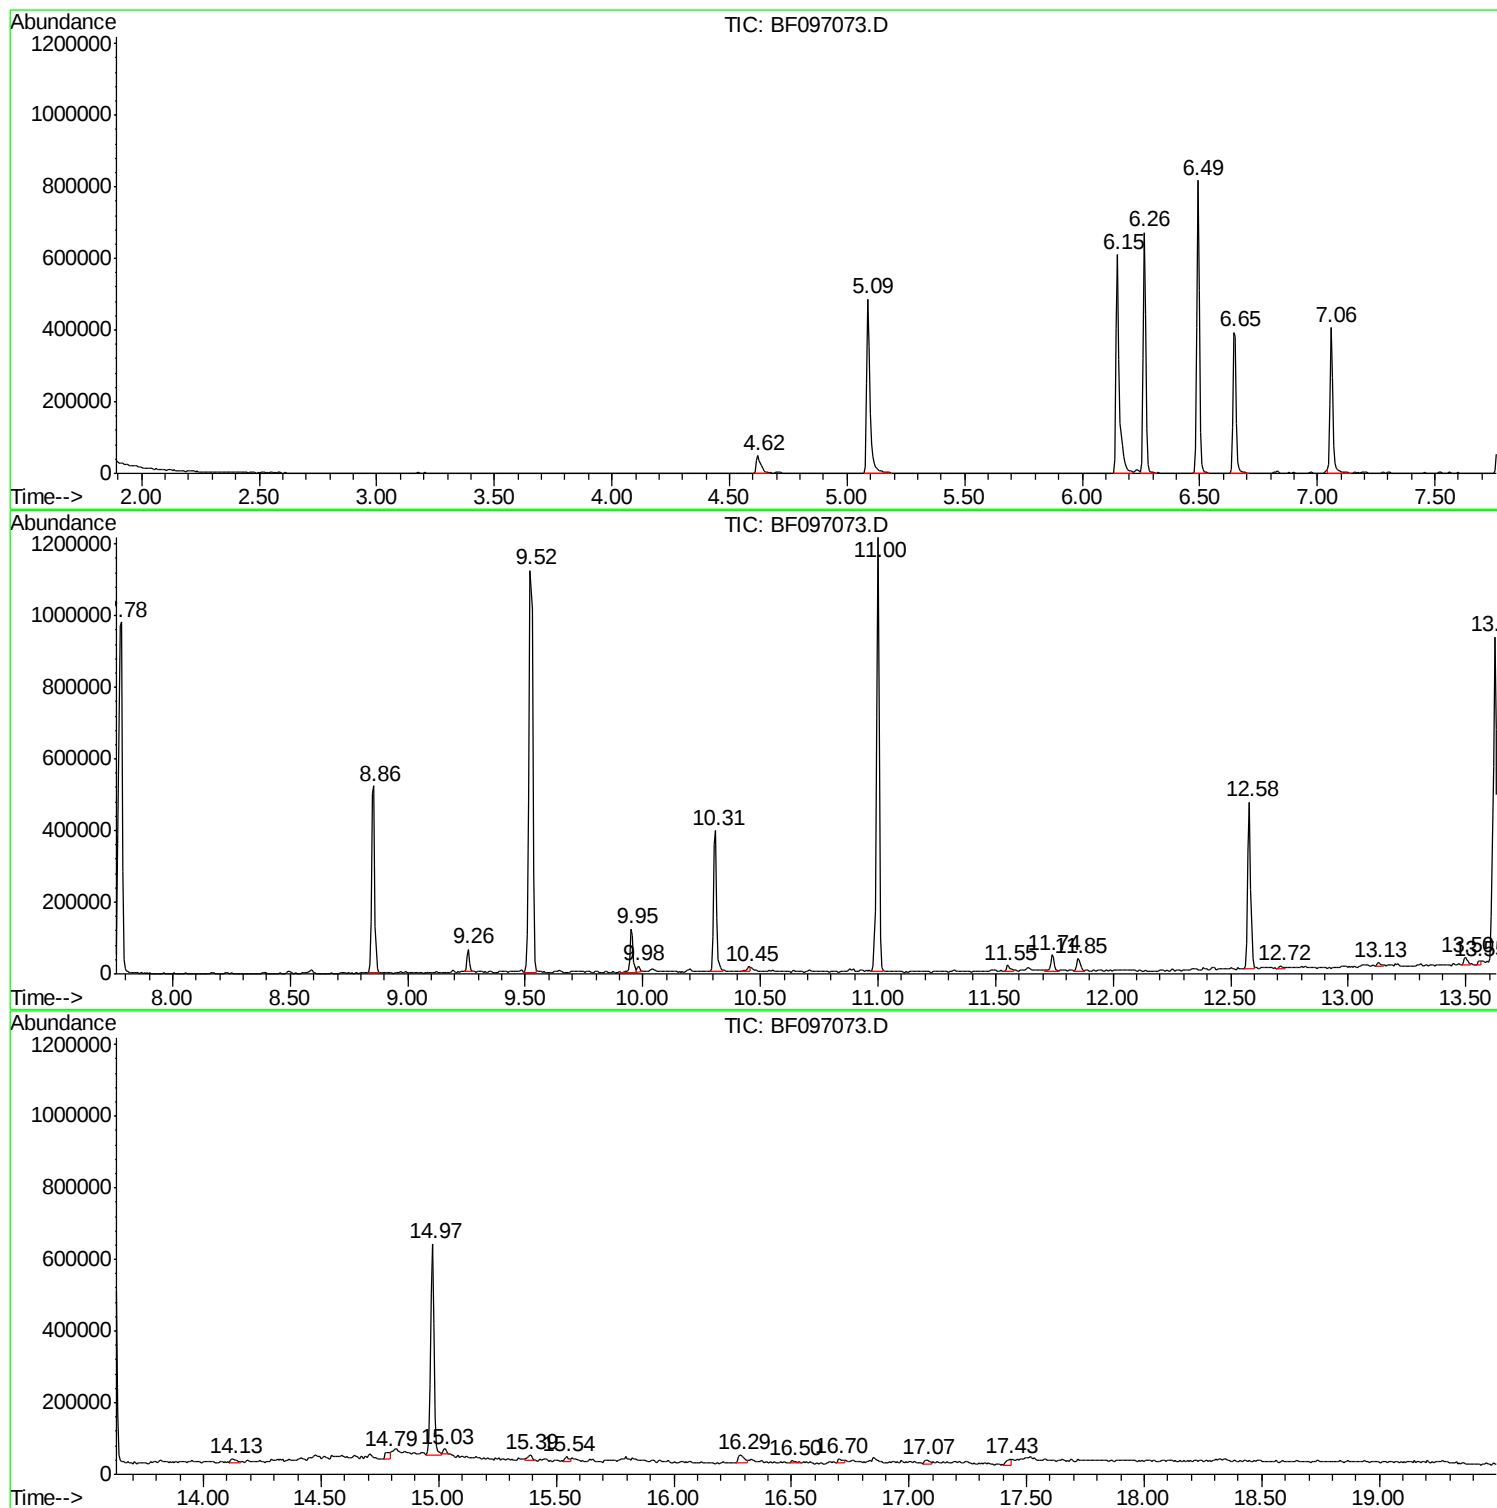

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072617\
Data File : BF097073.D
Acq On : 26 Jul 2017 14:12
Operator : SJ/JU
Sample : I4443-04 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-M7-NSW










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.26 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.26	16.59 ng	573096	1,4-Dichlorobenzene-d4	6.49

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

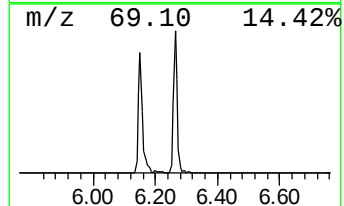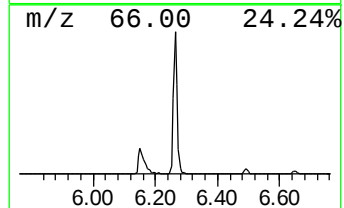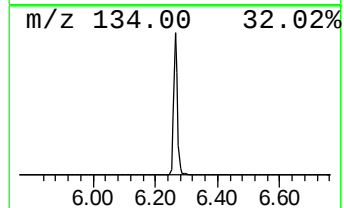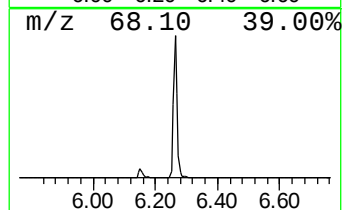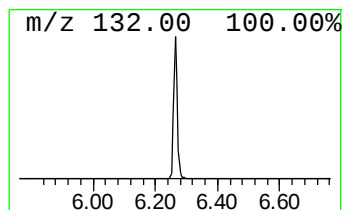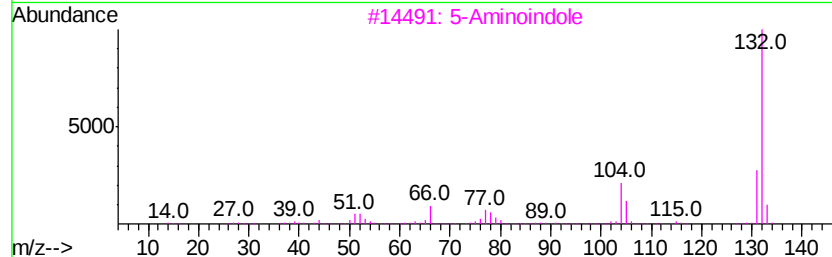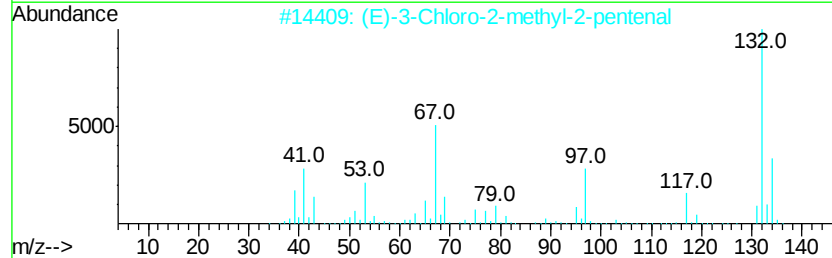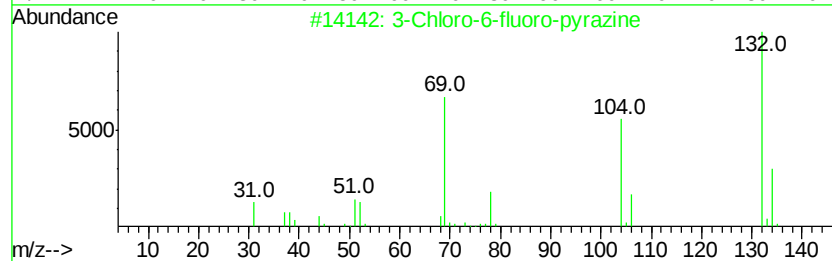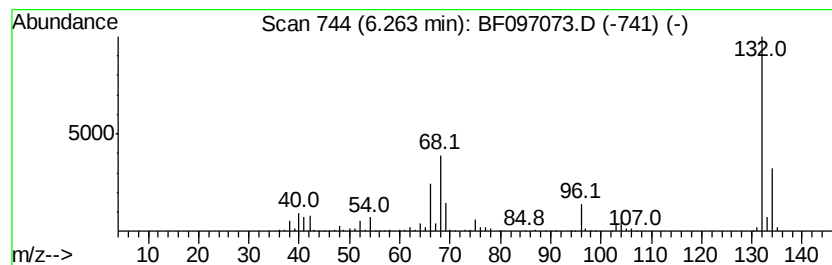

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072617\
Data File : BF097073.D
Acq On : 26 Jul 2017 14:12
Operator : SJ/JU
Sample : I4443-04 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-M7-NSW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.26	6.26	16.6	ng	573096	1	6.49	690755	20.0