


Data Path : Z:\HPCHEM1\BNA F\Data\BF072617\
 Data File : BF097067.D
 Acq On : 26 Jul 2017 11:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 25 14:11:51 2017

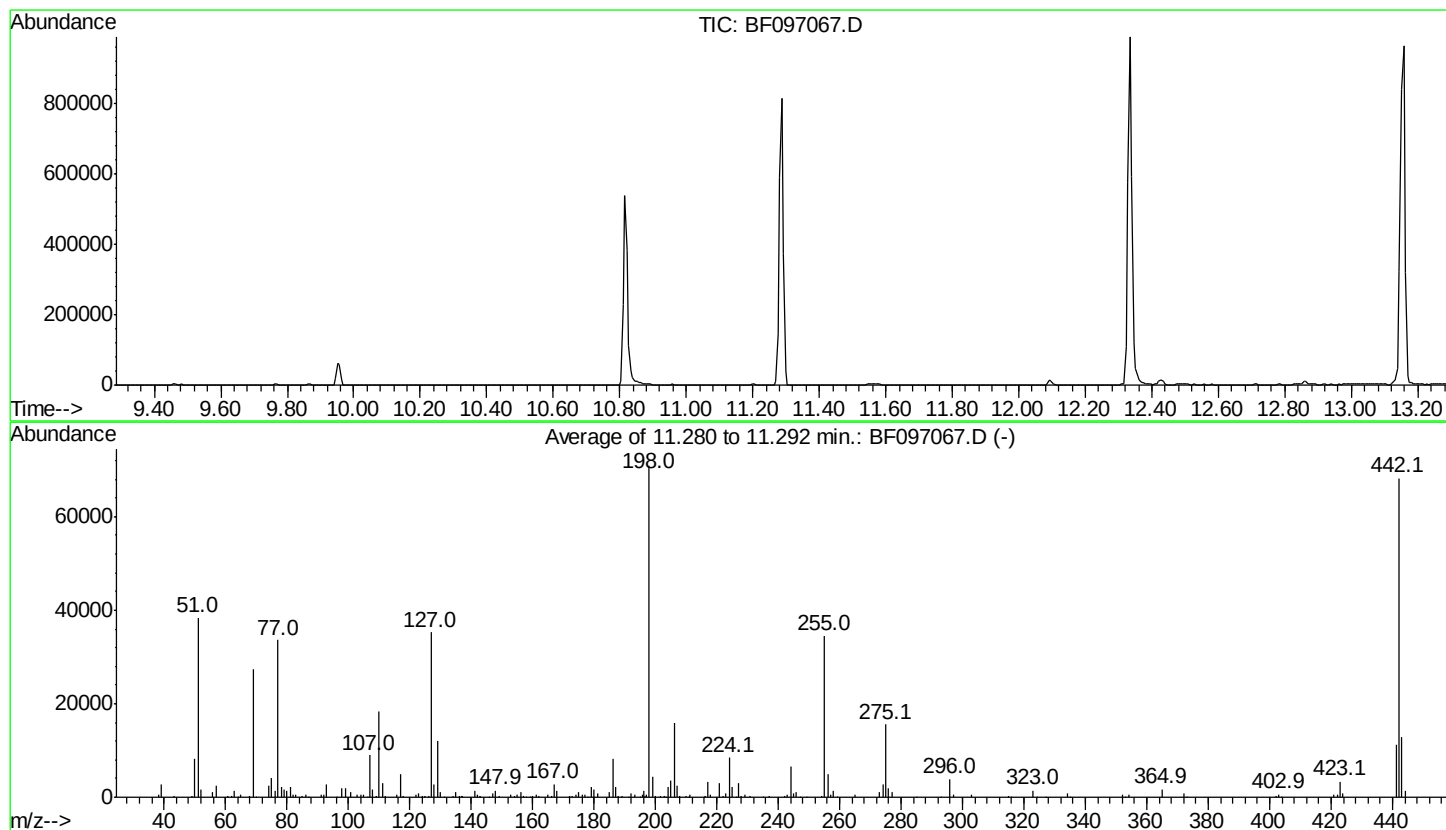

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	38375	PASS
68	69	0.00	2	1.1	290	PASS
69	198	0.00	100	38.7	27417	PASS
70	69	0.00	2	0.5	138	PASS
127	198	10	80	49.6	35202	PASS
197	198	0.00	2	1.0	693	PASS
198	198	100	100	100.0	70906	PASS
199	198	5	9	6.3	4443	PASS
275	198	10	60	22.0	15584	PASS
365	198	1	100	2.5	1750	PASS
441	442	0.01	24	16.5	11262	PASS
442	198	50	100	96.3	68250	PASS
443	442	15	24	19.0	12965	PASS