

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
 Data File : BF124778.D
 Acq On : 26 Jul 2021 22:39
 Operator : JU/CG
 Sample : M3151-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-3

Quant Time: Jul 27 04:26:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 15:28:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	5122	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	17376	20.000	ng	# 0.00
39) Acenaphthene-d10	9.910	164	8147	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	12789	20.000	ng	0.00
76) Chrysene-d12	14.039	240	11722	20.000	ng	0.00
86) Perylene-d12	15.515	264	9353	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.492	112	31740	104.922	ng	0.01
7) Phenol-d6	6.498	99	34893	92.007	ng	0.00
23) Nitrobenzene-d5	7.434	82	23090	79.090	ng	0.00
42) 2,4,6-Tribromophenol	10.698	330	6332	90.522	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	42037	75.785	ng	0.00
79) Terphenyl-d14	12.986	244	40768	59.616	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.434	70	3070	15.160	ng	# 72
25) Isophorone	7.434	82	23090	44.729	ng	# 59
51) 2,6-Dinitrotoluene	9.910	165	1034	8.343	ng	# 26
57) 2,4-Dinitrotoluene	9.910	165	1034	6.148	ng	# 18
67) 4-Bromophenyl-phenylether	10.698	248	446	3.288	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124778.D
Acq On : 26 Jul 2021 22:39
Operator : JU/CG
Sample : M3151-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-3

Quant Time: Jul 27 04:26:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration




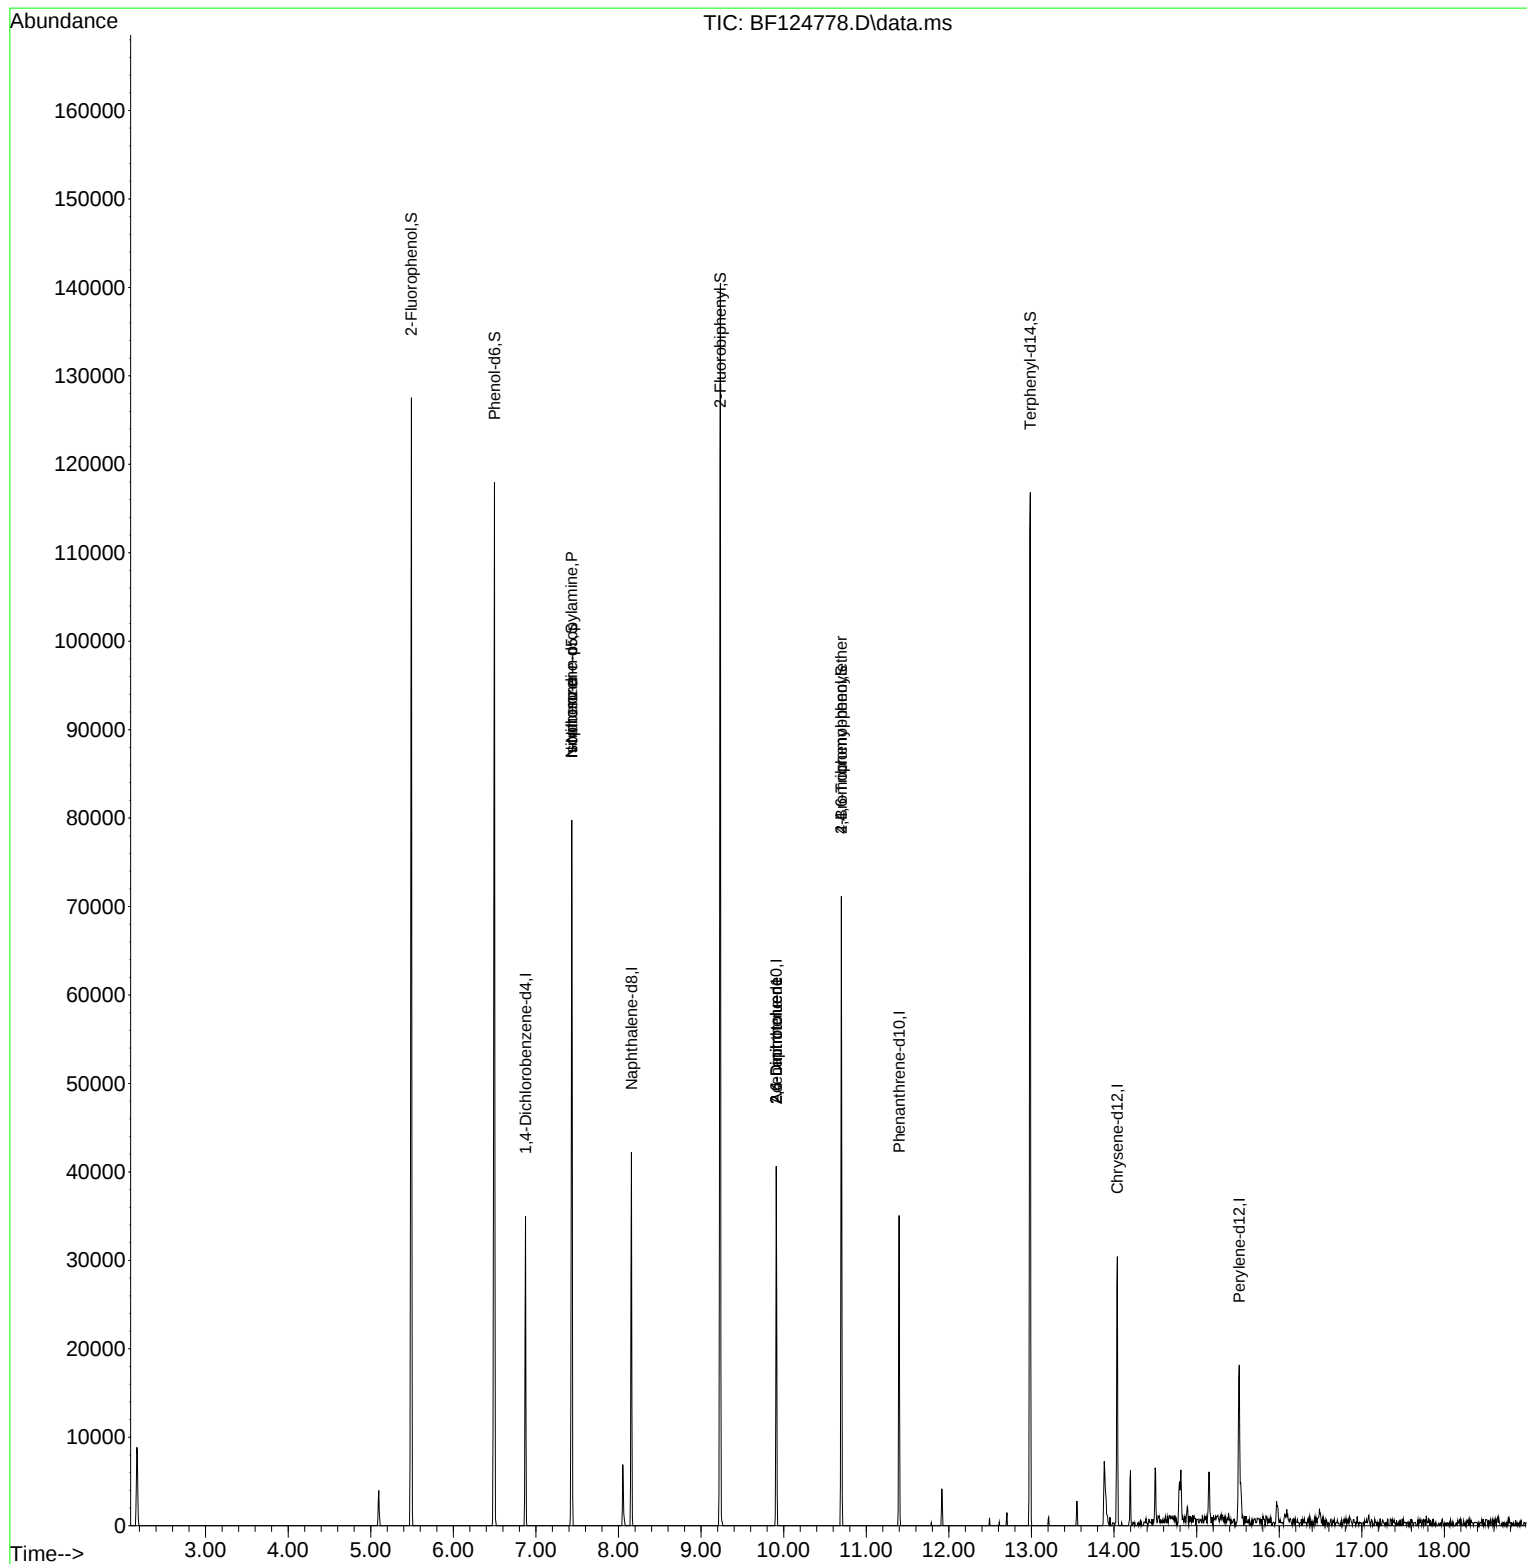


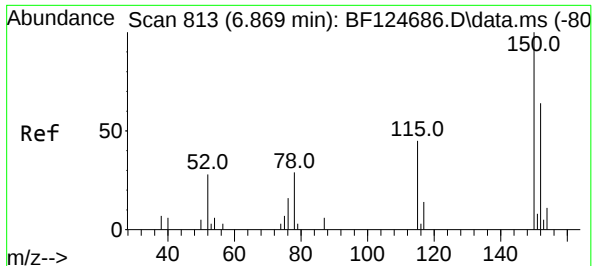

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 814
Delta R.T. 0.006 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39




Instrument :
BNA_F
ClientSampled :
COMP-3


Tgt Ion:152 Resp: 5122
Ion Ratio Lower Upper
152 100
150 143.7 117.6 176.4
115 65.4 47.1 70.7

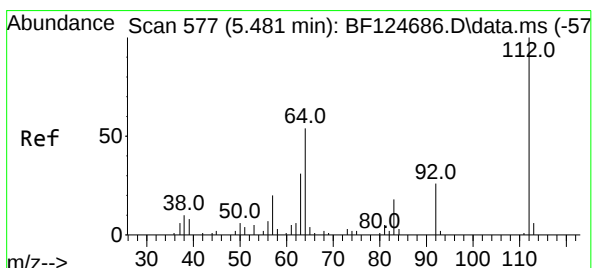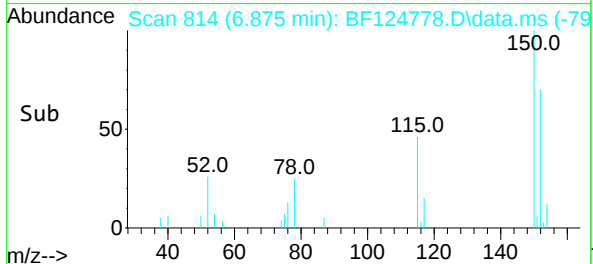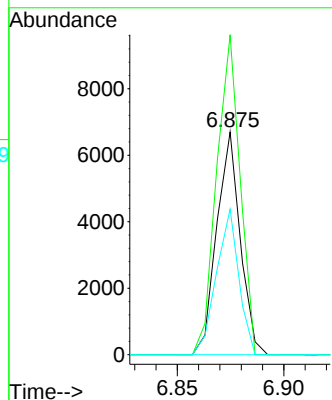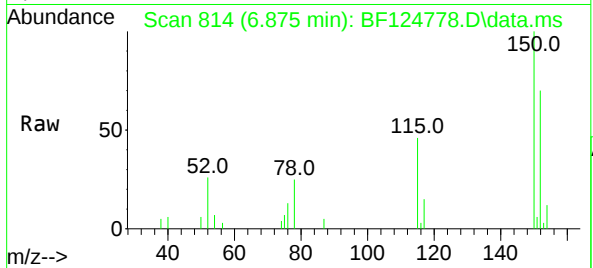

#5
2-Fluorophenol
Concen: 104.922 ng
RT: 5.492 min Scan# 579
Delta R.T. 0.012 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39

Tgt Ion:112 Resp: 31740
Ion Ratio Lower Upper
112 100
64 54.2 44.2 66.2
63 32.2 26.2 39.2


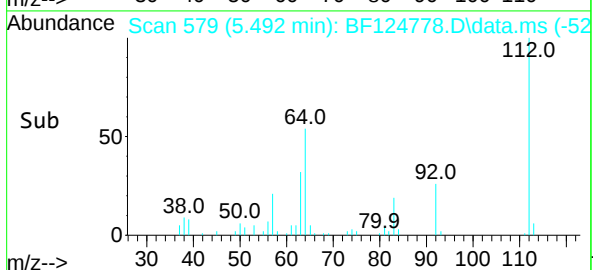
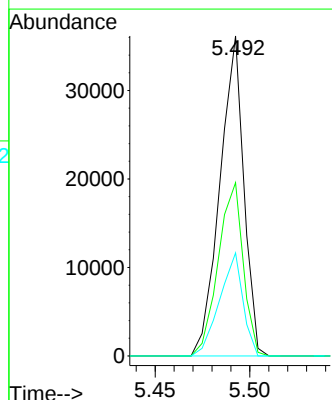
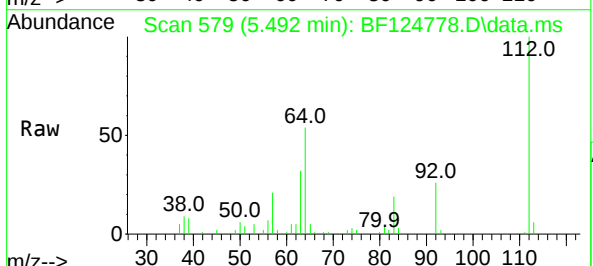




#7
Phenol-d6
Concen: 92.007 ng
RT: 6.498 min Scan# 750
Delta R.T. -0.000 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39




Instrument :
BNA_F
ClientSampleId :
COMP-3


Tgt Ion:	99	Resp:	34893
Ion	Ratio	Lower	Upper
99	100		
42	26.5	23.5	35.3
71	34.9	25.6	38.4

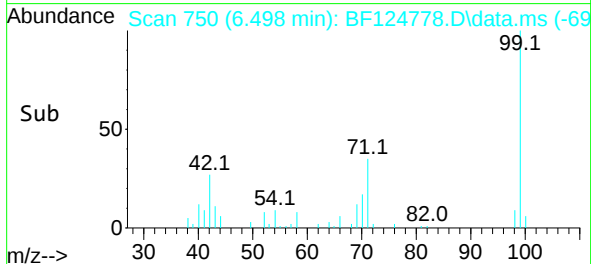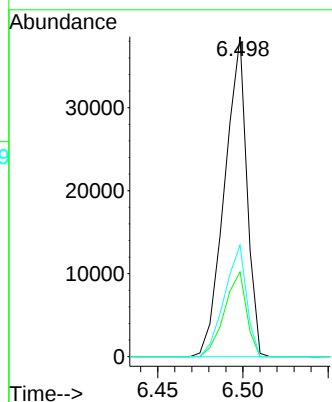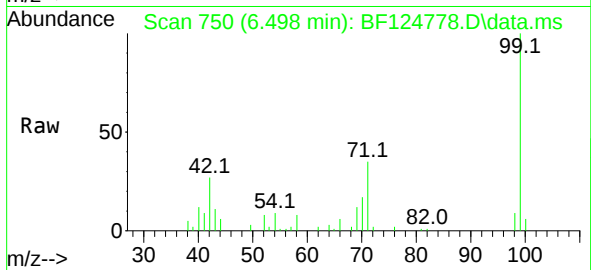

#19
n-Nitroso-di-n-propylamine
Concen: 15.160 ng
RT: 7.434 min Scan# 909
Delta R.T. 0.141 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39

Tgt Ion:	70	Resp:	3070
Ion	Ratio	Lower	Upper
70	100		
42	70.9	72.2	108.2#
101	0.0	7.8	11.8#
130	0.0	21.8	32.6#


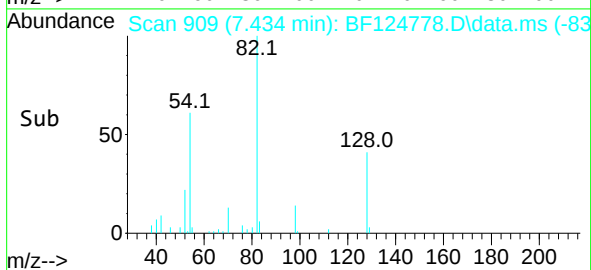
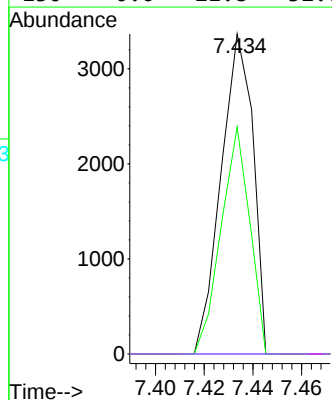
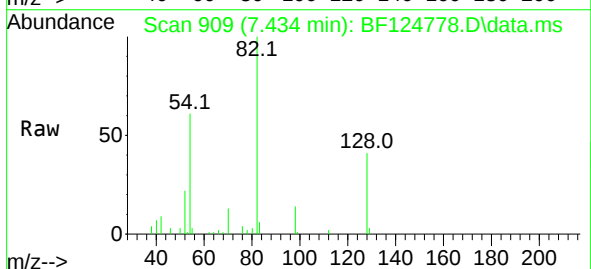


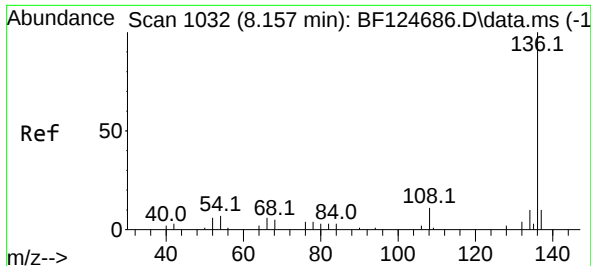

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1032
Delta R.T. -0.000 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39




Instrument :
BNA_F
ClientSampleId :
COMP-3


Tgt Ion:	136	Resp:	17376
Ion Ratio	Lower	Upper	
136	100		
137	10.2	9.8	14.6
54	7.3	6.4	9.6
68	5.0	3.3	4.9

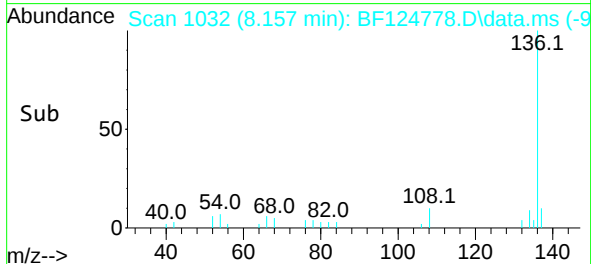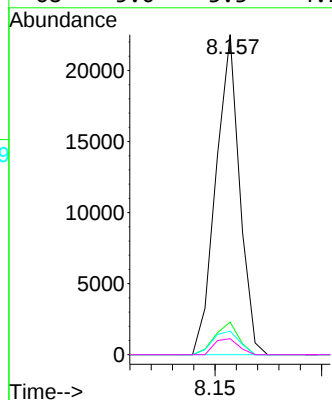

#23
Nitrobenzene-d5
Concen: 79.090 ng
RT: 7.434 min Scan# 909
Delta R.T. -0.006 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39

Tgt Ion:	82	Resp:	23090
Ion Ratio	Lower	Upper	
82	100		
128	40.6	40.6	60.8
54	60.7	49.6	74.4


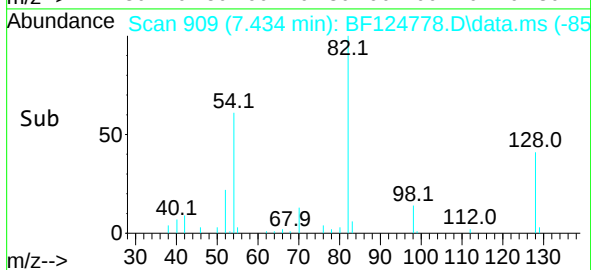
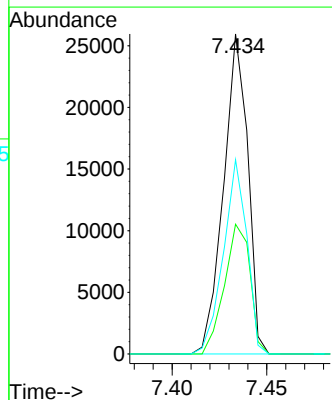
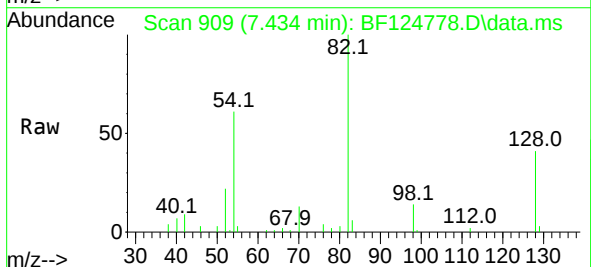


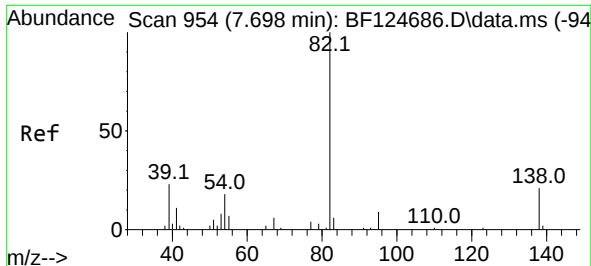

#25
Isophorone
Concen: 44.729 ng
RT: 7.434 min Scan# 909
Delta R.T. -0.265 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39




Instrument :
BNA_F
ClientSampled :
COMP-3


Tgt Ion: 82 Resp: 23090
Ion Ratio Lower Upper
82 100
95 0.0 6.5 9.7#
138 0.0 18.4 27.6#

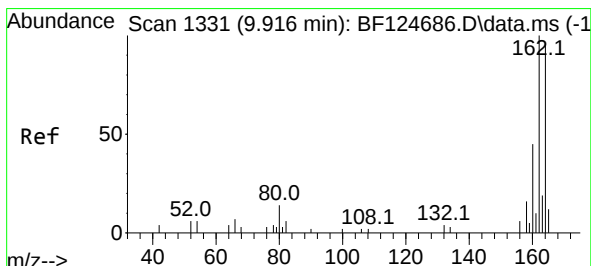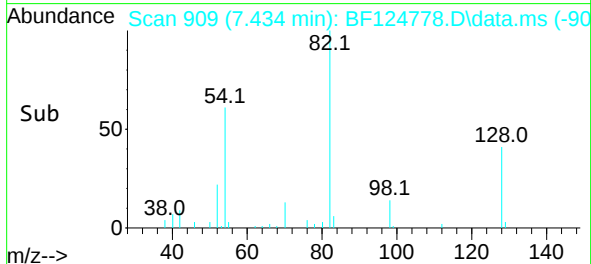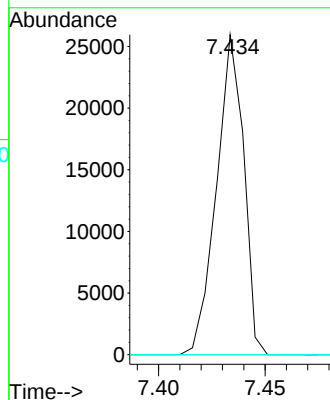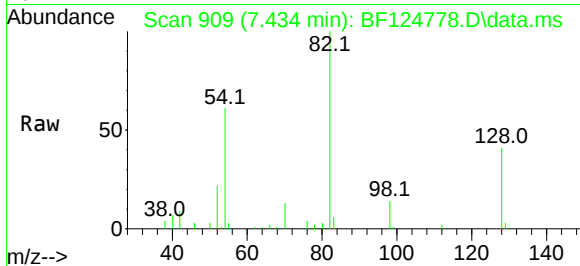

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1330
Delta R.T. -0.006 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39


Tgt Ion: 164 Resp: 8147
Ion Ratio Lower Upper
164 100
162 104.6 81.3 121.9
160 45.3 38.0 57.0

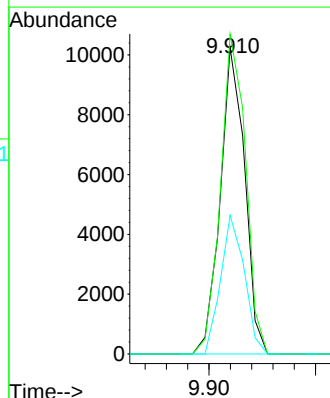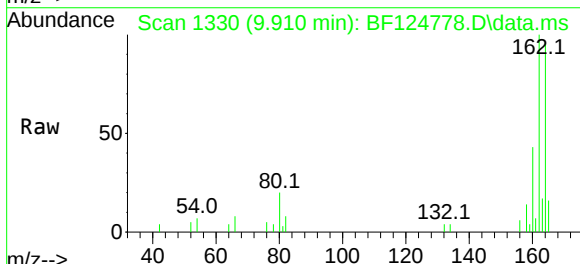



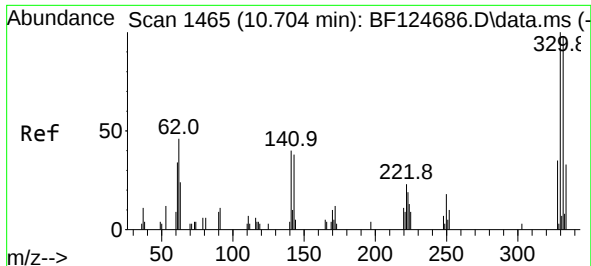


#42
2,4,6-Tribromophenol
Concen: 90.522 ng
RT: 10.698 min Scan# 1464
Delta R.T. -0.006 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39

Instrument :
BNA_F
ClientSampleId :
COMP-3







Tgt Ion: 330 Resp: 6332
Ion Ratio Lower Upper
330 100
332 102.0 76.2 114.4
141 49.6 44.6 66.8

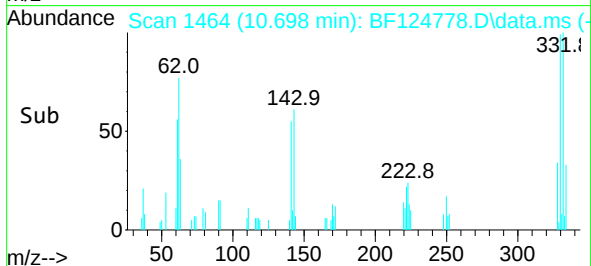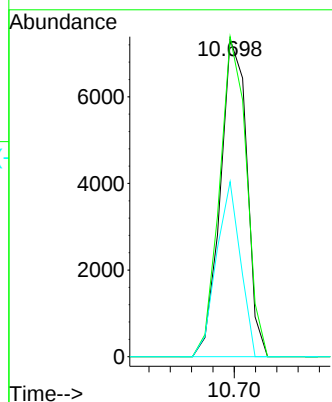

#45
2-Fluorobiphenyl
Concen: 75.785 ng
RT: 9.233 min Scan# 1215
Delta R.T. -0.000 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39

Tgt Ion: 172 Resp: 42037
Ion Ratio Lower Upper
172 100
171 33.8 26.5 39.7
170 23.5 18.8 28.2


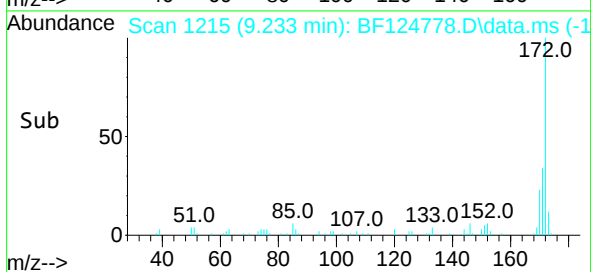
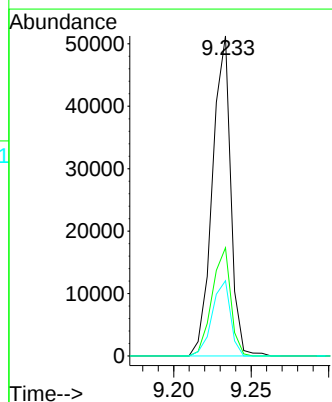
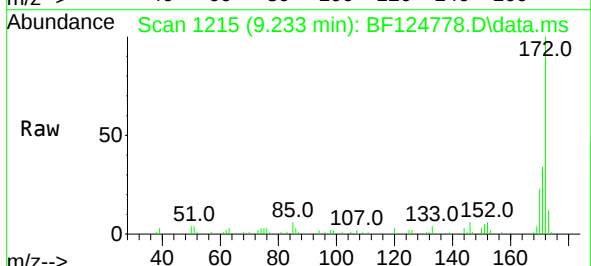




#51
2,6-Dinitrotoluene
Concen: 8.343 ng
RT: 9.910 min Scan# 1330
Delta R.T. 0.212 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39




Instrument :
BNA_F
ClientSampled :
COMP-3


Tgt Ion:165 Resp: 1034
Ion Ratio Lower Upper
165 100
63 0.0 42.6 63.8#
89 0.0 40.6 60.8#

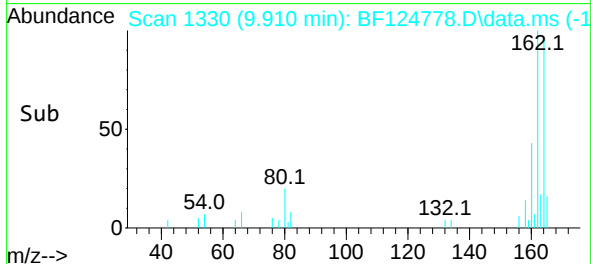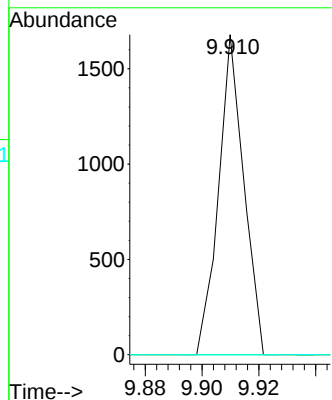

#57
2,4-Dinitrotoluene
Concen: 6.148 ng
RT: 9.910 min Scan# 1330
Delta R.T. -0.188 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39

Tgt Ion:165 Resp: 1034
Ion Ratio Lower Upper
165 100
63 0.0 40.9 61.3#
89 0.0 59.7 89.5#
182 0.0 0.0 0.0



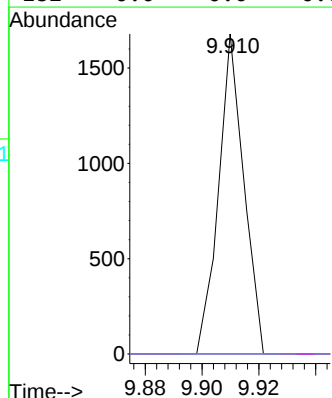
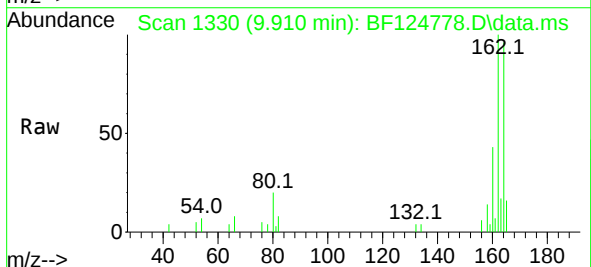


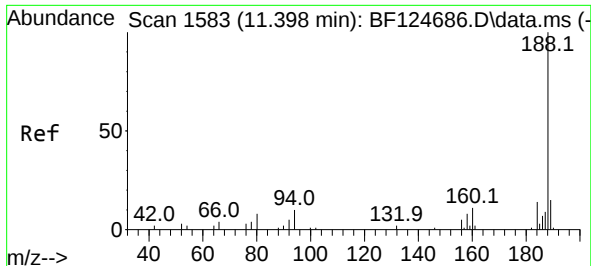

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 1583
Delta R.T. -0.000 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39




Instrument :
BNA_F
ClientSampleId :
COMP-3


Tgt Ion:188 Resp: 12789
Ion Ratio Lower Upper
188 100
94 8.4 6.7 10.1
80 9.2 7.5 11.3

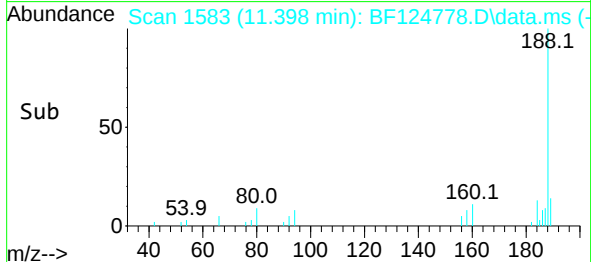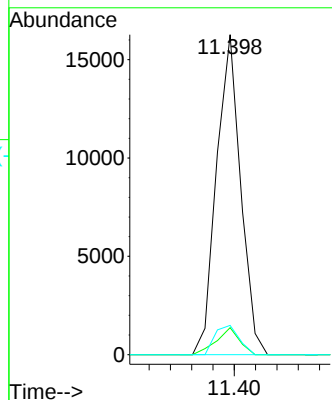

#67
4-Bromophenyl-phenylether
Concen: 3.288 ng
RT: 10.698 min Scan# 1464
Delta R.T. -0.247 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39

Tgt Ion:248 Resp: 446
Ion Ratio Lower Upper
248 100
250 219.1 74.2 111.4#
141 696.6 60.4 90.6#


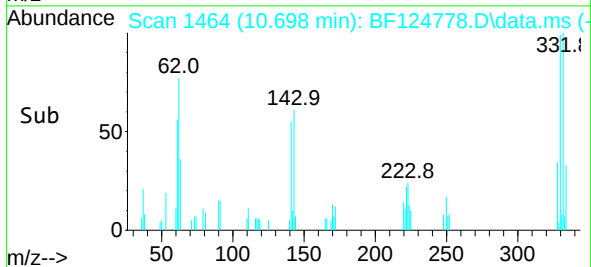
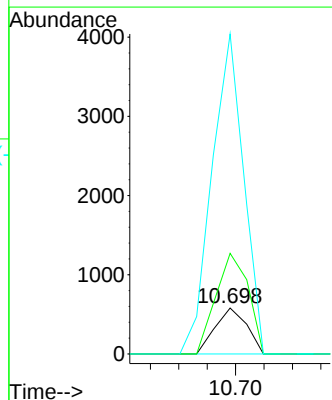
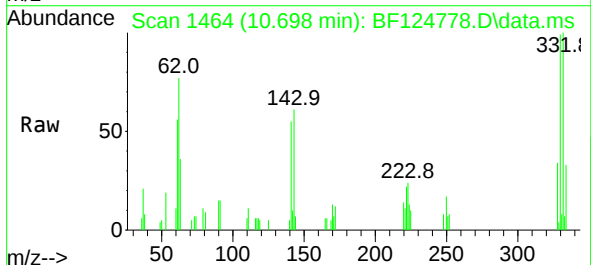


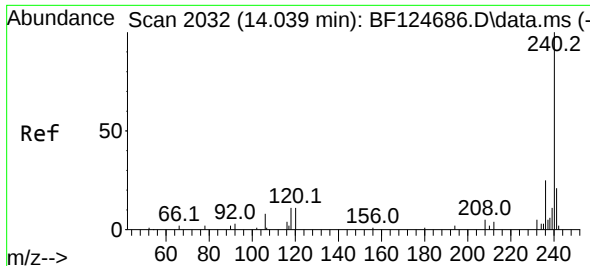

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 2032
Delta R.T. -0.000 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39




Instrument :
BNA_F
ClientSampleId :
COMP-3


Tgt Ion:240 Resp: 11722
Ion Ratio Lower Upper
240 100
120 11.9 10.8 16.2
236 27.5 21.6 32.4

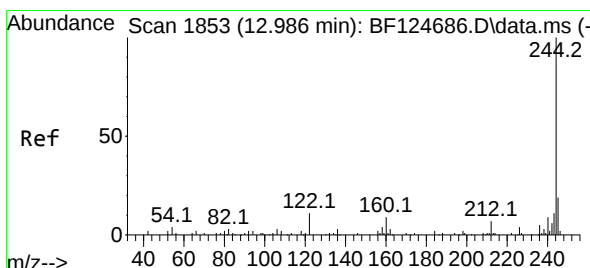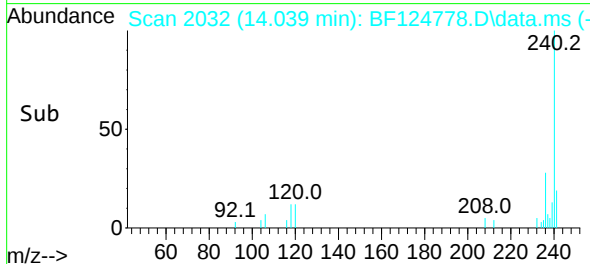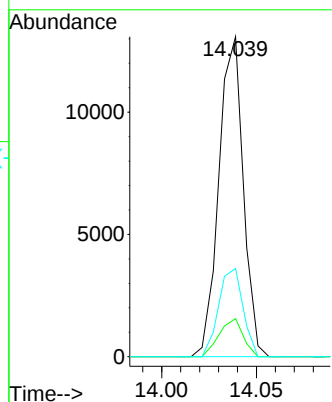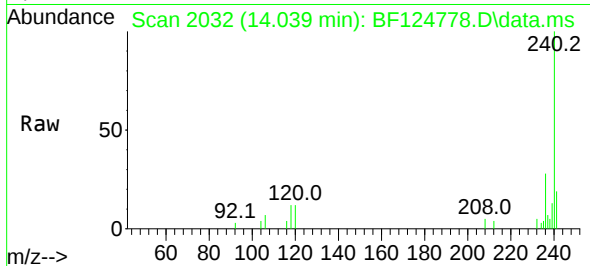

#79
Terphenyl-d14
Concen: 59.616 ng
RT: 12.986 min Scan# 1853
Delta R.T. -0.000 min
Lab File: BF124778.D
Acq: 26 Jul 2021 22:39


Tgt Ion:244 Resp: 40768
Ion Ratio Lower Upper
244 100
212 6.7 5.9 8.9
122 9.2 9.0 13.4

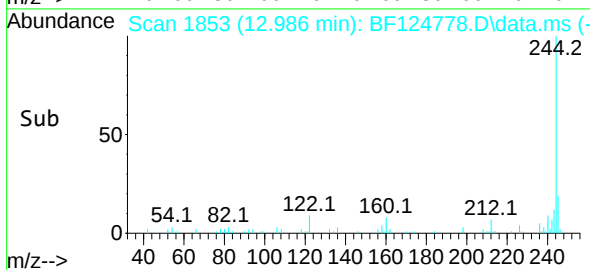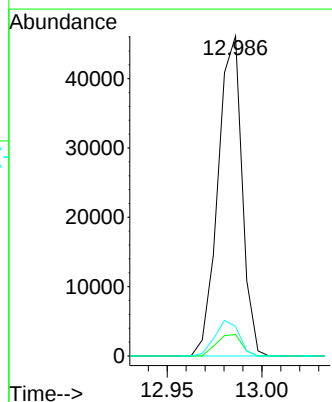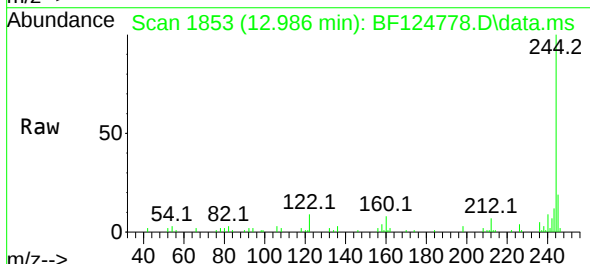



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.515 min Scan# 2283
 Delta R.T. 0.006 min
 Lab File: BF124778.D
 Acq: 26 Jul 2021 22:39

Instrument :
 BNA_F
 ClientSampleId :
 COMP-3

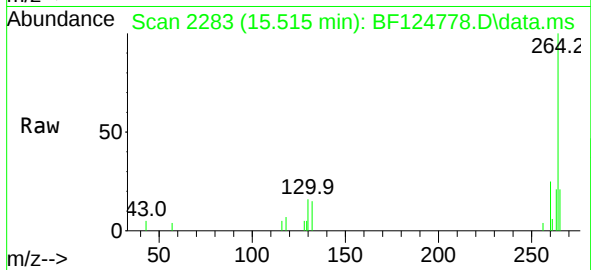

Tgt Ion:	264	Resp:	9353
Ion Ratio	Lower	Upper	
264	100		
260	24.7	19.6	29.4
265	21.3	17.2	25.8

