
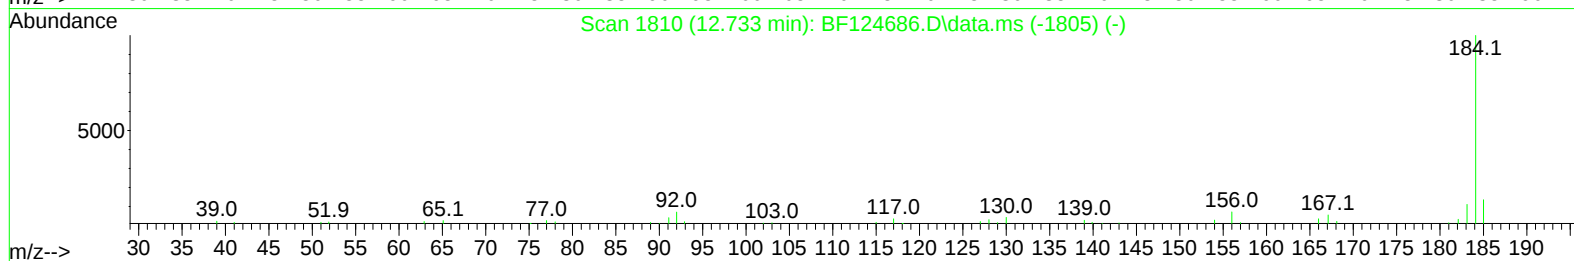
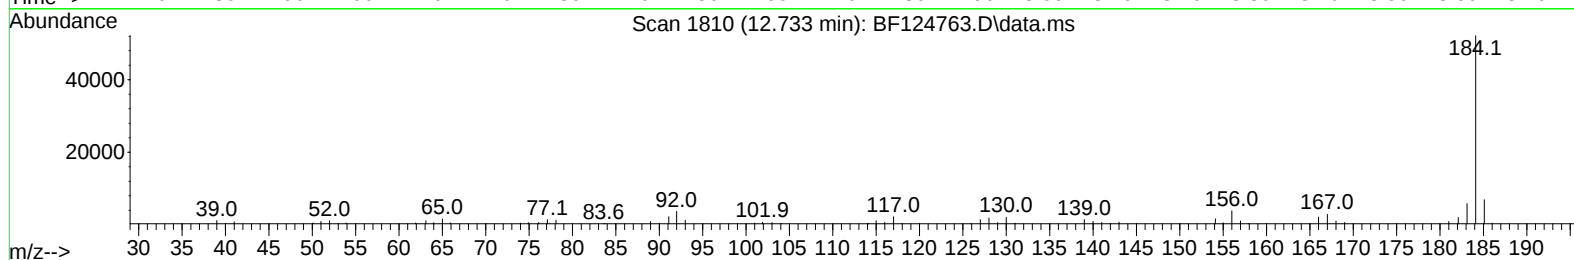


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124763.D
Acq On : 26 Jul 2021 13:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 14:59:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

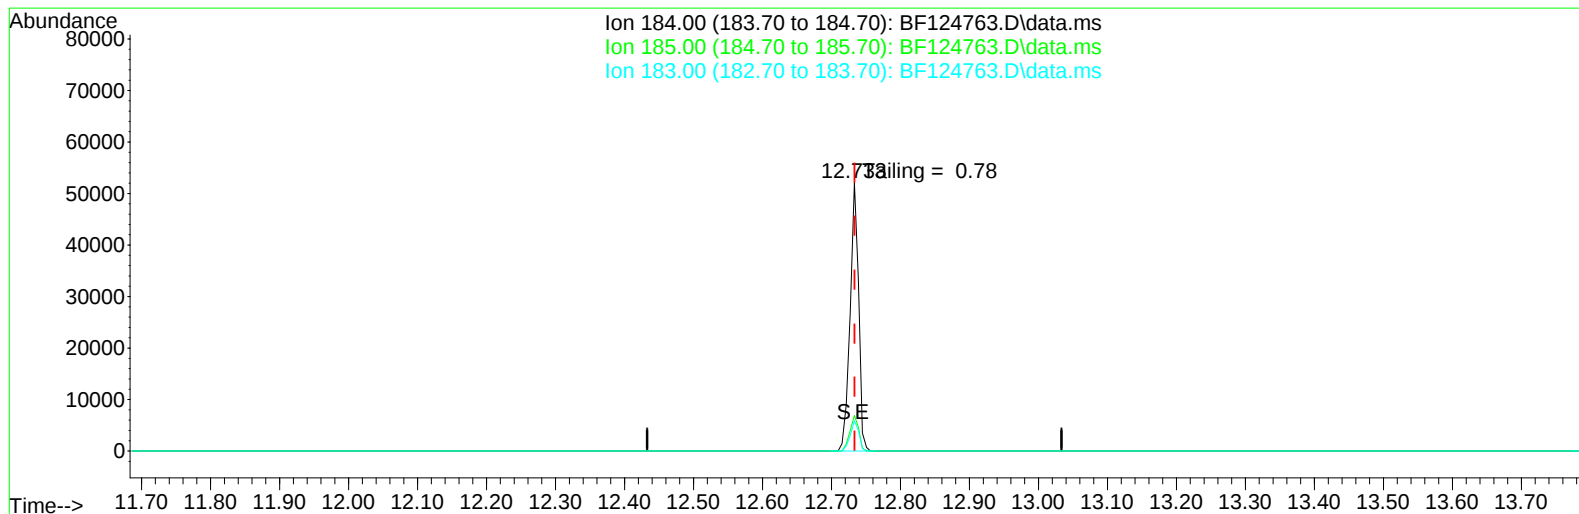

TIC: BF124763.D\data.ms

(77) Benzidine




12.733min (-0.000) 0.00 ng

response 44727

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.30
183.00	10.10	11.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124763.D
Acq On : 26 Jul 2021 13:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 14:59:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

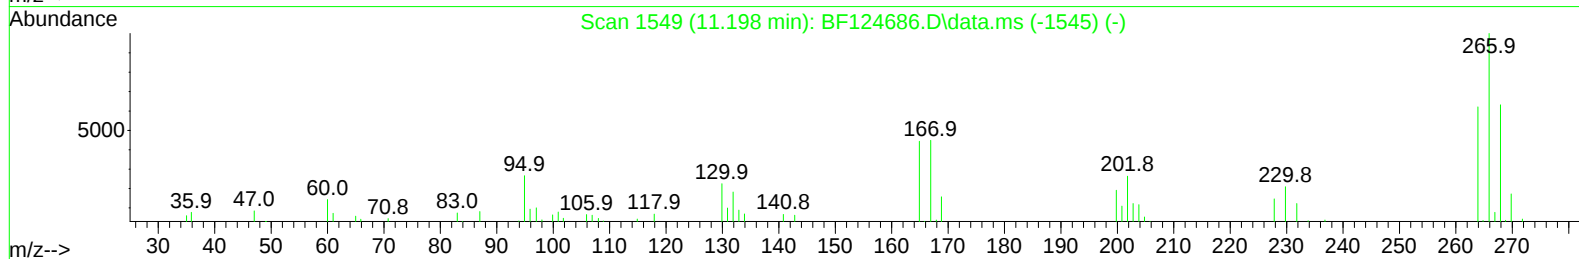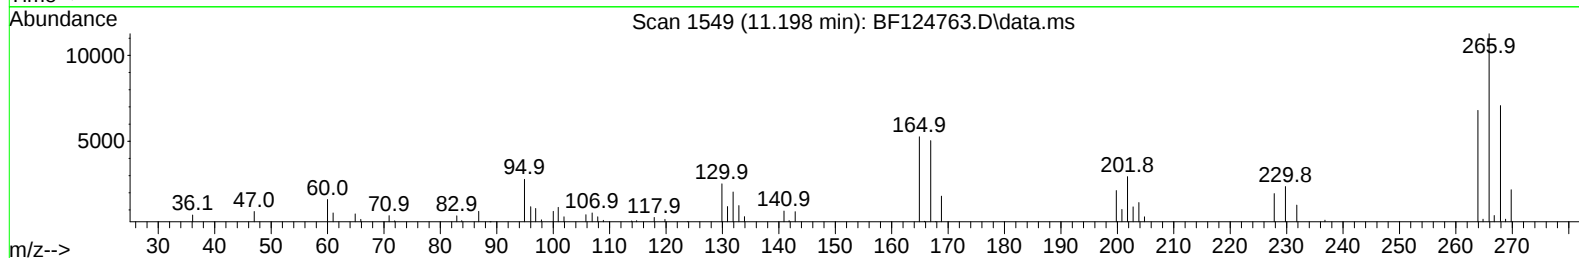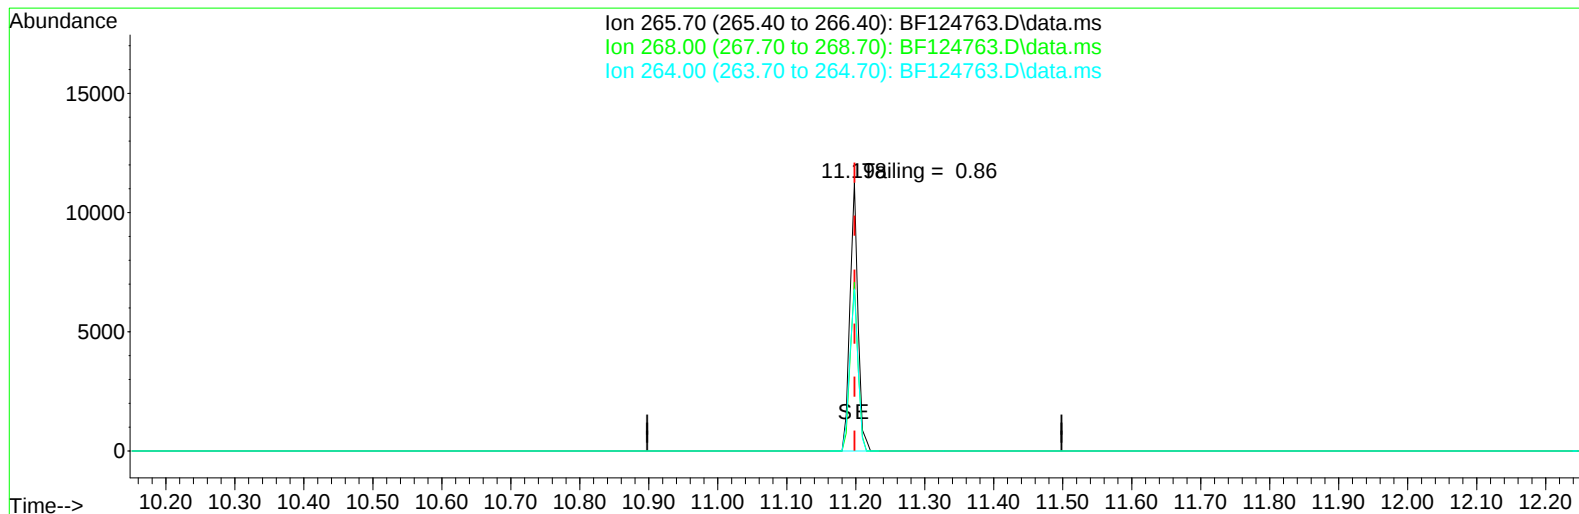

TIC: BF124763.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 0.00 ng

response 9104

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.84
264.00	69.90	60.40
0.00	0.00	0.00