

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
 Data File : BF124759.D
 Acq On : 26 Jul 2021 10:44
 Operator : JU/CG
 Sample : PB137879BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137879BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.134	515	518	523	rBB	3117	4128	1.21%	0.221%
2	5.504	575	581	584	rBB	242373	243206	71.11%	13.013%
3	6.504	745	751	753	rBB	213946	249120	72.84%	13.329%
4	6.869	810	813	816	rBB	55215	45019	13.16%	2.409%
5	7.439	904	910	912	rBB	152063	165006	48.25%	8.829%
6	8.151	1027	1031	1035	rBB	65466	60252	17.62%	3.224%
7	9.233	1209	1215	1218	rBV	337450	320422	93.69%	17.144%
8	9.910	1326	1330	1333	rBB	89761	71302	20.85%	3.815%
9	10.704	1460	1465	1468	rBV	216961	198485	58.04%	10.620%
10	11.398	1579	1583	1586	rBV	94353	71708	20.97%	3.837%
11	12.992	1848	1854	1857	rBV	346819	342003	100.00%	18.299%
12	14.033	2028	2031	2035	rBB	61867	55287	16.17%	2.958%
13	15.510	2277	2282	2286	rBV	37793	43043	12.59%	2.303%




Sum of corrected areas: 1868981

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124759.D
Acq On : 26 Jul 2021 10:44
Operator : JU/CG
Sample : PB137879BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137879BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

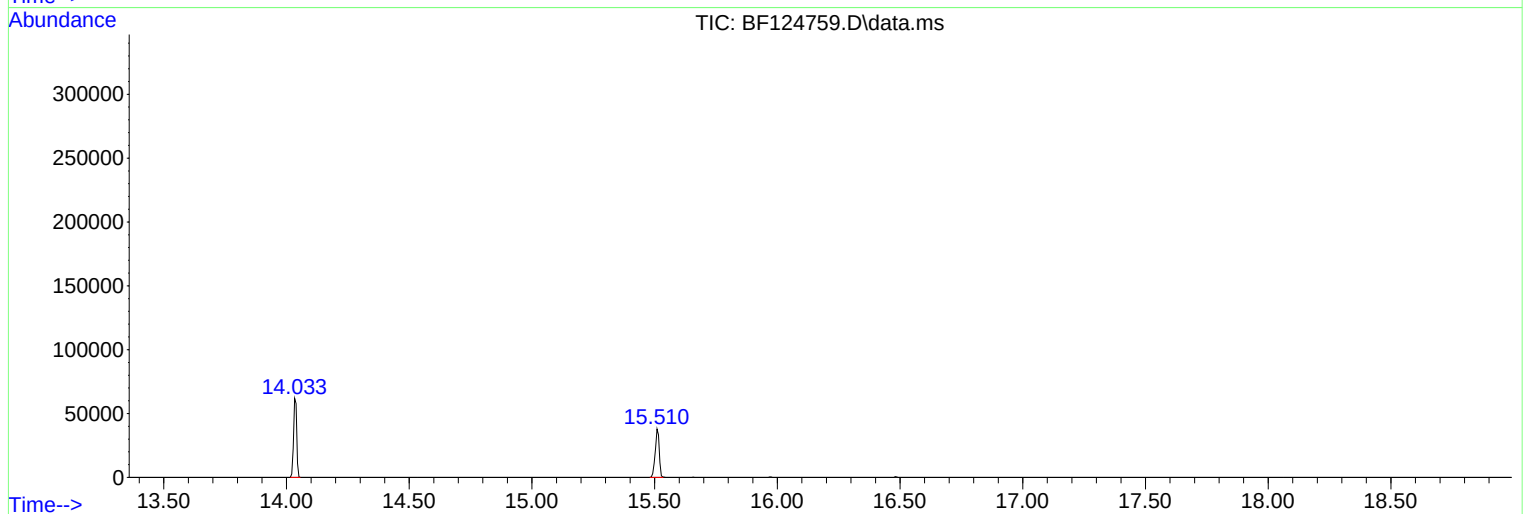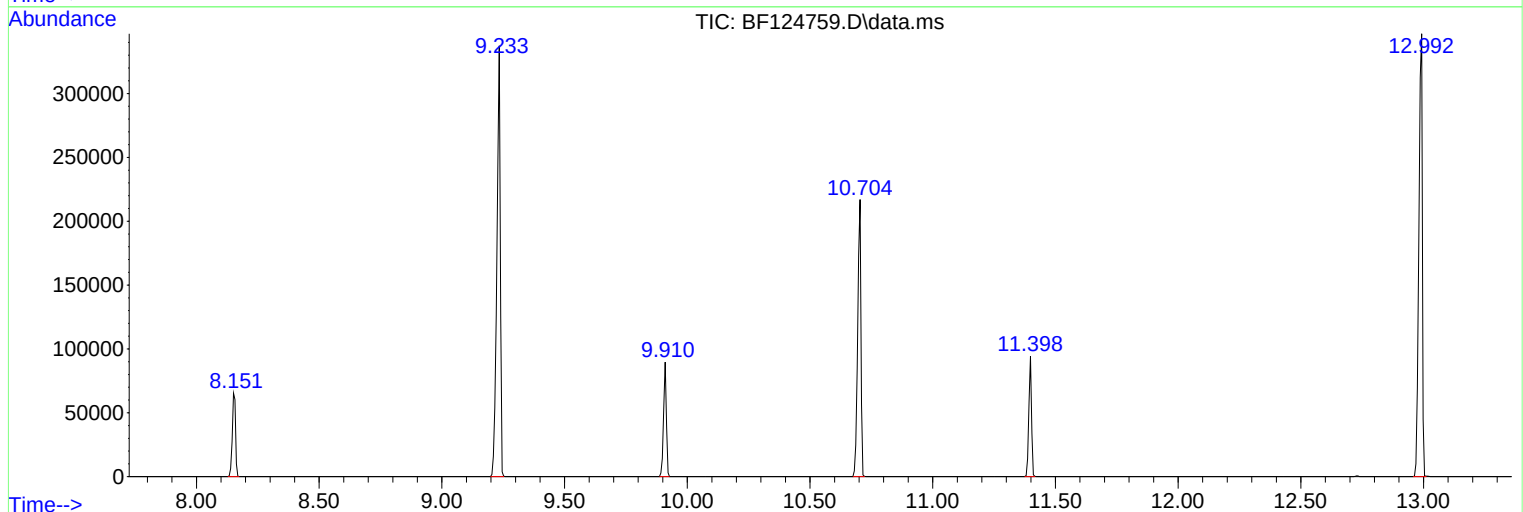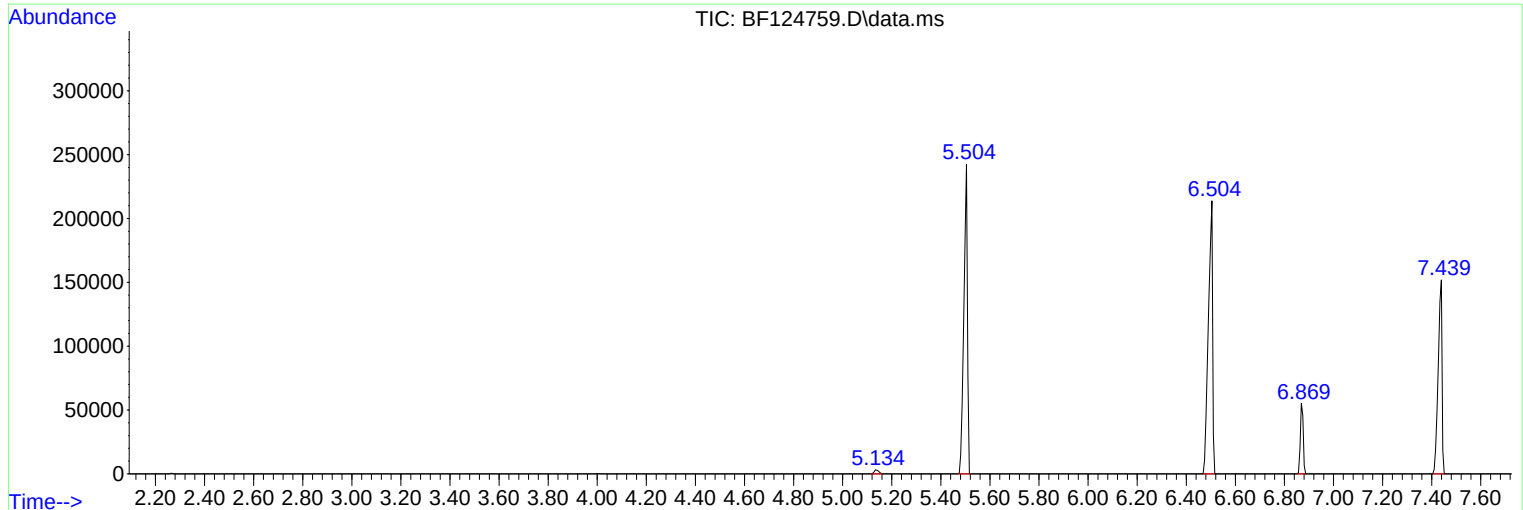

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124759.D
Acq On : 26 Jul 2021 10:44
Operator : JU/CG
Sample : PB137879BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137879BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124759.D
Acq On : 26 Jul 2021 10:44
Operator : JU/CG
Sample : PB137879BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137879BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------