

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
 Data File : BF124765.D
 Acq On : 26 Jul 2021 15:04
 Operator : JU/CG
 Sample : PB137846BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137846BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.498	575	580	583	rBB	206449	203907	69.60%	12.969%
2	6.498	744	750	753	rBB	189715	202539	69.13%	12.882%
3	6.869	810	813	816	rBB	53465	39026	13.32%	2.482%
4	7.434	904	909	912	rBB	134086	136906	46.73%	8.708%
5	8.151	1027	1031	1034	rBV	63156	52579	17.95%	3.344%
6	9.228	1209	1214	1217	rBV	267519	271668	92.73%	17.279%
7	9.910	1325	1330	1333	rBB	70777	62907	21.47%	4.001%
8	10.698	1459	1464	1467	rBV	176001	156602	53.45%	9.960%
9	11.398	1579	1583	1586	rVB	72328	64512	22.02%	4.103%
10	12.986	1848	1853	1856	rBV	310217	292971	100.00%	18.634%
11	14.033	2028	2031	2034	rBB	61782	49499	16.90%	3.148%
12	15.509	2277	2282	2286	rBB	34227	39126	13.35%	2.489%




Sum of corrected areas: 1572242

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124765.D
Acq On : 26 Jul 2021 15:04
Operator : JU/CG
Sample : PB137846BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137846BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

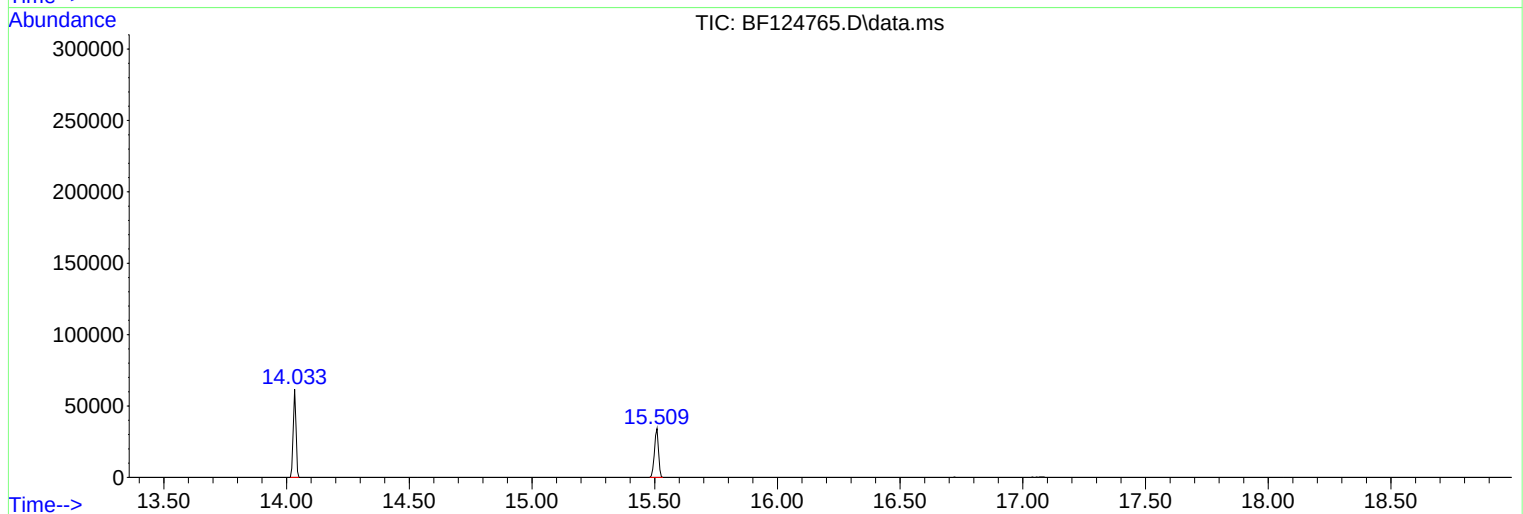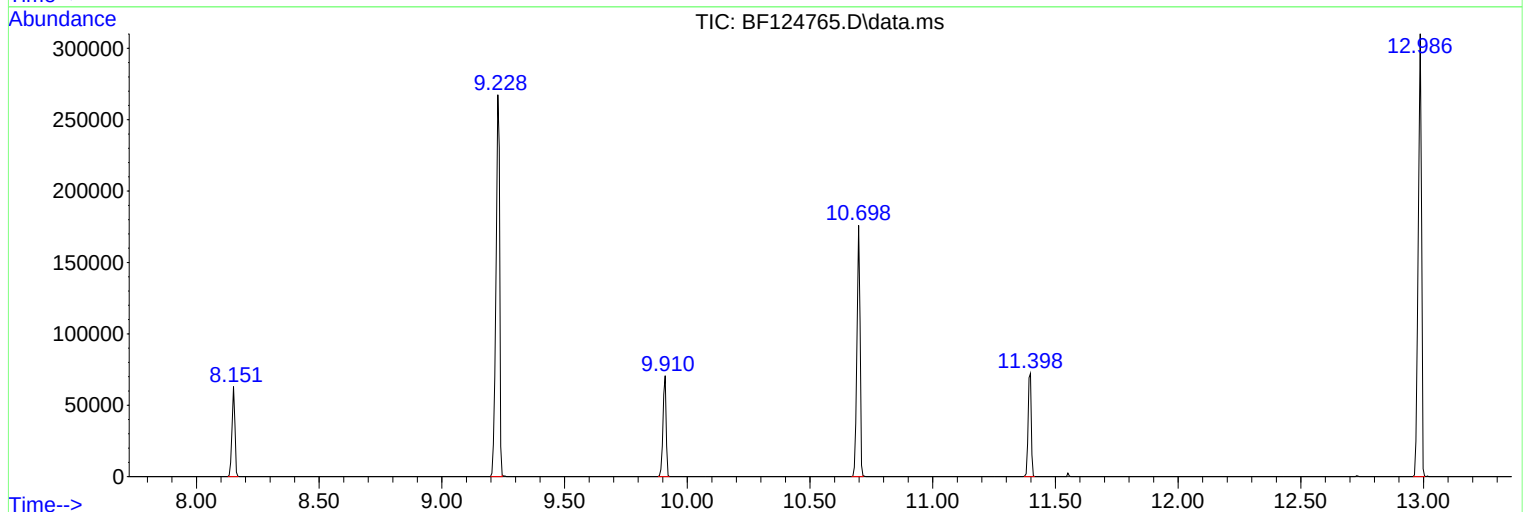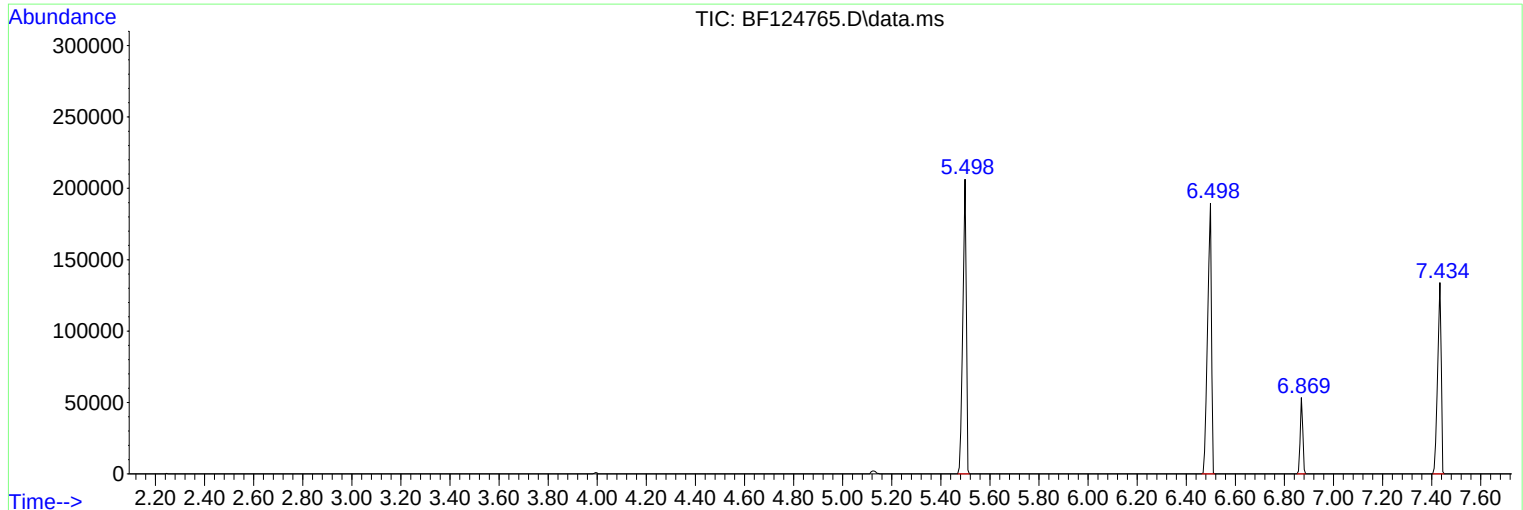

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124765.D
Acq On : 26 Jul 2021 15:04
Operator : JU/CG
Sample : PB137846BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137846BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072621\
Data File : BF124765.D
Acq On : 26 Jul 2021 15:04
Operator : JU/CG
Sample : PB137846BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137846BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------