
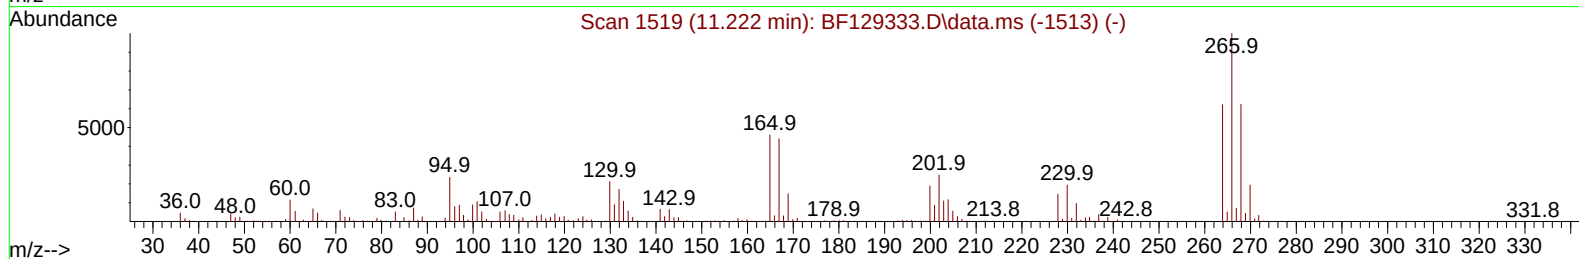
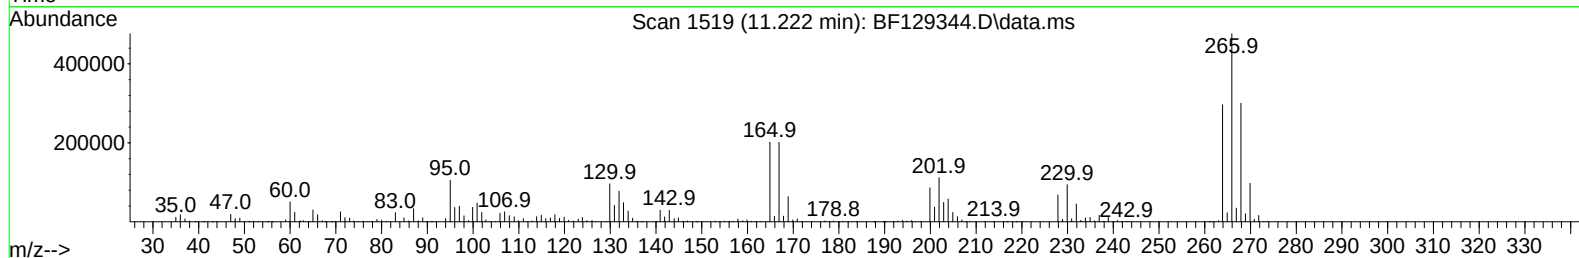


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129344.D
Acq On : 26 Jul 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 06:11:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

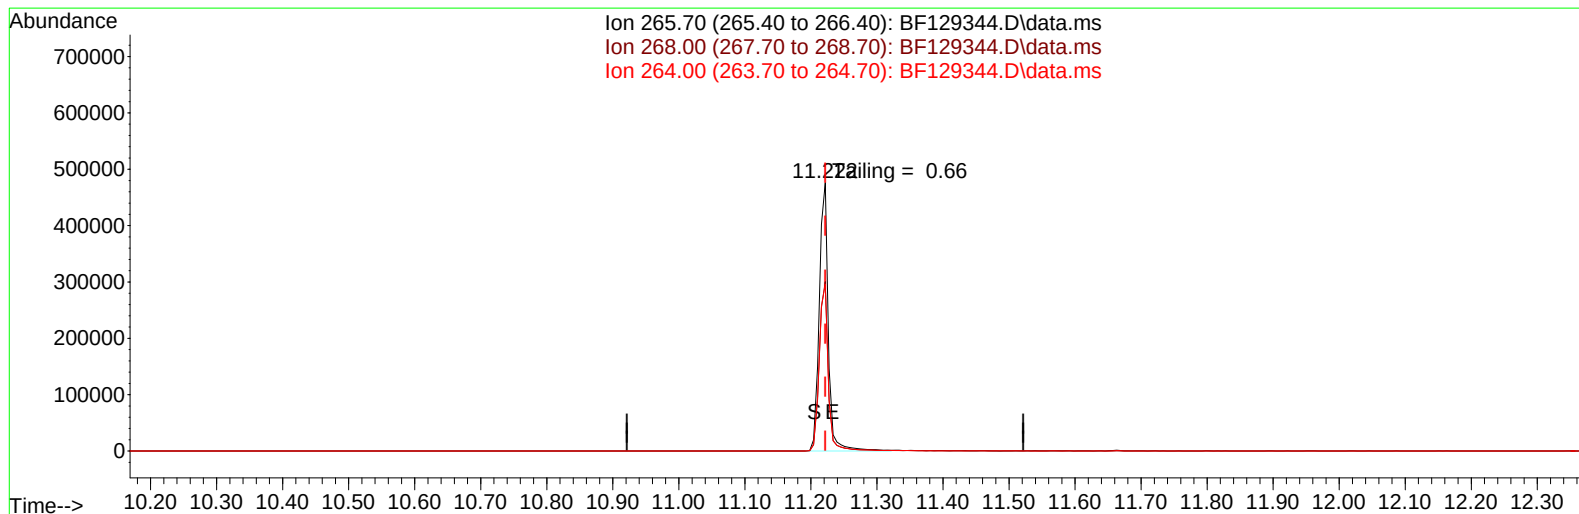

TIC: BF129344.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.000) 331843.20 ng

response 460196

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.09
264.00	61.80	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129344.D
Acq On : 26 Jul 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 06:11:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

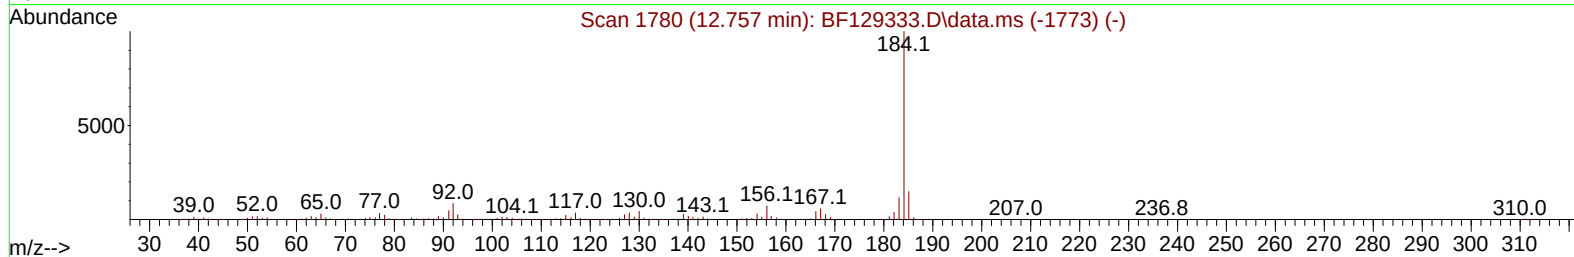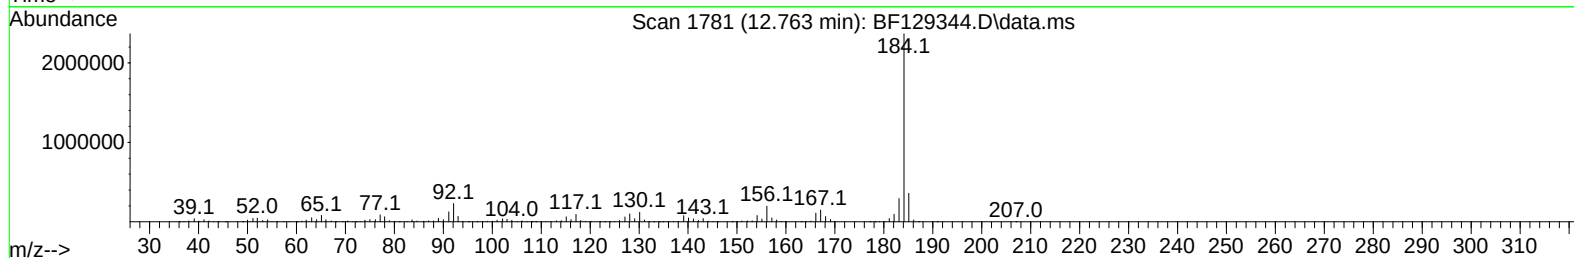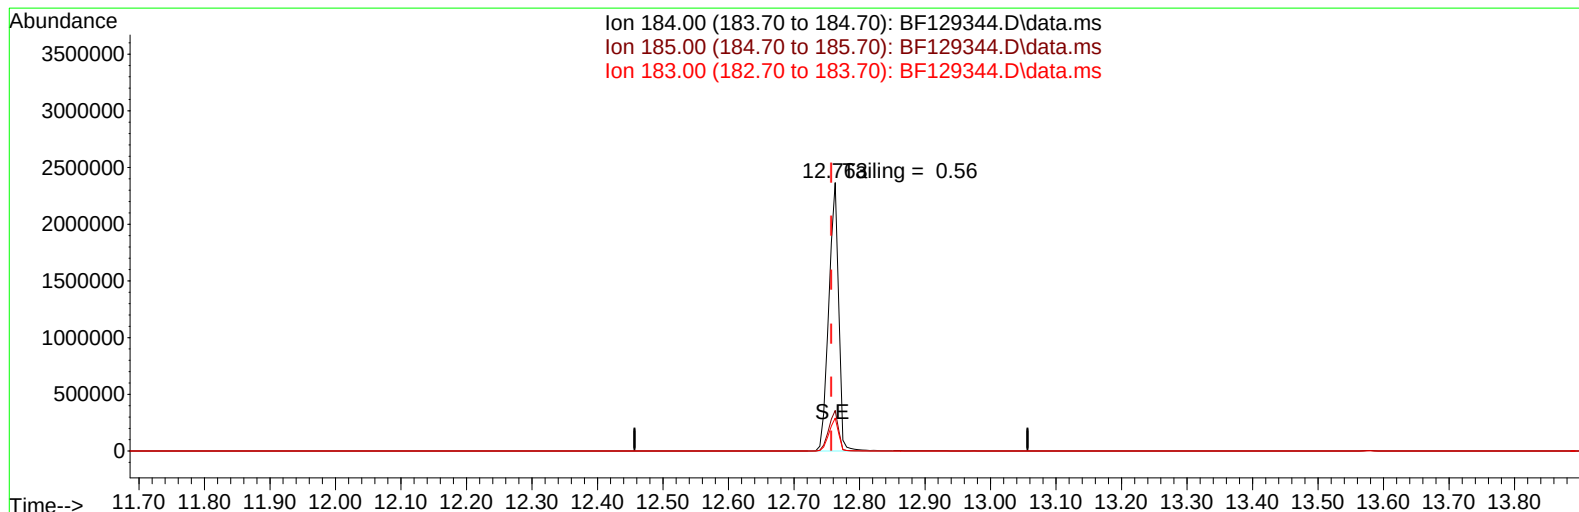

TIC: BF129344.D\data.ms

(77) Benzidine**12.763min (+ 0.006) 53831.50 ng****response 2489369**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.13
183.00	11.60	12.31
0.00	0.00	0.00