

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072622\  
 Data File : BF129352.D  
 Acq On : 26 Jul 2022 13:22  
 Operator : CG\JU  
 Sample : N3840-03  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 FIELD-DUPLICATE-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129352.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.498       | 541           | 546         | 549          | rBV      | 3229245        | 2920264       | 38.95%          | 7.687%        |
| 2         | 6.498       | 713           | 716         | 720          | rBV      | 1958306        | 1775808       | 23.69%          | 4.674%        |
| 3         | 6.881       | 777           | 781         | 785          | rBV      | 1733004        | 1354397       | 18.07%          | 3.565%        |
| 4         | 7.445       | 872           | 877         | 880          | rBV      | 4079017        | 4295121       | 57.29%          | 11.306%       |
| 5         | 8.163       | 995           | 999         | 1003         | rBV      | 2205948        | 1861683       | 24.83%          | 4.900%        |
| 6         | 9.245       | 1177          | 1183        | 1186         | rBV      | 7844492        | 7497326       | 100.00%         | 19.734%       |
| 7         | 9.922       | 1294          | 1298        | 1301         | rBV      | 2545377        | 2100671       | 28.02%          | 5.529%        |
| 8         | 9.957       | 1301          | 1304        | 1307         | rVB      | 145544         | 125805        | 1.68%           | 0.331%        |
| 9         | 10.716      | 1428          | 1433        | 1436         | rBV      | 5162507        | 4855337       | 64.76%          | 12.780%       |
| 10        | 11.410      | 1548          | 1551        | 1554         | rBV      | 2229706        | 2055644       | 27.42%          | 5.411%        |
| 11        | 11.639      | 1586          | 1590        | 1594         | rBV      | 91837          | 90551         | 1.21%           | 0.238%        |
| 12        | 11.763      | 1609          | 1611        | 1615         | rBV      | 130488         | 112535        | 1.50%           | 0.296%        |
| 13        | 13.004      | 1817          | 1822        | 1825         | rBV      | 7130857        | 6602736       | 88.07%          | 17.380%       |
| 14        | 14.057      | 1997          | 2001        | 2005         | rBV      | 1446828        | 1261639       | 16.83%          | 3.321%        |
| 15        | 15.545      | 2249          | 2254        | 2262         | rBV      | 851165         | 1081849       | 14.43%          | 2.848%        |




Sum of corrected areas: 37991366

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072622\  
Data File : BF129352.D  
Acq On : 26 Jul 2022 13:22  
Operator : CG\JU  
Sample : N3840-03  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
FIELD-DUPLICATE-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

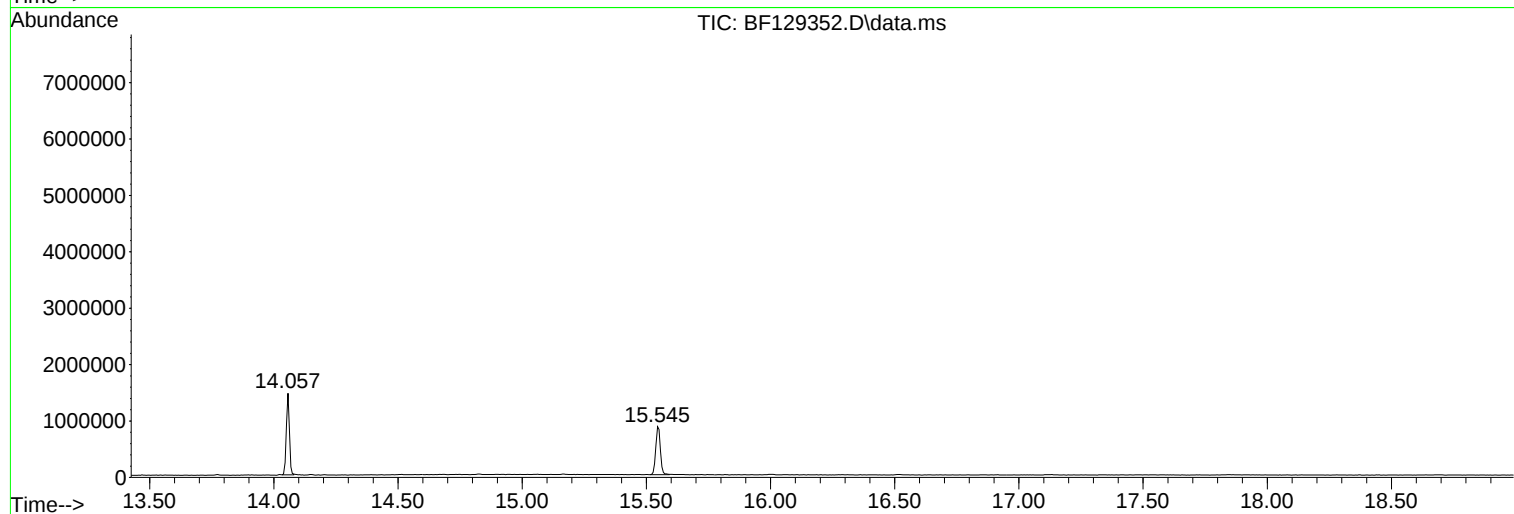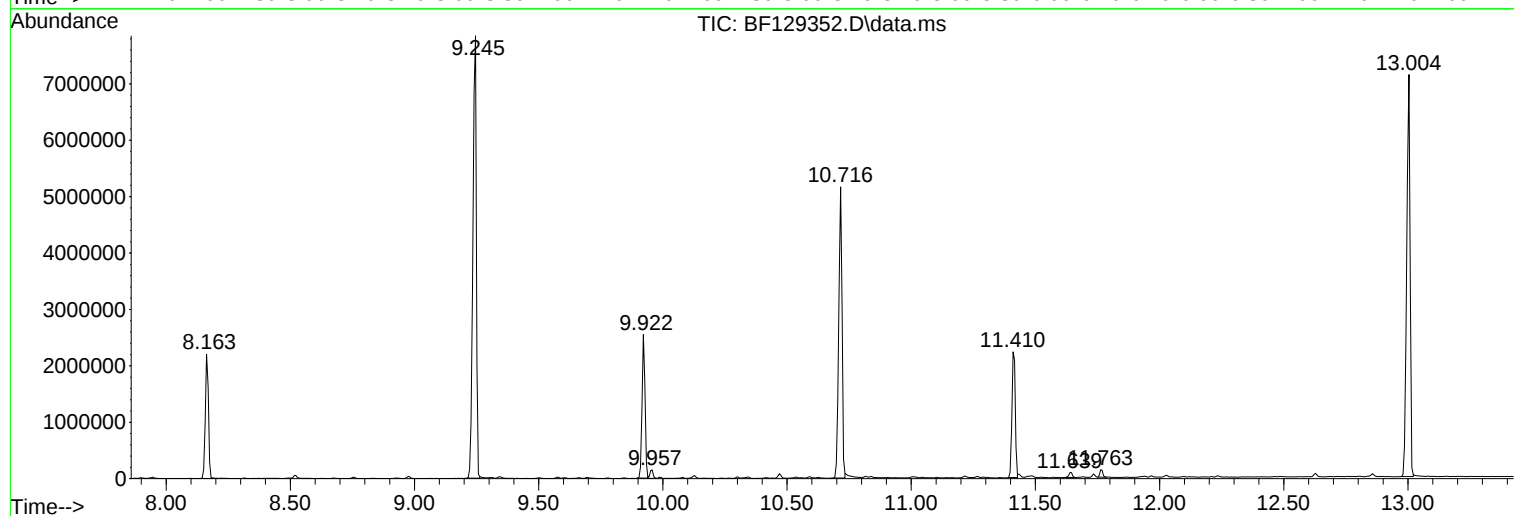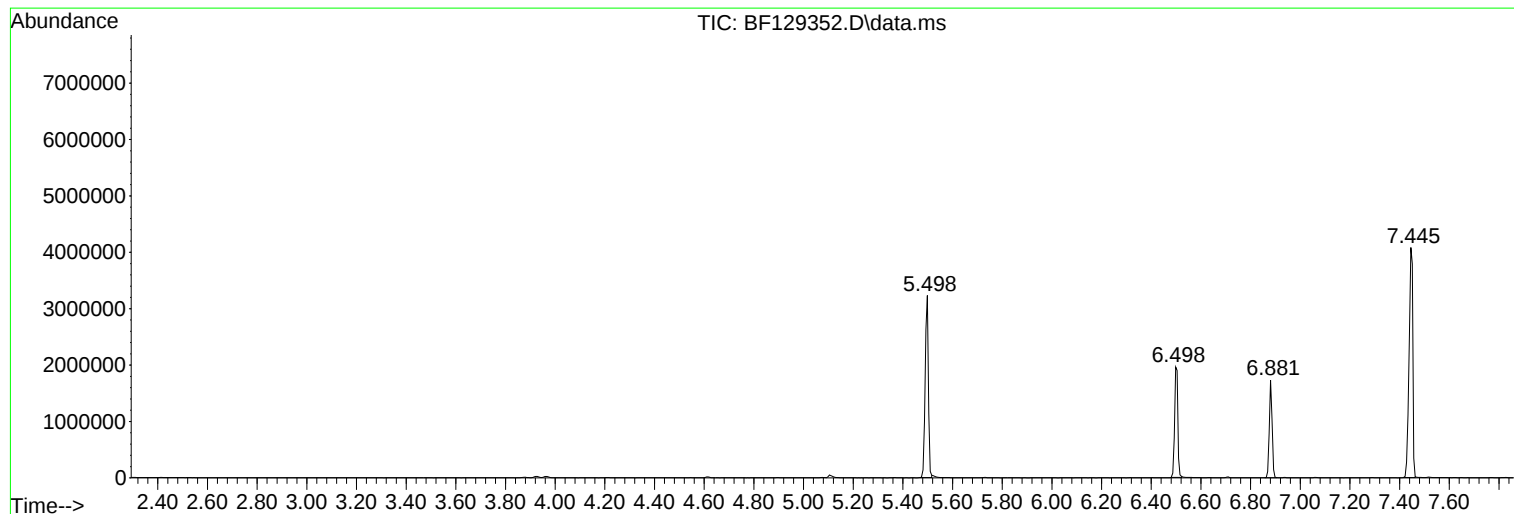

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072622\  
Data File : BF129352.D  
Acq On : 26 Jul 2022 13:22  
Operator : CG\JU  
Sample : N3840-03  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
FIELD-DUPLICATE-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072622\  
Data File : BF129352.D  
Acq On : 26 Jul 2022 13:22  
Operator : CG\JU  
Sample : N3840-03  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
FIELD-DUPLICATE-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|