

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
 Data File : BF129355.D
 Acq On : 26 Jul 2022 15:00
 Operator : CG\JU
 Sample : N3839-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ENV-DE-1-(10-15)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.122	480	482	489	rBV	50833	62387	1.03%	0.157%
2	5.504	542	547	550	rBV	5553278	5281681	86.95%	13.324%
3	6.510	712	718	721	rBV	5203452	5578456	91.84%	14.073%
4	6.881	778	781	785	rBV	1693321	1357370	22.35%	3.424%
5	7.445	872	877	880	rBV	3735851	3500630	57.63%	8.831%
6	8.163	995	999	1003	rBV	2146338	1836881	30.24%	4.634%
7	9.245	1177	1183	1186	rBV	6259139	6074375	100.00%	15.324%
8	9.922	1294	1298	1302	rBV	2520180	2073763	34.14%	5.231%
9	10.716	1428	1433	1436	rBV	4599356	4065039	66.92%	10.255%
10	10.816	1447	1450	1455	rVB	91172	83200	1.37%	0.210%
11	11.416	1548	1552	1554	rBV	2098094	1953681	32.16%	4.928%
12	11.433	1554	1555	1559	rVB	129808	92215	1.52%	0.233%
13	11.927	1634	1639	1644	rBV2	77064	118882	1.96%	0.300%
14	12.627	1755	1758	1761	rBV	211292	176818	2.91%	0.446%
15	12.857	1791	1797	1801	rBV	184251	181185	2.98%	0.457%
16	12.998	1817	1821	1825	rBV	4925054	4667340	76.84%	11.774%
17	14.057	1997	2001	2004	rBV	1244120	1066833	17.56%	2.691%
18	15.110	2176	2180	2183	rBV2	75312	107818	1.77%	0.272%
19	15.480	2240	2243	2248	rVV	50422	66665	1.10%	0.168%
20	15.545	2249	2254	2267	rVB	908228	1234362	20.32%	3.114%
21	17.045	2505	2509	2517	rVB3	31112	61037	1.00%	0.154%




Sum of corrected areas: 39640618

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129355.D
Acq On : 26 Jul 2022 15:00
Operator : CG\JU
Sample : N3839-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ENV-DE-1-(10-15)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

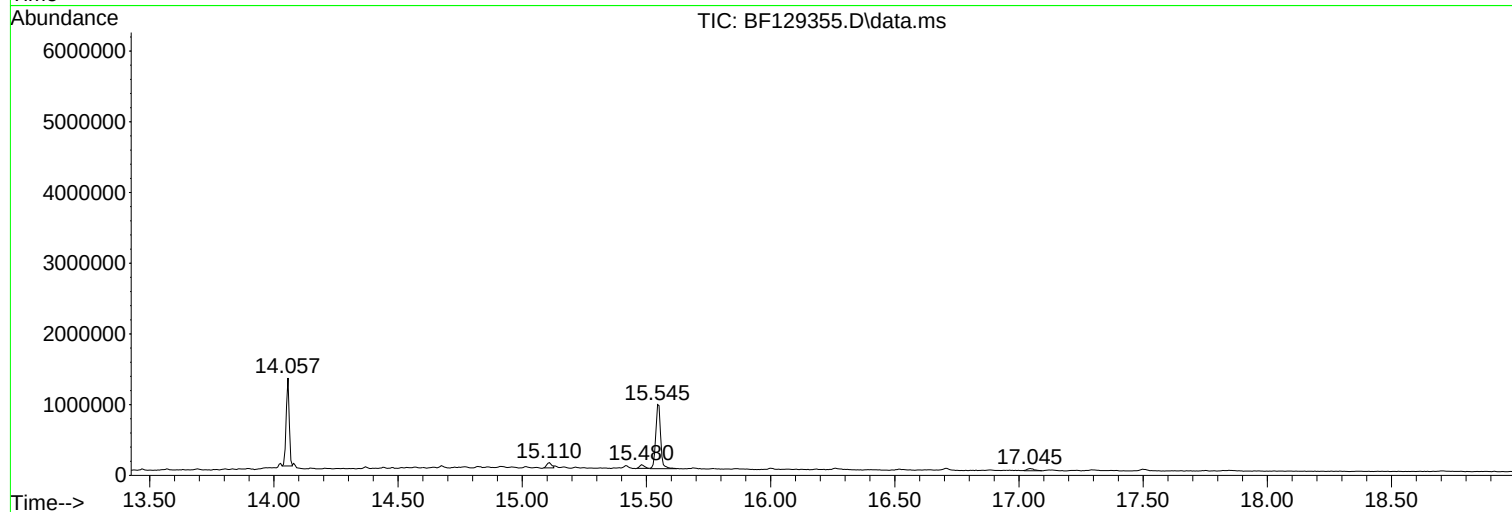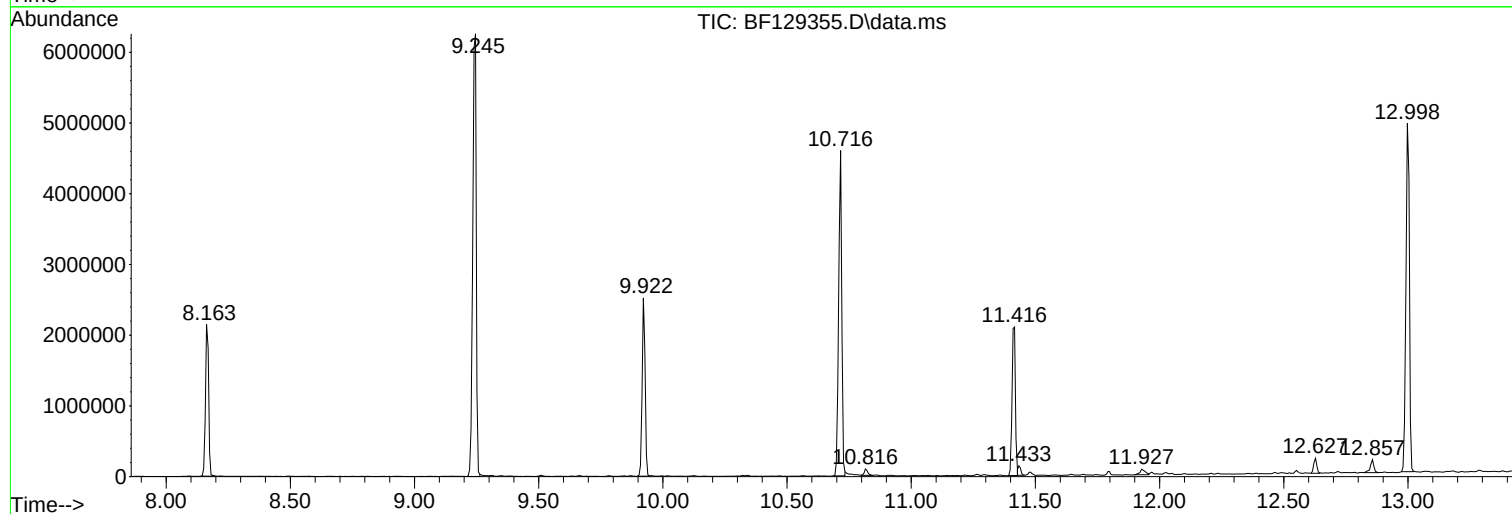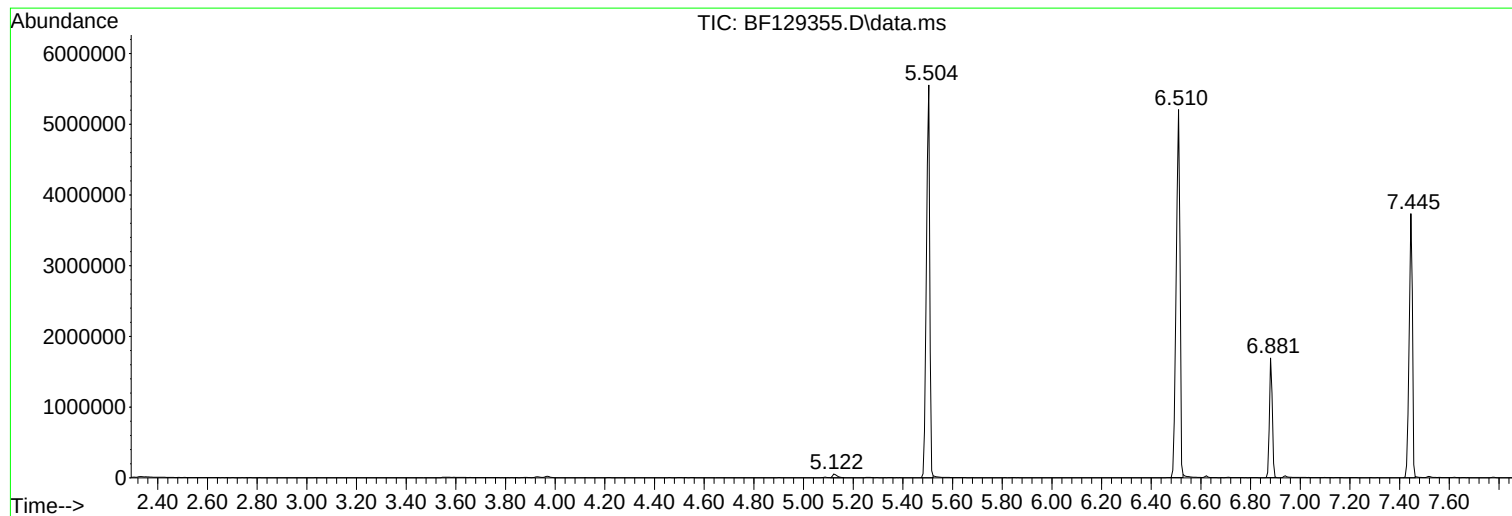

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129355.D
Acq On : 26 Jul 2022 15:00
Operator : CG\JU
Sample : N3839-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ENV-DE-1-(10-15)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129355.D
Acq On : 26 Jul 2022 15:00
Operator : CG\JU
Sample : N3839-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ENV-DE-1-(10-15)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------