

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
 Data File : BF129363.D
 Acq On : 26 Jul 2022 19:24
 Operator : CG\JU
 Sample : N3886-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WH-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	480	483	498	rVB	84136	106523	1.69%	0.269%
2	5.504	542	547	550	rBV	5623373	5885652	93.53%	14.878%
3	6.510	713	718	721	rBV	5172314	5885015	93.52%	14.877%
4	6.881	778	781	785	rBV	1680005	1311345	20.84%	3.315%
5	7.445	872	877	880	rBV	3895990	3851093	61.20%	9.735%
6	8.163	995	999	1003	rBV	2093321	1711742	27.20%	4.327%
7	9.239	1177	1182	1186	rBV	6668986	6293026	100.00%	15.908%
8	9.922	1294	1298	1301	rBV	2234267	1760093	27.97%	4.449%
9	10.716	1428	1433	1436	rBV	3473281	3427649	54.47%	8.665%
10	11.410	1547	1551	1554	rBV	1806983	1474777	23.44%	3.728%
11	11.433	1554	1555	1558	rVB	188588	107852	1.71%	0.273%
12	11.792	1613	1616	1619	rBV	94655	79041	1.26%	0.200%
13	11.927	1634	1639	1644	rBV2	62724	129462	2.06%	0.327%
14	12.627	1755	1758	1761	rVB	232641	191356	3.04%	0.484%
15	12.857	1791	1797	1800	rBV	207493	220507	3.50%	0.557%
16	12.998	1817	1821	1824	rBV	4528036	3961354	62.95%	10.014%
17	14.057	1996	2001	2004	rBV	1301235	1281651	20.37%	3.240%
18	14.080	2004	2005	2010	rVB	137294	90066	1.43%	0.228%
19	15.104	2176	2179	2182	rBV2	91080	127203	2.02%	0.322%
20	15.162	2186	2189	2196	rVB2	55999	77331	1.23%	0.195%
21	15.415	2229	2232	2237	rVB	69925	90372	1.44%	0.228%
22	15.480	2240	2243	2248	rVV	71708	99118	1.58%	0.251%
23	15.545	2249	2254	2267	rVB	1009474	1332535	21.17%	3.369%
24	15.998	2328	2331	2335	rVB2	49168	63604	1.01%	0.161%




Sum of corrected areas: 39558367

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129363.D
Acq On : 26 Jul 2022 19:24
Operator : CG\JU
Sample : N3886-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WH-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

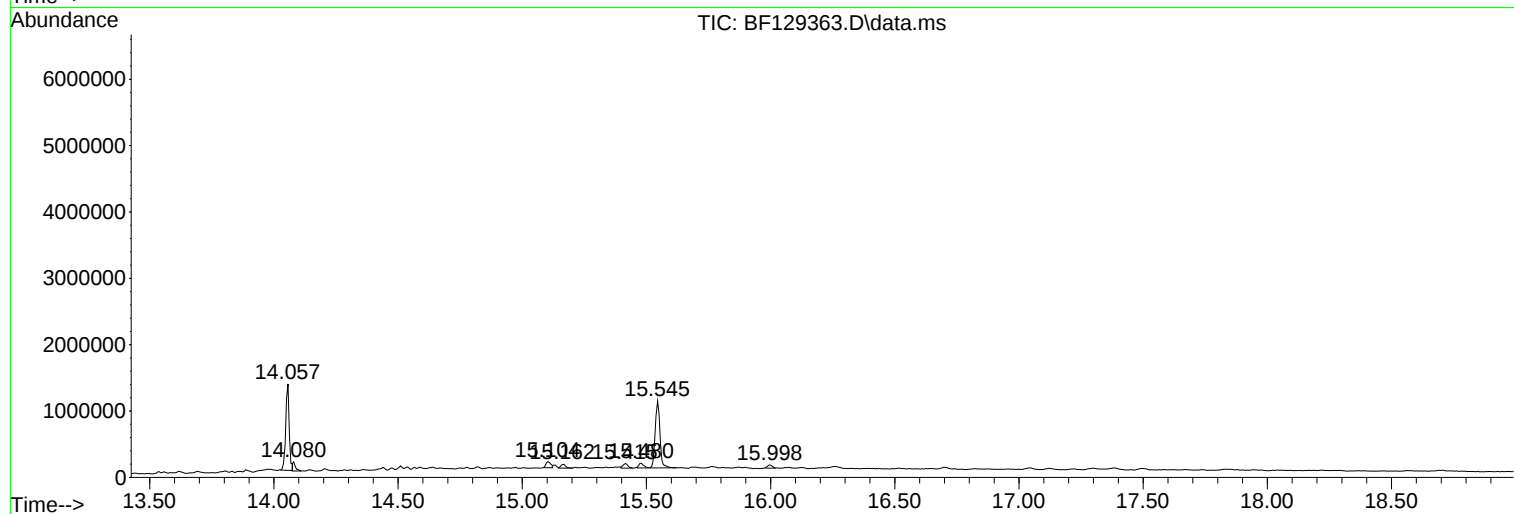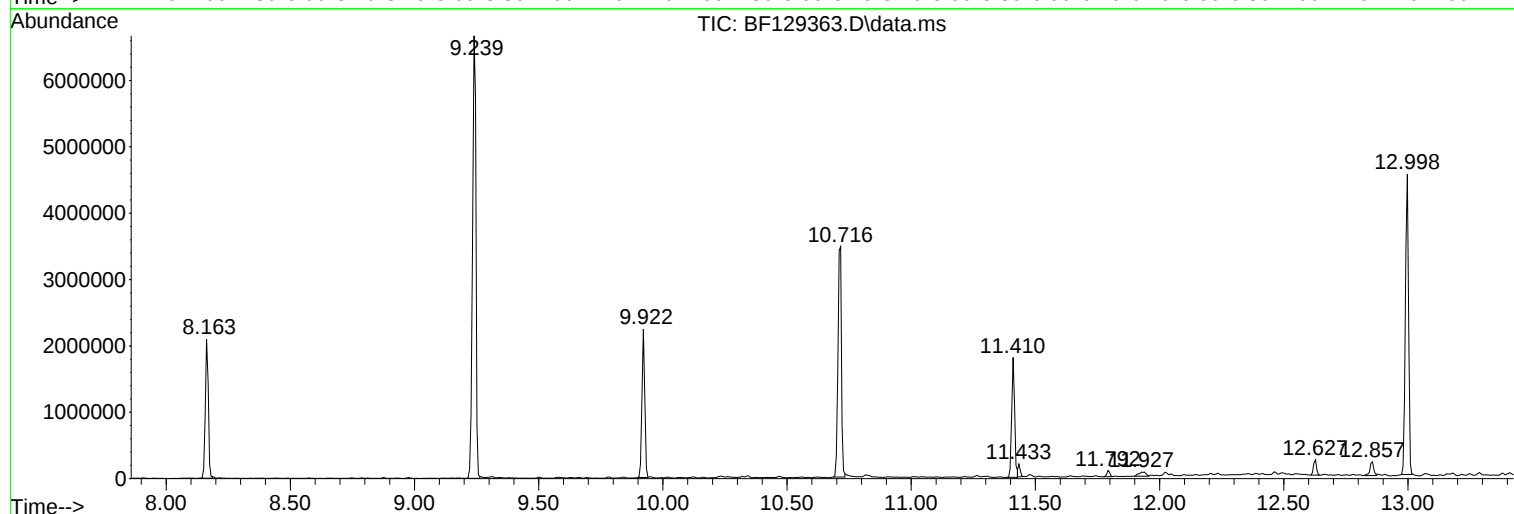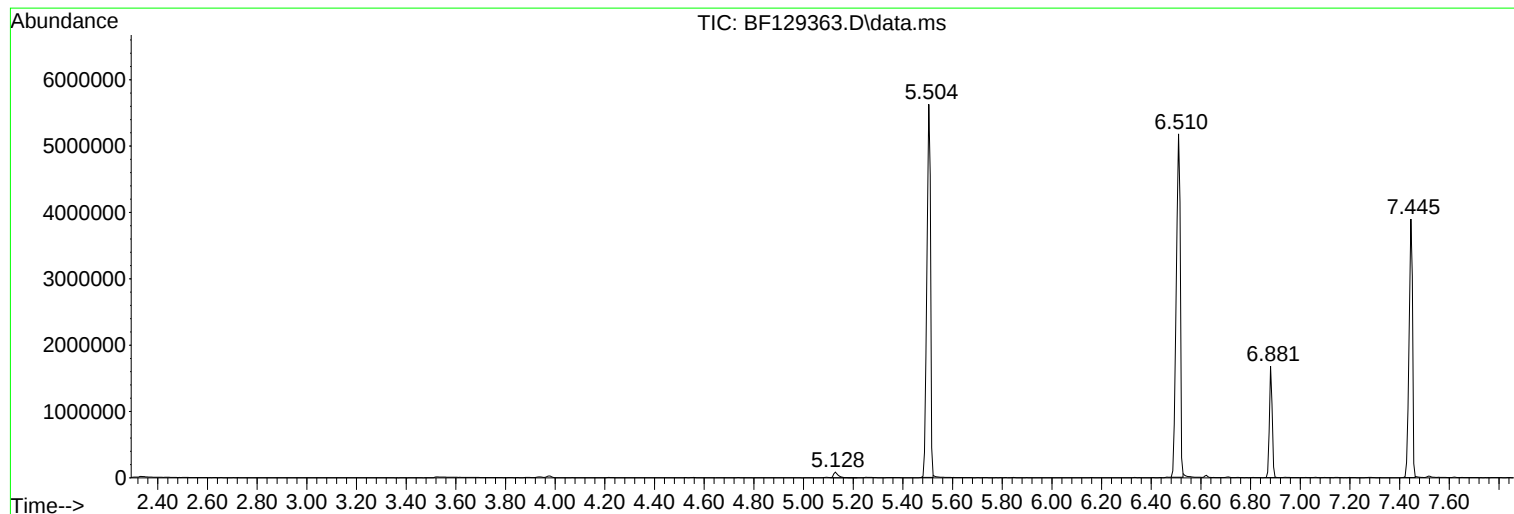

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129363.D
Acq On : 26 Jul 2022 19:24
Operator : CG\JU
Sample : N3886-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WH-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129363.D
Acq On : 26 Jul 2022 19:24
Operator : CG\JU
Sample : N3886-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WH-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------