


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
 Data File : BF129344.D
 Acq On : 26 Jul 2022 08:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 25 17:24:17 2022

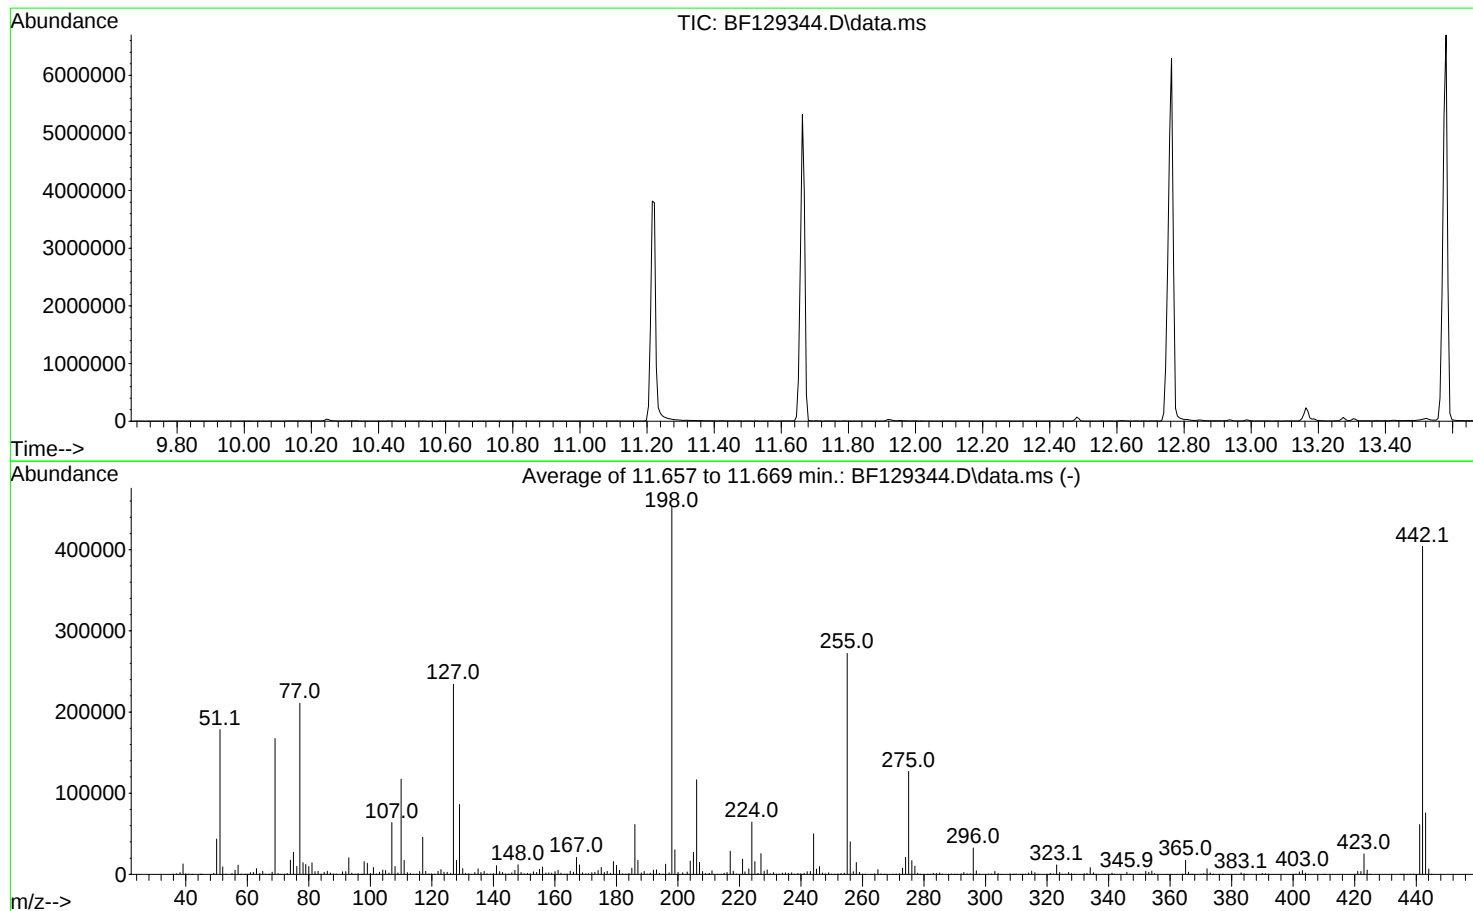




AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	178499	PASS
68	69	0.00	2	1.7	2820	PASS
69	198	0.00	100	36.9	167453	PASS
70	69	0.00	2	0.6	943	PASS
127	198	10	80	51.7	234432	PASS
197	198	0.00	2	0.4	1918	PASS
198	198	100	100	100.0	453227	PASS
199	198	5	9	6.6	30128	PASS
275	198	10	60	28.0	126893	PASS
365	198	1	100	3.8	17401	PASS
441	198	0.01	100	13.5	61283	PASS
442	442	50	100	100.0	404053	PASS
443	442	15	24	18.8	75765	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
 Data File : BF129344.D
 Acq On : 26 Jul 2022 08:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 27 06:11:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 17:24:17 2022
 Response via : Initial Calibration

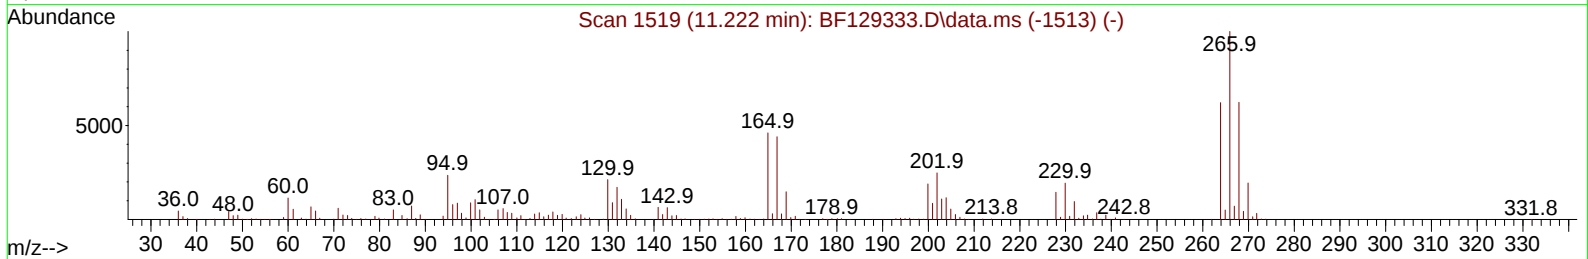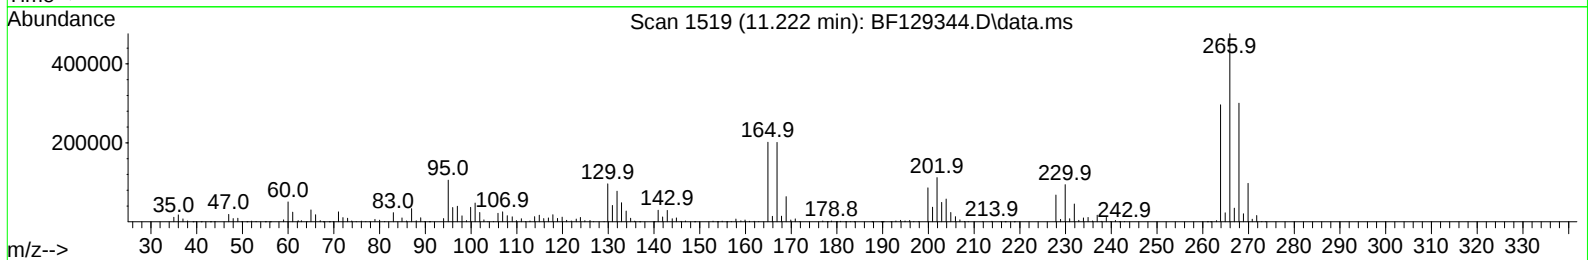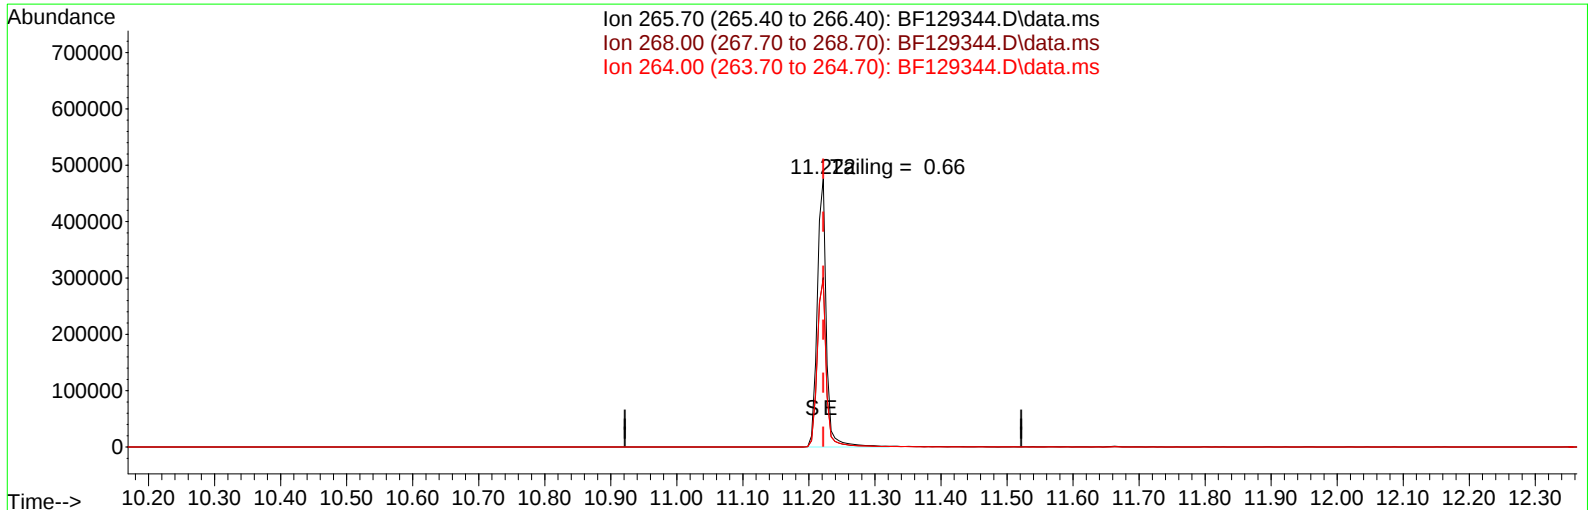

TIC: BF129344.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 331843.20 ng




response 460196

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.09
264.00	61.80	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072622\
Data File : BF129344.D
Acq On : 26 Jul 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 27 06:11:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 17:24:17 2022
Response via : Initial Calibration

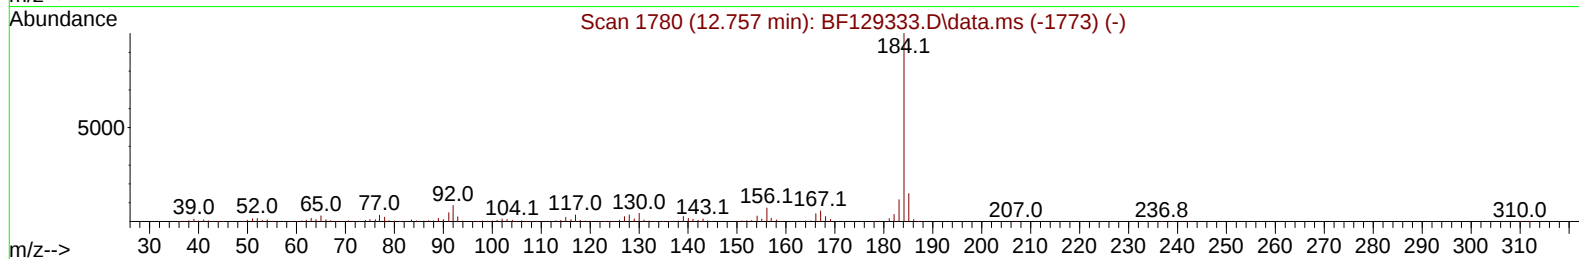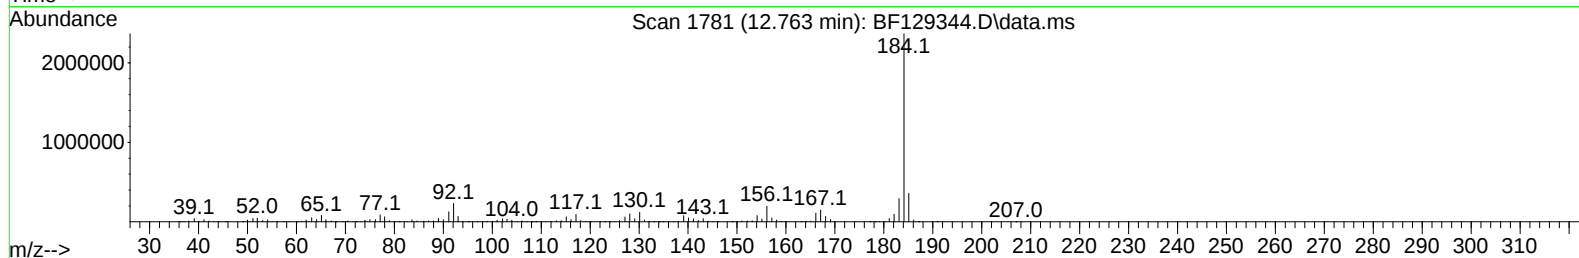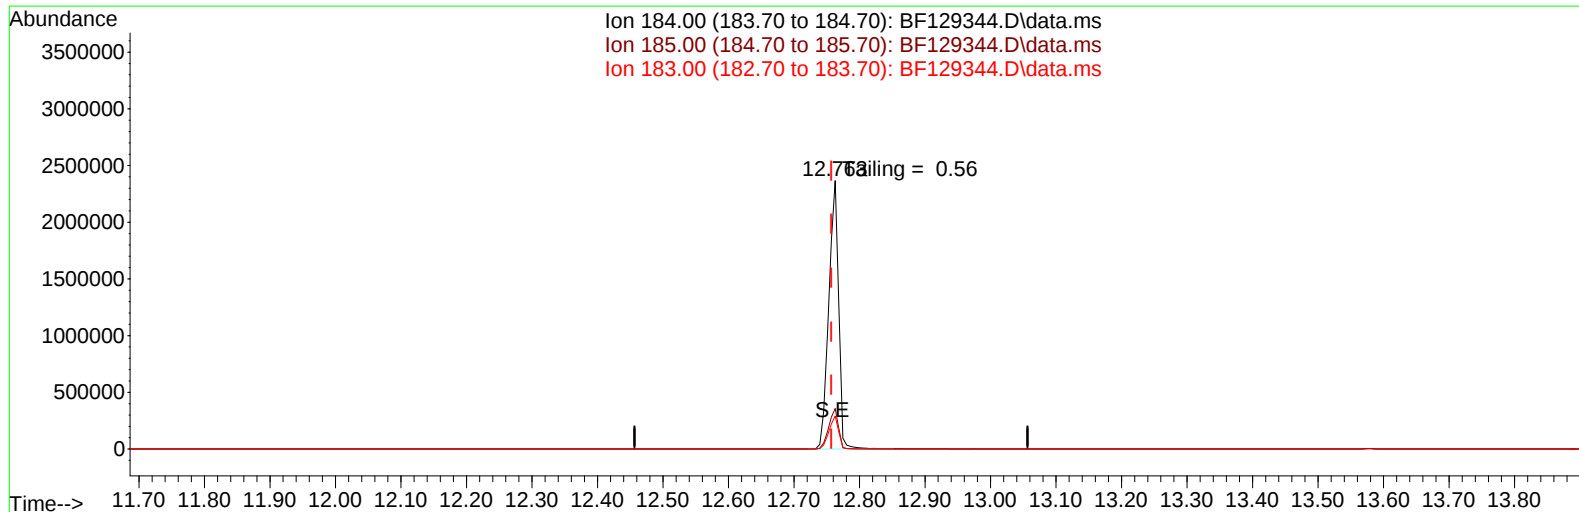

TIC: BF129344.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 53831.50 ng

response 2489369

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.13
183.00	11.60	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/26/2022	BNA_F	<u>BF129344.D</u>
Compound Name	Response	Retention Time
DDT	1135141	13.58
DDD	15536	13.275
DDE	1950	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17486	1152627	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP