

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072715\
 Data File : BF080688.D
 Acq On : 28 Jul 2015 00:04
 Operator : TP/UM
 Sample : PB84659BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB84659BL

Quant Time: Jul 28 07:55:13 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 28 05:06:30 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.92	152	30821	20.00	ng	0.00
21) Naphthalene-d8	8.21	136	104631	20.00	ng	0.00
38) Acenaphthene-d10	9.96	164	53989	20.00	ng	0.00
63) Phenanthrene-d10	11.45	188	93783	20.00	ng	0.00
75) Chrysene-d12	14.17	240	61678	20.00	ng	-0.08
86) Perylene-d12	15.76	264	38115	20.00	ng	-0.16
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	249333	128.84	ng	0.00
7) Phenol-d6	6.53	99	292428	140.45	ng	0.00
23) Nitrobenzene-d5	7.48	82	196780	96.63	ng	0.00
41) 2,4,6-Tribromophenol	10.75	330	63803	135.02	ng	0.00
44) 2-Fluorobiphenyl	9.29	172	336344	78.50	ng	0.00
78) Terphenyl-d14	13.05	244	301189	83.65	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072715\
Data File : BF080688.D
Acq On : 28 Jul 2015 00:04
Operator : TP/UM
Sample : PB84659BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB84659BL

Quant Time: Jul 28 07:55:13 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 28 05:06:30 2015
Response via : Initial Calibration

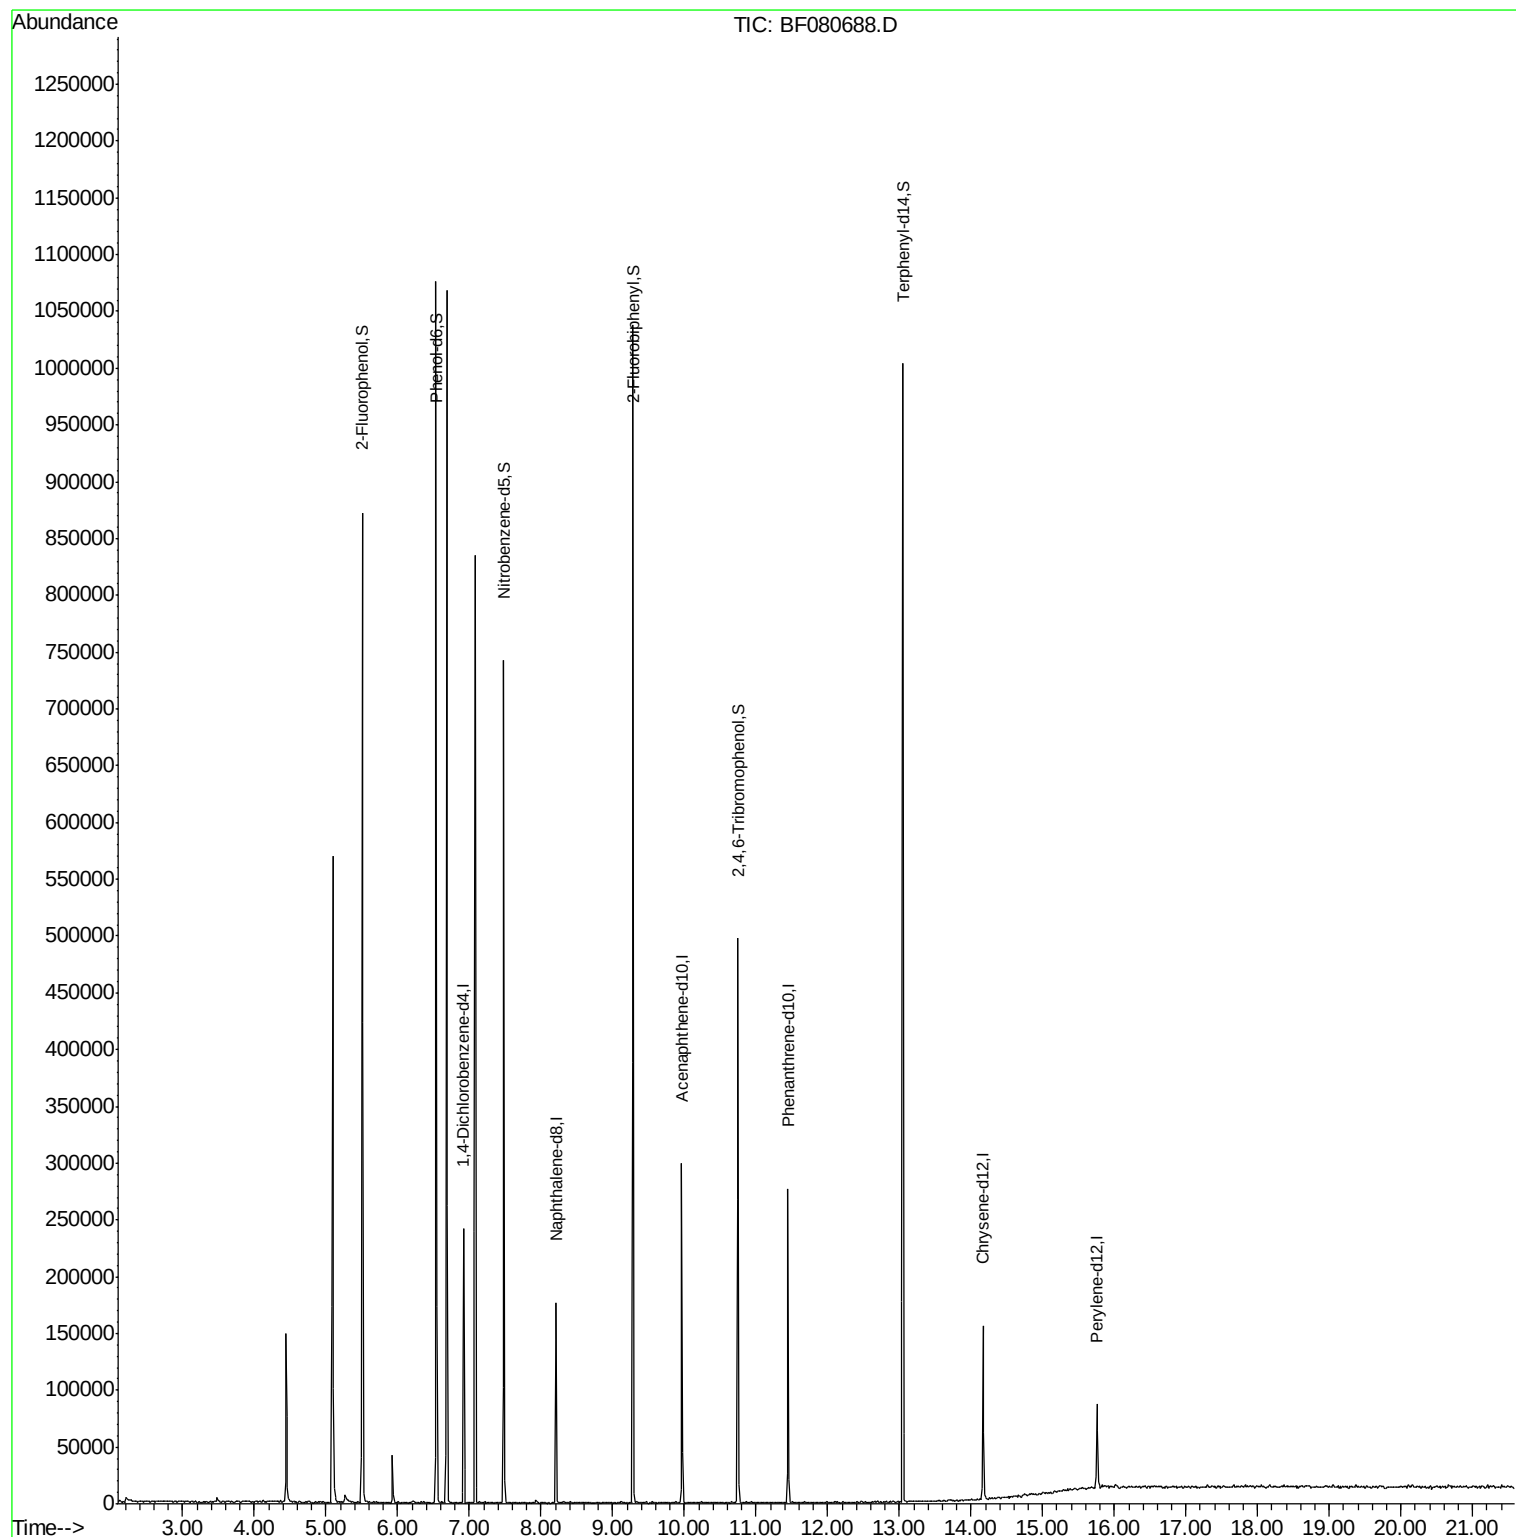

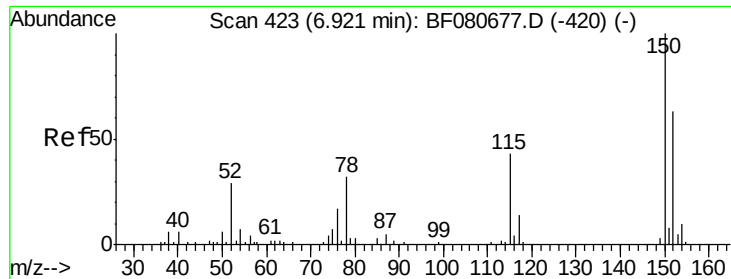


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.92 min Scan# 423
Delta R.T. 0.00 min
Lab File: BF080688.D
Acq: 28 Jul 2015 00:04

Instrument :
BNA_F
ClientSampleId :
PB84659BL

Tot Ion:152 Resp: 30821
Ion Ratio Lower Upper
152 100
150 156.0 127.7 191.5
115 69.6 54.2 81.4

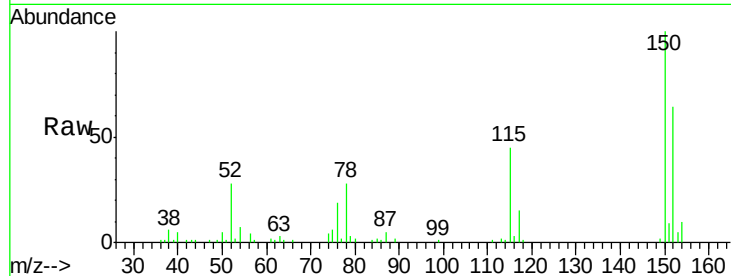


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

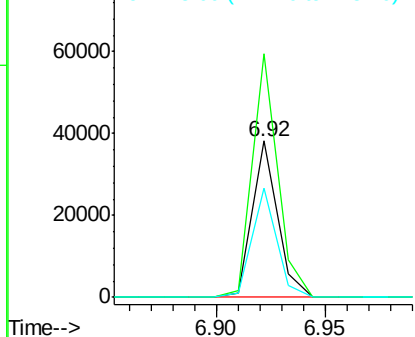



#5


2-Fluorophenol
Concen: 128.84 ng
RT: 5.50 min Scan# 299
Delta R.T. 0.00 min
Lab File: BF080688.D
Acq: 28 Jul 2015 00:04

Tgt Ion:112 Resp: 249333
Ion Ratio Lower Upper
112 100
64 70.1 53.2 79.8
63 39.4 30.4 45.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

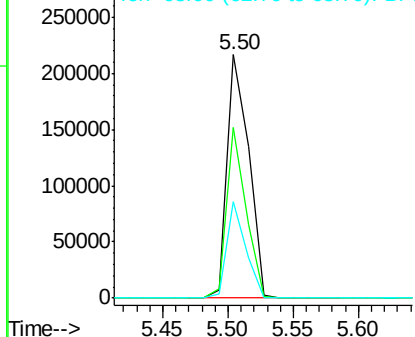

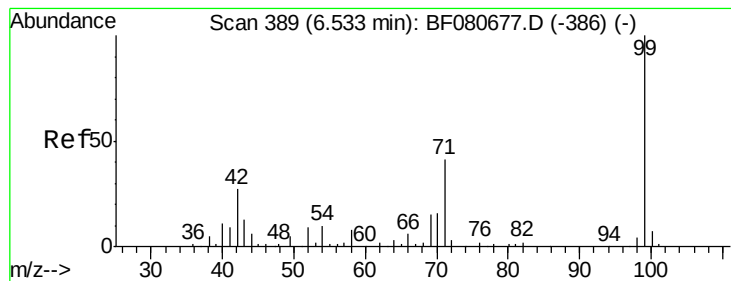

#7

Phenol-d6

Concen: 140.45 ng

RT: 6.53 min Scan# 389

Delta R.T. 0.00 min

Lab File: BF080688.D

Acq: 28 Jul 2015 00:04

Instrument :

BNA_F

ClientSampleId :

PB84659BL


Tot Ion: 99 Resp: 292428

Ion Ratio Lower Upper

99 100

42 26.0 21.8 32.8




71 40.2 32.9 49.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

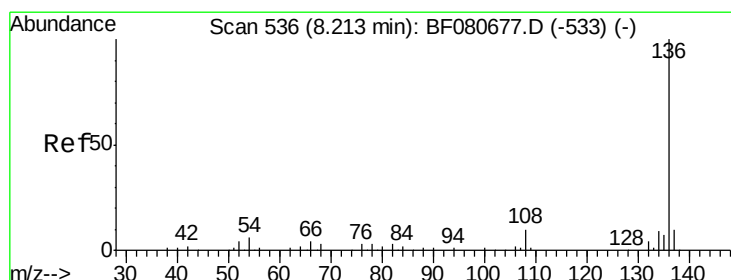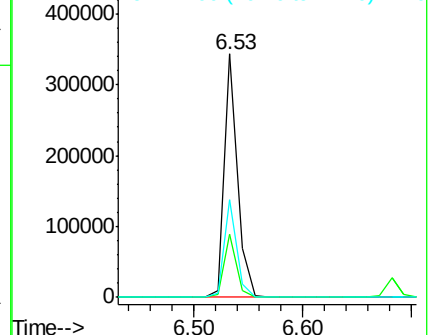

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.21 min Scan# 536

Delta R.T. 0.00 min

Lab File: BF080688.D

Acq: 28 Jul 2015 00:04

Tgt Ion: 136 Resp: 104631


Ion Ratio Lower Upper

136 100

137 10.3 8.2 12.2

54 6.0 5.0 7.4

68 3.7 2.7 4.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

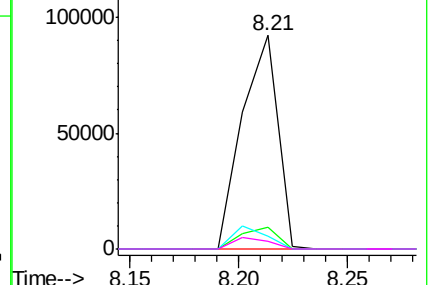



#23

Nitrobenzene-d5

Concen: 96.63 ng

RT: 7.48 min Scan# 472

Delta R.T. 0.00 min

Lab File: BF080688.D

Acq: 28 Jul 2015 00:04

Instrument :

BNA_F

ClientSampleId :

PB84659BL


Tot Ion: 82 Resp: 196780

Ion Ratio Lower Upper




82 100

128 43.1 33.7 50.5

54 55.0 47.3 70.9

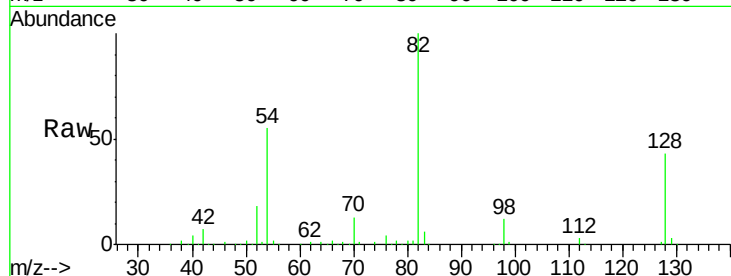

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

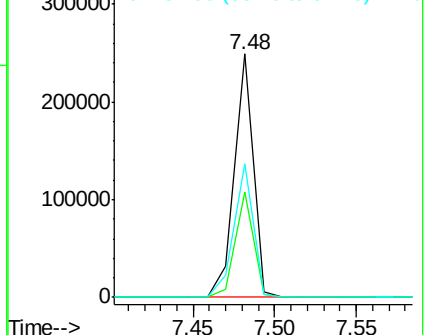

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.96 min Scan# 689

Delta R.T. 0.00 min

Lab File: BF080688.D

Acq: 28 Jul 2015 00:04


Tgt Ion:164 Resp: 53989

Ion Ratio Lower Upper



164 100


162 102.3 82.0 123.0

160 45.4 36.7 55.1



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

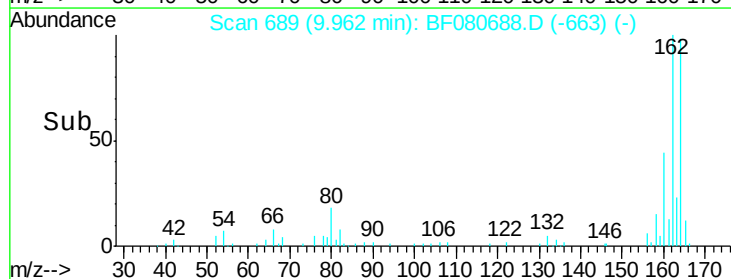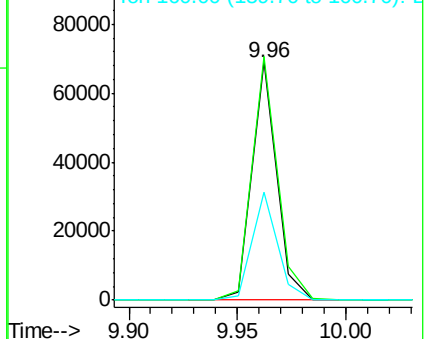







#41
 2,4,6-Tribromophenol
 Concen: 135.02 ng
 RT: 10.75 min Scan# 758
 Delta R.T. 0.00 min
 Lab File: BF080688.D
 Acq: 28 Jul 2015 00:04

Instrument :
 BNA_F
 ClientSampleId :
 PB84659BL

Tot Ion:330 Resp: 63803
 Ion Ratio Lower Upper
 330 100
 332 96.3 76.9 115.3
 141 38.2 30.6 45.8

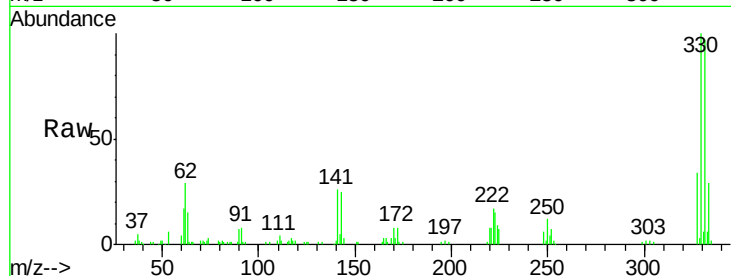


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


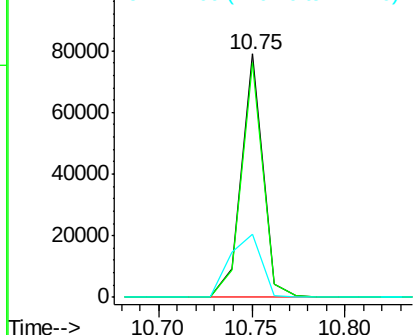



#44
 2-Fluorobiphenyl
 Concen: 78.50 ng
 RT: 9.29 min Scan# 630
 Delta R.T. 0.00 min
 Lab File: BF080688.D
 Acq: 28 Jul 2015 00:04

Tgt Ion:172 Resp: 336344
 Ion Ratio Lower Upper
 172 100
 171 35.4 26.6 39.8
 170 24.5 18.6 28.0



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

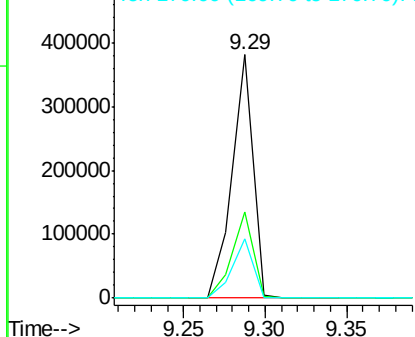







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.45 min Scan# 819
Delta R.T. 0.00 min
Lab File: BF080688.D
Acq: 28 Jul 2015 00:04

Instrument :
BNA_F
ClientSampleId :
PB84659BL

Tot Ion:188 Resp: 93783
Ion Ratio Lower Upper
188 100
94 8.1 7.2 10.8
80 8.4 8.2 12.2

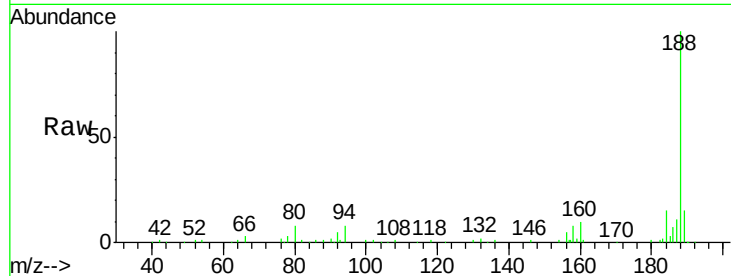


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

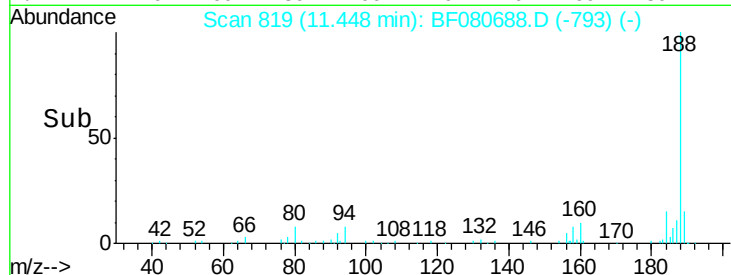
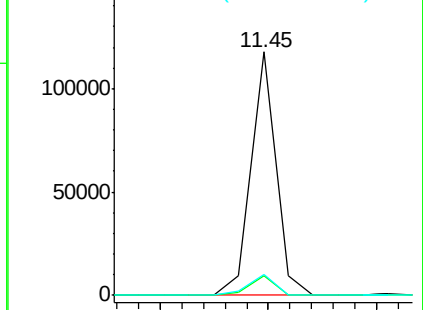



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.17 min Scan# 1057
Delta R.T. -0.08 min
Lab File: BF080688.D
Acq: 28 Jul 2015 00:04

Tgt Ion:240 Resp: 61678
Ion Ratio Lower Upper
240 100
120 12.4 8.0 12.0#
236 24.3 20.0 30.0

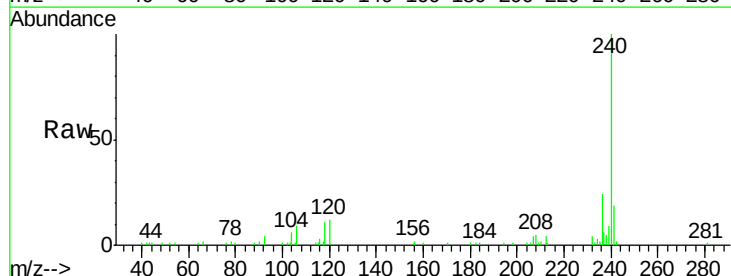

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



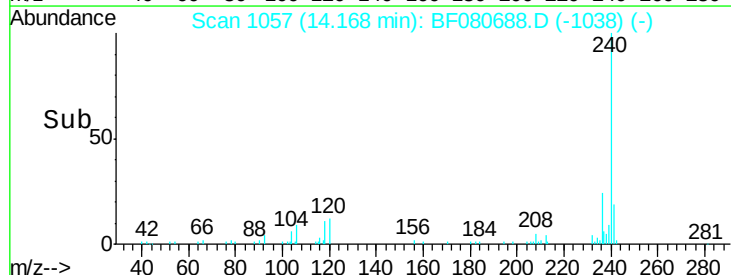
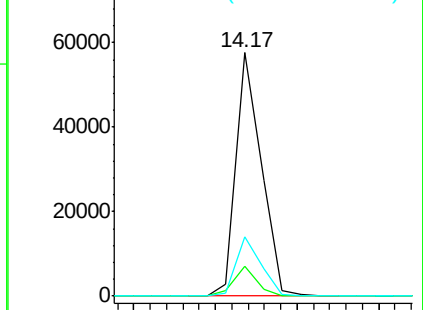


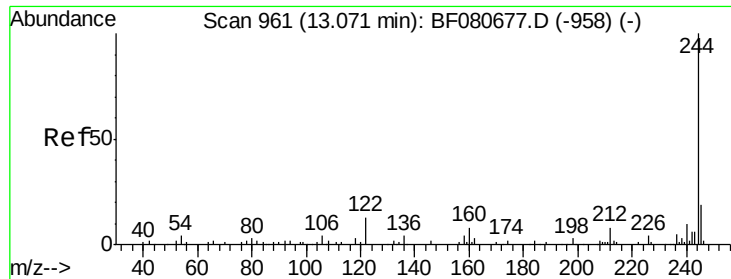

#78
 Terphenyl-d14
 Concen: 83.65 ng
 RT: 13.05 min Scan# 959
 Delta R.T. -0.02 min
 Lab File: BF080688.D
 Acq: 28 Jul 2015 00:04

Instrument :
 BNA_F
 ClientSampleId :
 PB84659BL

Tot Ion	Ratio	Lower	Upper
244	100		
212	7.3	6.1	9.1
122	9.0	10.2	15.2

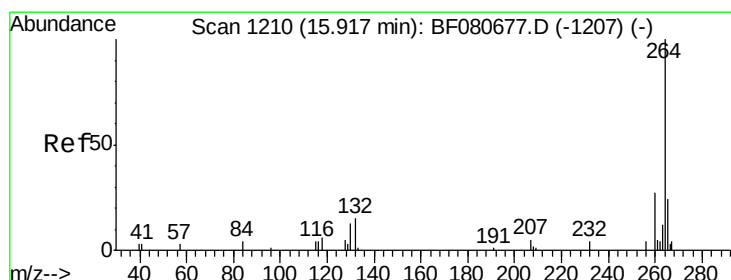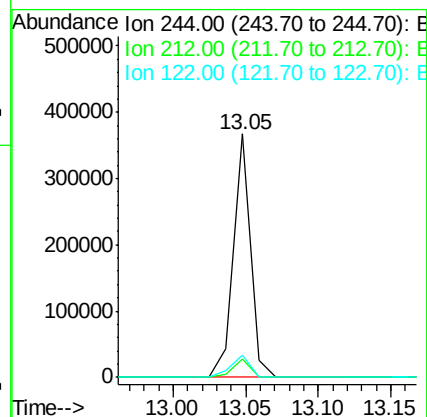

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.76 min Scan# 1196
 Delta R.T. -0.16 min
 Lab File: BF080688.D
 Acq: 28 Jul 2015 00:04

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.0	21.6	32.4
265	20.8	19.3	28.9

