


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072715\
 Data File : BF080682.D
 Acq On : 27 Jul 2015 20:09
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 28 15:18:55 2015

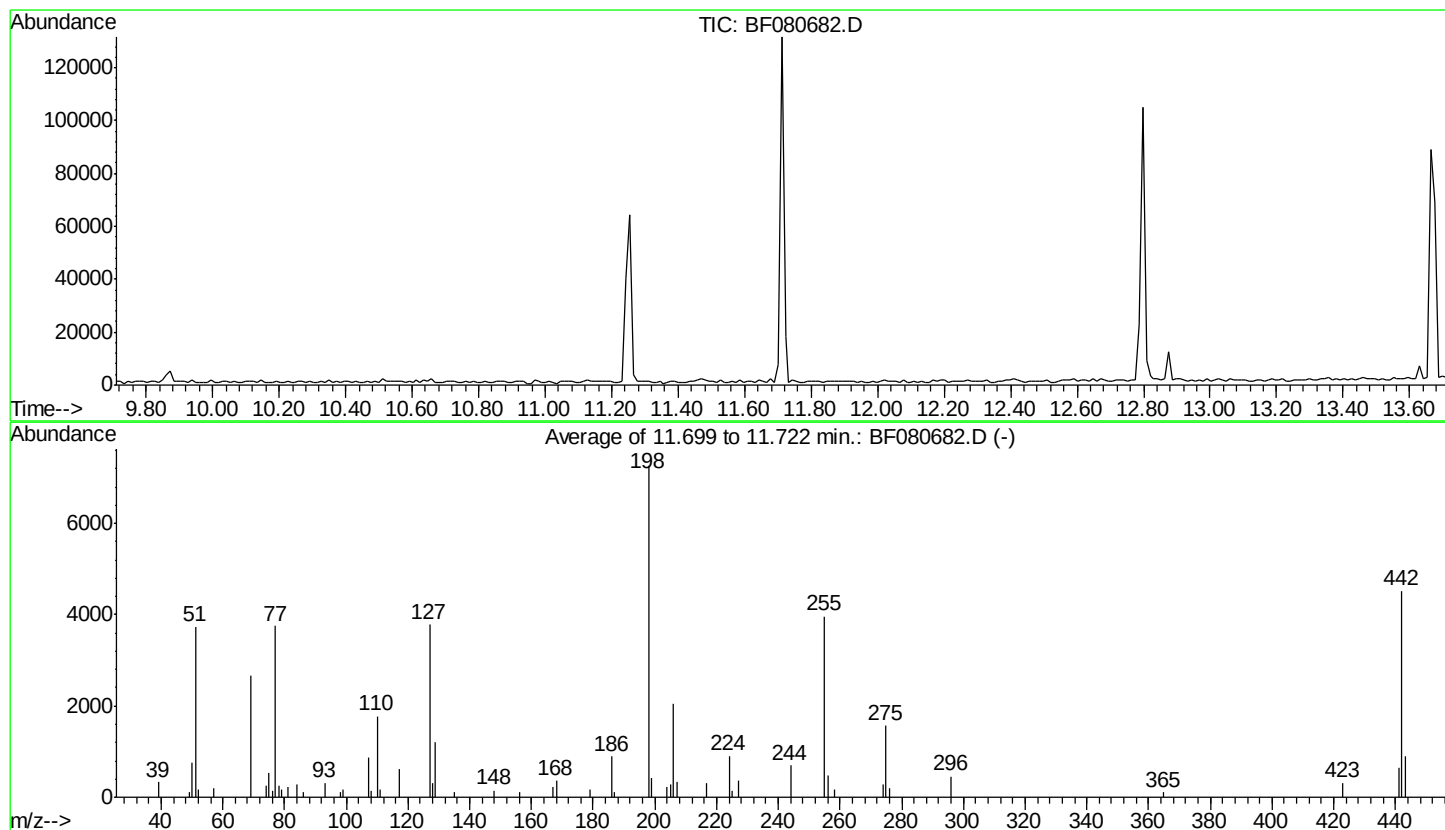

AutoFind: Scans 841, 842, 843; Background Corrected with Scan 838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	3731	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.7	2664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	3782	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7267	PASS
199	198	5	9	5.8	420	PASS
275	198	10	60	21.6	1567	PASS
365	198	1	100	1.4	101	PASS
441	442	0.01	24	14.0	633	PASS
442	198	50	100	62.3	4527	PASS
443	442	15	24	19.6	888	PASS