
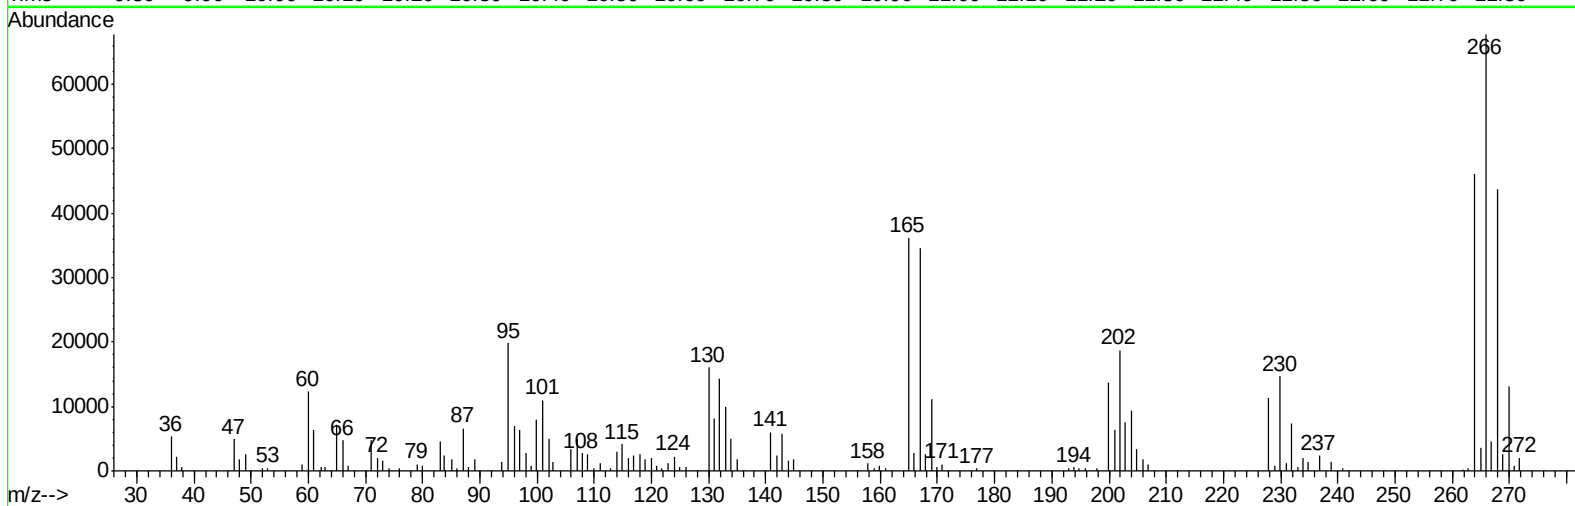


Data Path : Z:\HPCHEM1\BNA F\DATA\BF072717\
Data File : BF097117.D
Acq On : 27 Jul 2017 12:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 04:23:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

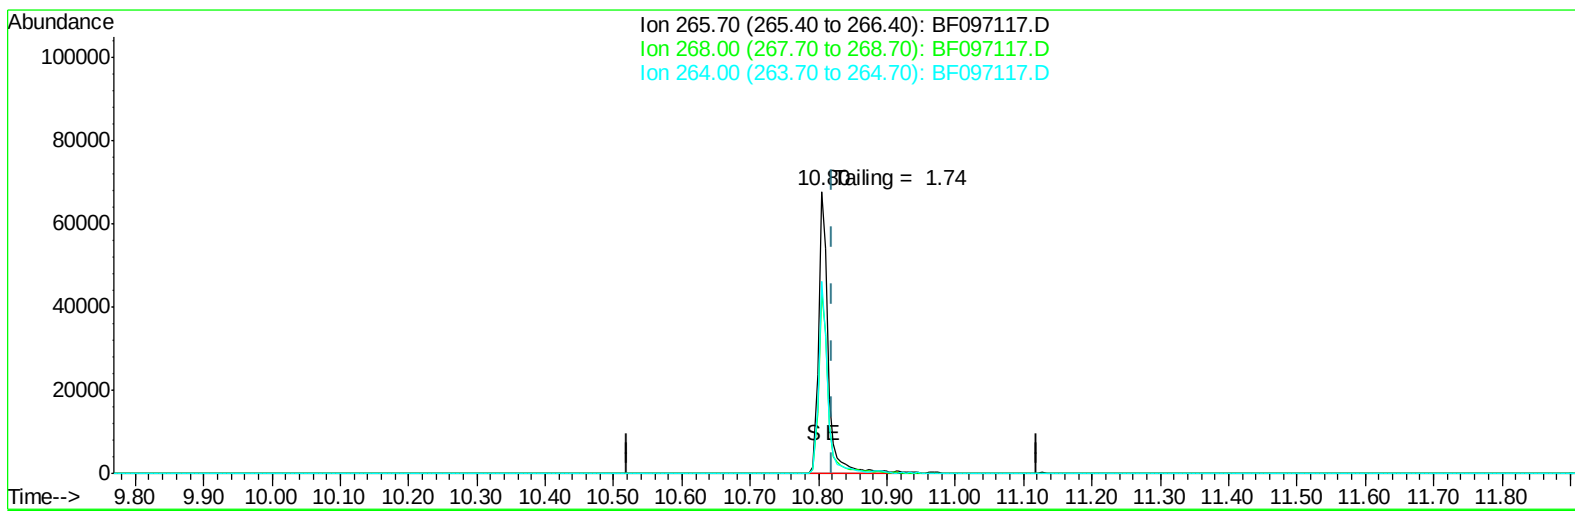

TIC: BF097117.D

(69) Pentachlorophenol (C)



10.804min (-0.017) 0.00ng

response 67062

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.52
264.00	64.60	67.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072717\
Data File : BF097117.D
Acq On : 27 Jul 2017 12:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 04:23:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

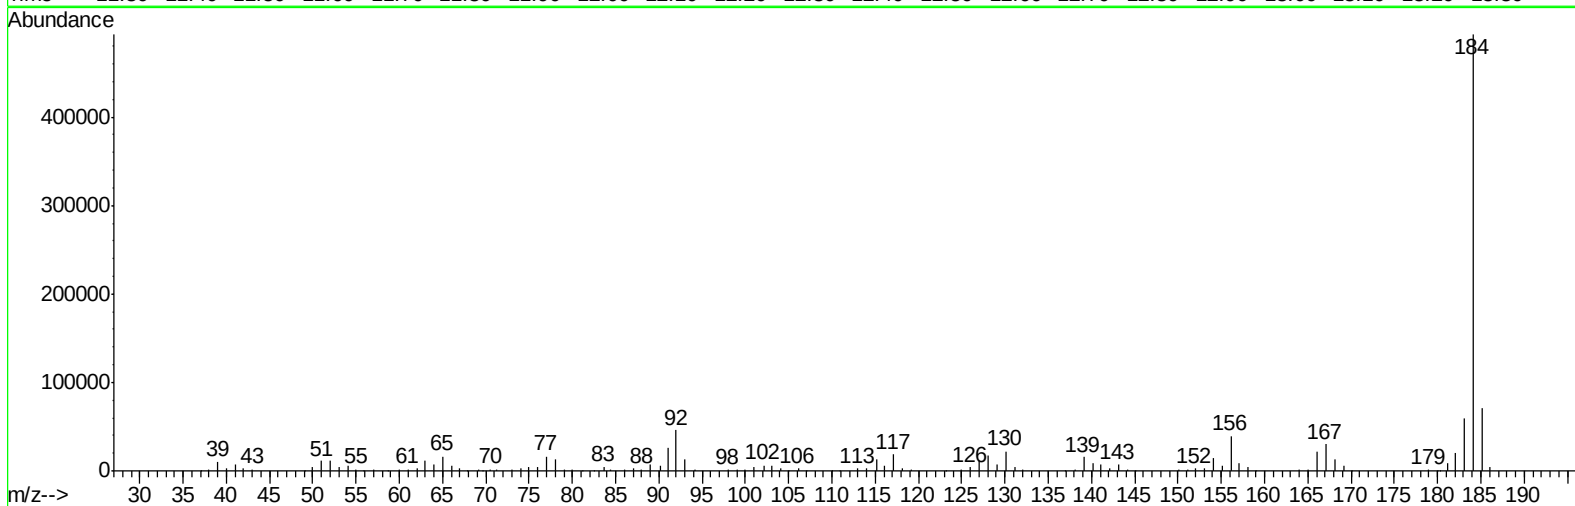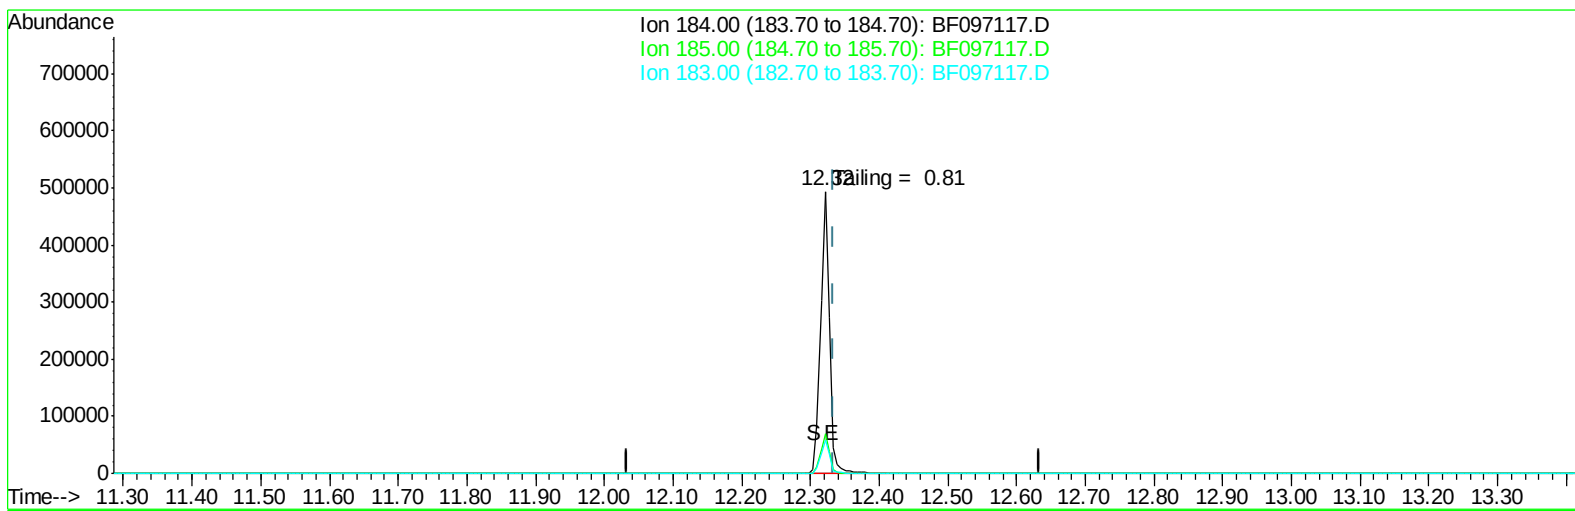

TIC: BF097117.D

(76) Benzidine

12.321min (-0.012) 38382.63ng

response 441496

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.32#
183.00	12.20	12.01
0.00	0.00	0.00