

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072717\
 Data File : BF097135.D
 Acq On : 27 Jul 2017 21:09
 Operator : SJ/JU
 Sample : I4422-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-12018-COMP

Quant Time: Jul 28 01:44:54 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 14:11:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.49	152	96579	20.00	ng	-0.01
21) Naphthalene-d8	7.77	136	421521	20.00	ng	-0.02
38) Acenaphthene-d10	9.51	164	161905	20.00	ng	-0.02
63) Phenanthrene-d10	10.99	188	257465	20.00	ng	-0.02
75) Chrysene-d12	13.61	240	205745	20.00	ng	-0.02
86) Perylene-d12	14.96	264	200383	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.09	112	658984	102.86	ng	-0.01
7) Phenol-d6	6.15	99	765088	104.61	ng	-0.02
23) Nitrobenzene-d5	7.05	82	415585	57.84	ng	-0.02
41) 2,4,6-Tribromophenol	10.30	330	128192	100.21	ng	-0.02
44) 2-Fluorobiphenyl	8.85	172	744530	78.04	ng	-0.02
78) Terphenyl-d14	12.57	244	467114	46.29	ng	-0.02
Target Compounds						
10) Phenol	6.16	94	24627	2.839	ng	Qvalue # 62
49) Dimethylphthalate	9.25	163	97484	7.929	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072717\
Data File : BF097135.D
Acq On : 27 Jul 2017 21:09
Operator : SJ/JU
Sample : I4422-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-12018-COMP

Quant Time: Jul 28 01:44:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

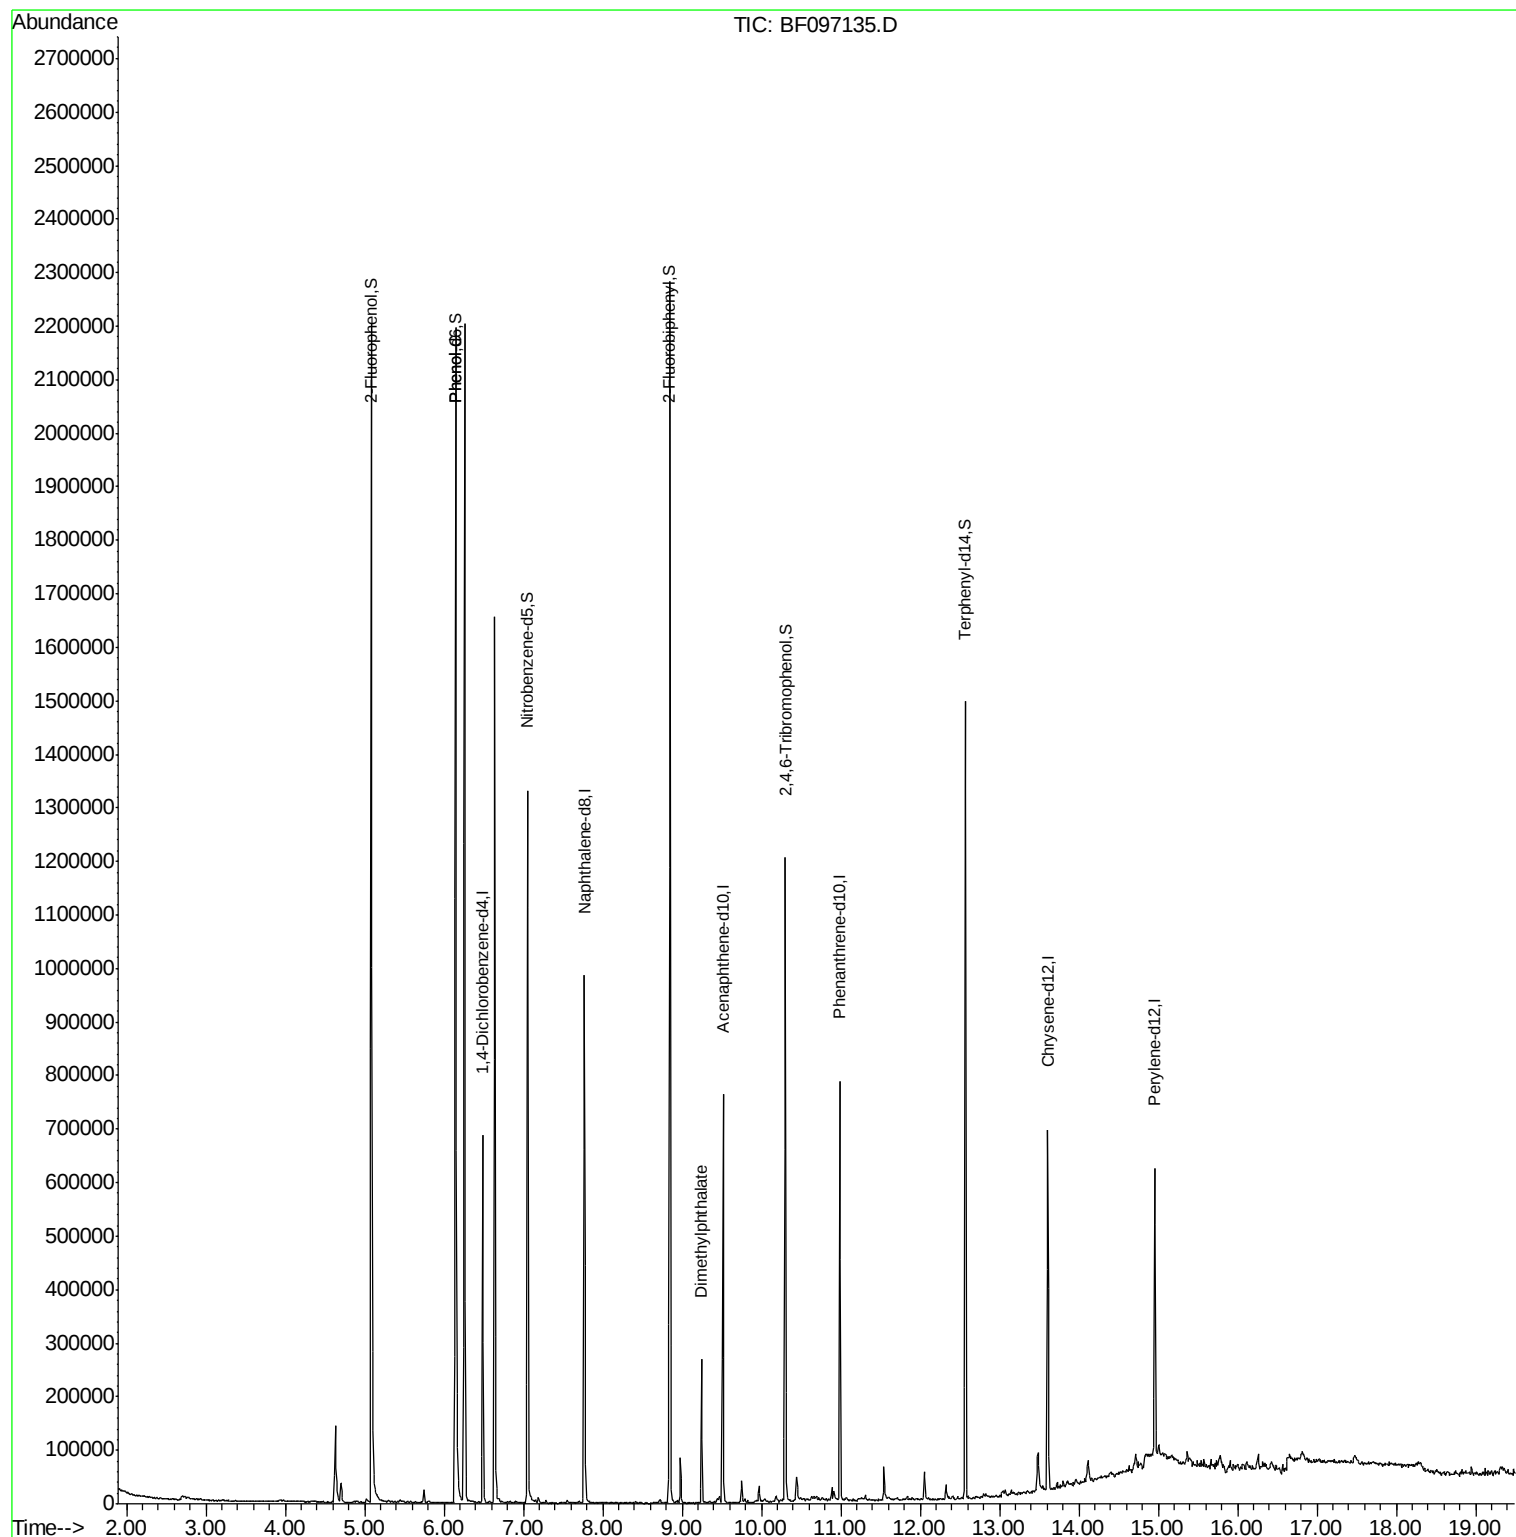




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.49 min Scan# 782
 Delta R.T. -0.01 min
 Lab File: BF097135.D
 Acq: 27 Jul 2017 21:09

Instrument :
 BNA_F
 ClientSampleId :
 72-12018-COMP

Tot Ion:152 Resp: 96579
 Ion Ratio Lower Upper
 152 100
 150 155.6 126.2 189.2
 115 63.1 52.2 78.2

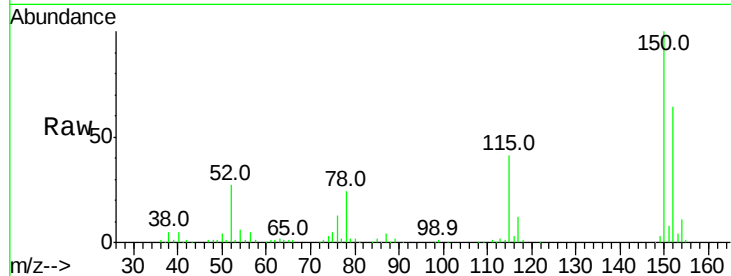


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

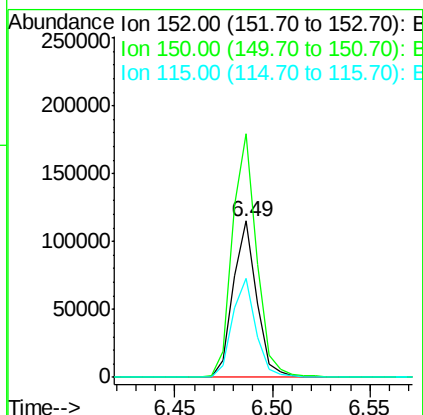



#5


2-Fluorophenol
 Concen: 102.860 ng
 RT: 5.09 min Scan# 544
 Delta R.T. -0.01 min
 Lab File: BF097135.D
 Acq: 27 Jul 2017 21:09

Tgt Ion:112 Resp: 658984
 Ion Ratio Lower Upper
 112 100
 64 65.3 46.0 69.0
 63 32.9 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

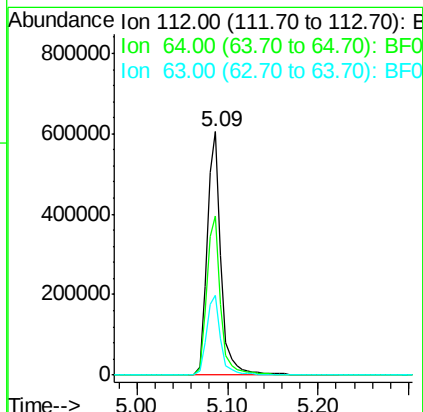

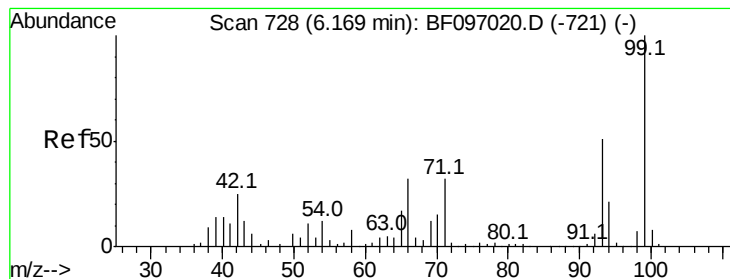

#7

Phenol-d6

Concen: 104.607 ng

RT: 6.15 min Scan# 725

Delta R.T. -0.02 min

Lab File: BF097135.D

Acq: 27 Jul 2017 21:09

Instrument :

BNA_F

ClientSampleId :

72-12018-COMP


Tot Ion: 99 Resp: 765088

Ion Ratio Lower Upper

99 100

42 22.8 13.5 20.3#

71 32.3 24.5 36.7

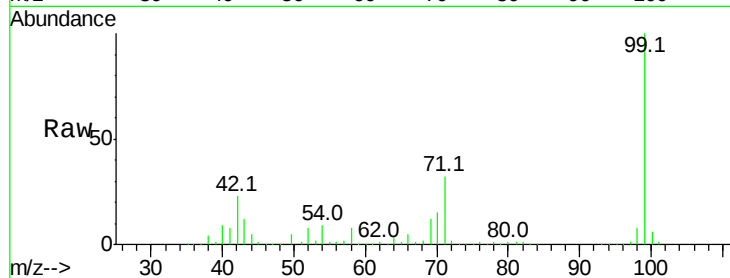

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

6.15

800000



600000

400000

200000

0

Time-->

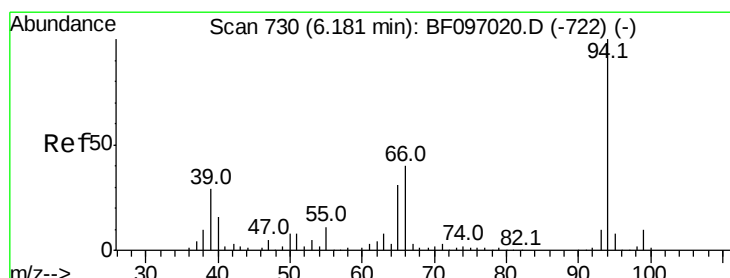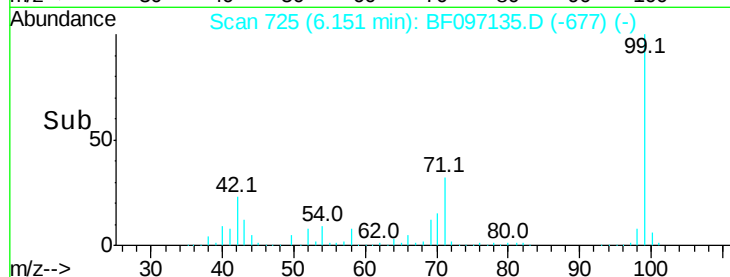

#10

Phenol

Concen: 2.839 ng

RT: 6.16 min Scan# 726

Delta R.T. -0.02 min

Lab File: BF097135.D

Acq: 27 Jul 2017 21:09


Tgt Ion: 94 Resp: 24627

Ion Ratio Lower Upper

94 100

65 40.0 9.9 49.9

66 75.7 23.1 63.1#

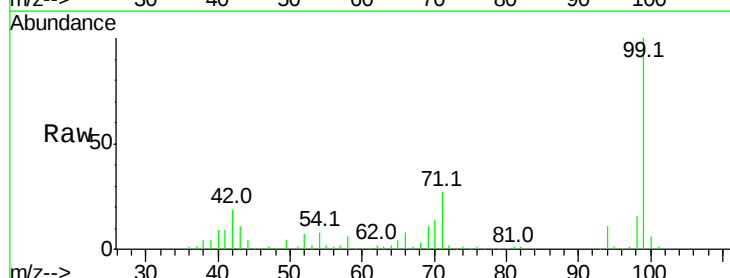

Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

200000


150000

100000

50000

0

Time-->

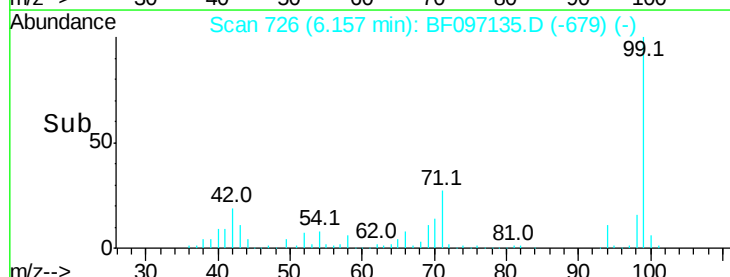



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.77 min Scan# 1000

Delta R.T. -0.02 min

Lab File: BF097135.D

Acq: 27 Jul 2017 21:09

Instrument :

BNA_F

ClientSampleId :

72-12018-COMP

Tot Ion:136 Resp: 421521


Ion Ratio Lower Upper

136 100

137 10.7 8.5 12.7

54 10.1 4.9 7.3#

68 5.2 4.1 6.1



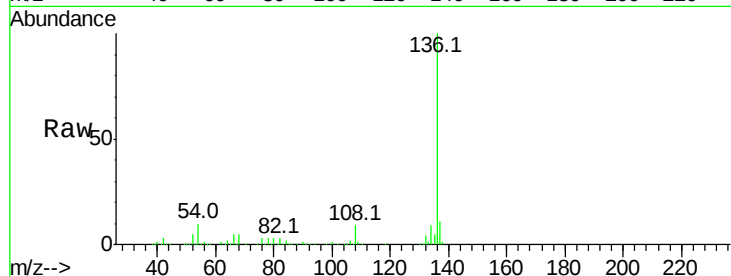


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

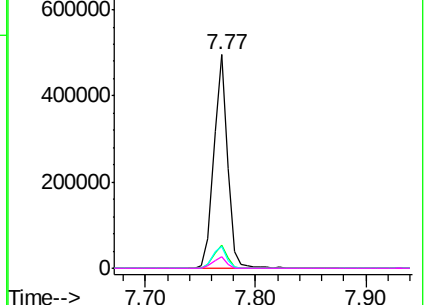

#23

Nitrobenzene-d5

Concen: 57.838 ng

RT: 7.05 min Scan# 878

Delta R.T. -0.02 min

Lab File: BF097135.D

Acq: 27 Jul 2017 21:09


Tgt Ion: 82 Resp: 415585

Ion Ratio Lower Upper

82 100

128 45.7 34.0 51.0



54 69.4 42.2 63.2#



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

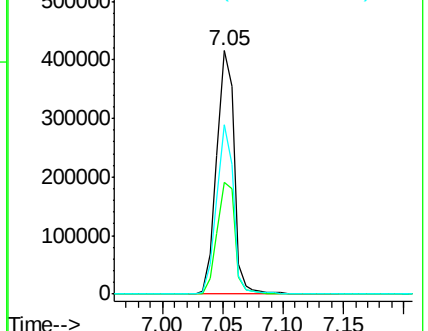







#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.51 min Scan# 1296
Delta R.T. -0.02 min
Lab File: BF097135.D
Acq: 27 Jul 2017 21:09

Instrument :
BNA_F
ClientSampleId :
72-12018-COMP

Tot Ion:164 Resp: 161905
Ion Ratio Lower Upper
164 100
162 105.2 82.6 123.8
160 46.0 36.2 54.2

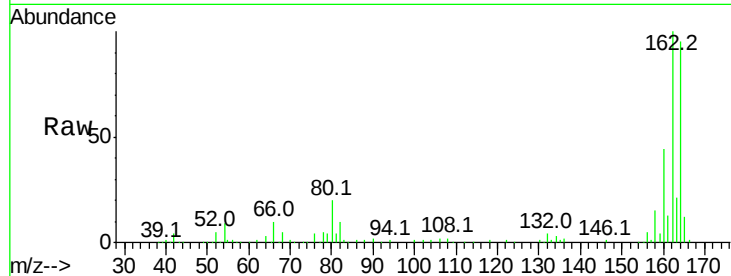


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

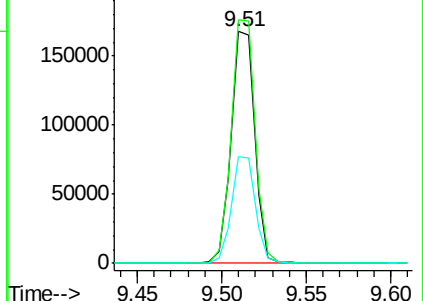
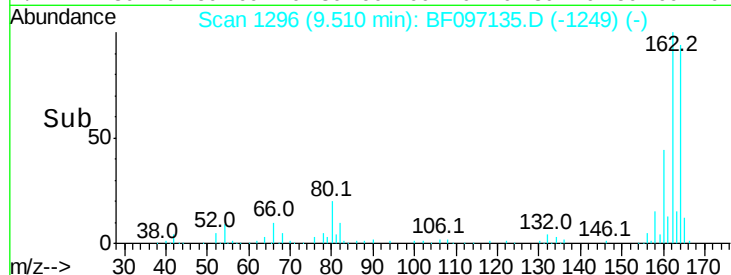


#41
2,4,6-Tribromophenol
Concen: 100.212 ng
RT: 10.30 min Scan# 1430
Delta R.T. -0.02 min
Lab File: BF097135.D
Acq: 27 Jul 2017 21:09

Tgt Ion:330 Resp: 128192
Ion Ratio Lower Upper
330 100
332 93.7 76.6 115.0
141 39.1 31.4 47.2



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



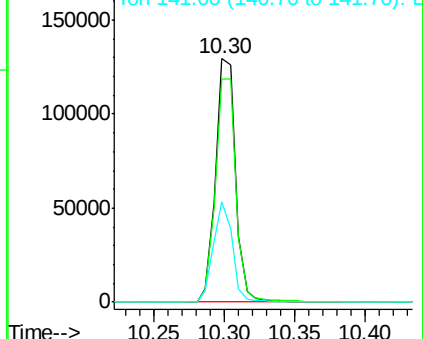





#44
2-Fluorobiphenyl
Concen: 78.042 ng
RT: 8.85 min Scan# 1183
Delta R.T. -0.02 min
Lab File: BF097135.D
Acq: 27 Jul 2017 21:09




Instrument :
BNA_F
ClientSampleId :
72-12018-COMP


Tot Ion:172 Resp: 744530
Ion Ratio Lower Upper
172 100
171 36.1 29.6 44.4
170 24.4 19.8 29.8

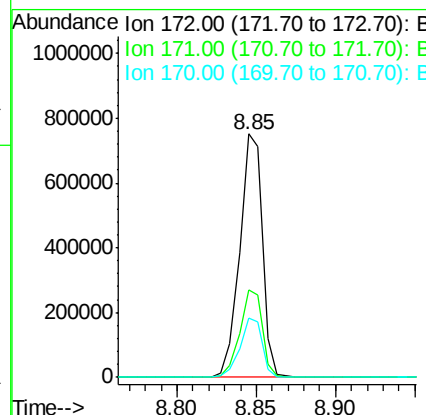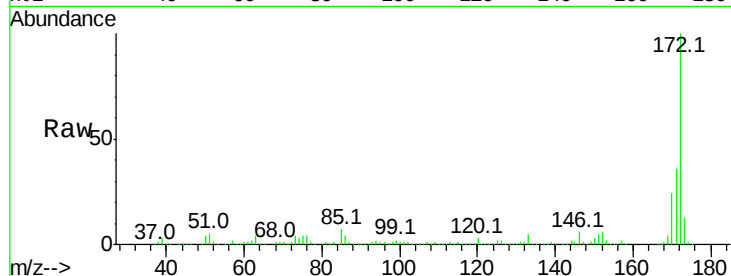

#49
Dimethylphthalate
Concen: 7.929 ng
RT: 9.25 min Scan# 1251
Delta R.T. -0.03 min
Lab File: BF097135.D
Acq: 27 Jul 2017 21:09

Tgt Ion:163 Resp: 97484
Ion Ratio Lower Upper
163 100
194 2.9 2.6 4.0
164 9.9 8.4 12.6

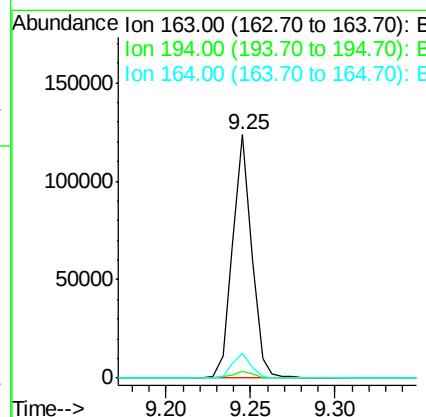







#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 10.99 min Scan# 1547
Delta R.T. -0.02 min
Lab File: BF097135.D
Acq: 27 Jul 2017 21:09

Instrument :
BNA_F
ClientSampleId :
72-12018-COMP

Tot Ion:188 Resp: 257465
Ion Ratio Lower Upper
188 100
94 12.0 9.4 14.2
80 11.7 10.2 15.2

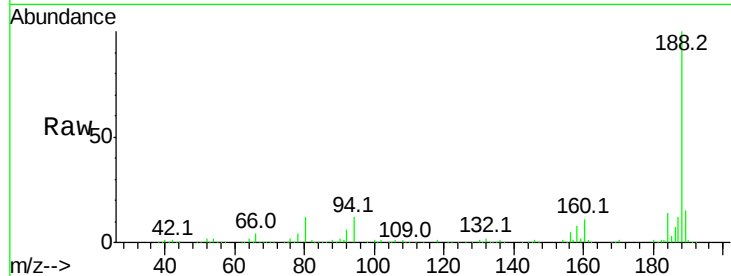


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


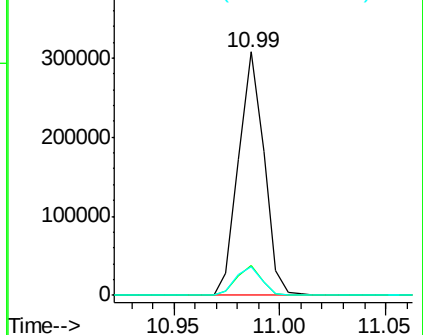



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.61 min Scan# 1993
Delta R.T. -0.02 min
Lab File: BF097135.D
Acq: 27 Jul 2017 21:09

Tgt Ion:240 Resp: 205745
Ion Ratio Lower Upper
240 100
120 14.5 5.8 8.8#
236 26.4 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

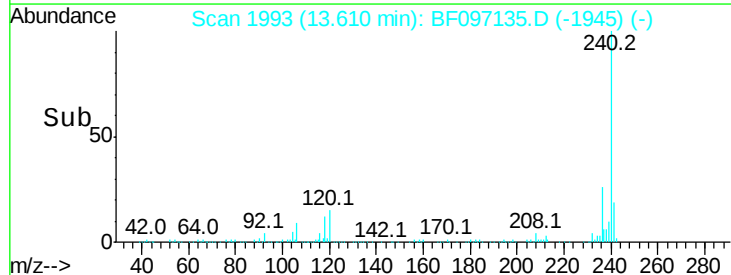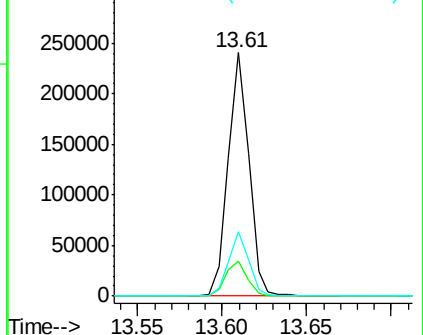

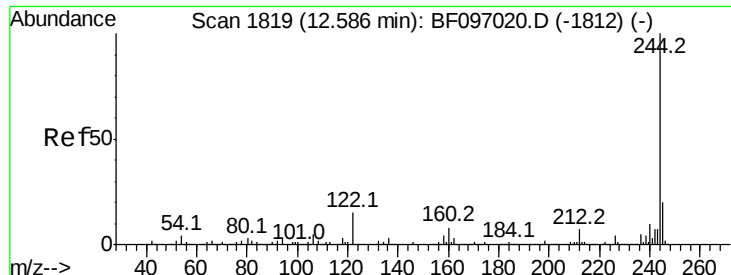

#78

Terphenyl-d14

Concen: 46.289 ng

RT: 12.57 min Scan# 1816

Delta R.T. -0.02 min

Lab File: BF097135.D

Acq: 27 Jul 2017 21:09

Instrument :

BNA_F

ClientSampleId :

72-12018-COMP


Tot Ion:244 Resp: 467114

Ion Ratio Lower Upper

244 100

212 6.3 6.0 9.0

122 16.1 10.3 15.5#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

12.57

400000

300000



200000

100000

0

12.55 12.60

Time-->



#86

Perylene-d12

Concen: 20.000 ng

RT: 14.96 min Scan# 2222

Delta R.T. -0.02 min

Lab File: BF097135.D

Acq: 27 Jul 2017 21:09


Tgt Ion:264 Resp: 200383

Ion Ratio Lower Upper

264 100

260 24.2 19.5 29.3

265 21.5 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

14.96

200000

150000

100000

50000

0

14.90 15.00

Time-->

