

Data Path : Z:\HPCHEM1\BNA F\DATA\BF072717\
 Data File : BF097119.D
 Acq On : 27 Jul 2017 13:43
 Operator : SJ/JU
 Sample : I4415-01RE
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-072417RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.616	460	464	472	rBV	142651	200507	4.19%	0.709%
2	5.081	539	543	556	rBV	1564350	2096379	43.82%	7.416%
3	5.181	556	560	572	rVB	103052	225796	4.72%	0.799%
4	6.151	721	725	736	rBV	2027305	2129156	44.51%	7.531%
5	6.257	739	743	754	rVB	2049802	2040399	42.65%	7.218%
6	6.487	778	782	786	rBV	662441	553836	11.58%	1.959%
7	6.640	804	808	815	rBV	1732480	1572682	32.88%	5.563%
8	7.051	874	878	881	rBV	1386773	1325940	27.72%	4.690%
9	7.769	996	1000	1004	rBV	942673	760867	15.91%	2.691%
10	8.845	1179	1183	1186	rBV	2204245	1915083	40.03%	6.774%
11	9.245	1248	1251	1253	rBV	232878	169901	3.55%	0.601%
12	9.469	1285	1289	1293	rBV2	74162	96688	2.02%	0.342%
13	9.510	1293	1296	1300	rVB	706576	611960	12.79%	2.165%
14	9.757	1333	1338	1341	rVB2	86490	95630	2.00%	0.338%
15	9.969	1371	1374	1377	rVB	61353	55188	1.15%	0.195%
16	10.192	1406	1412	1414	rBV2	40633	58563	1.22%	0.207%
17	10.233	1414	1419	1423	rVV2	48810	85523	1.79%	0.303%
18	10.298	1426	1430	1435	rVB	1012256	902927	18.87%	3.194%
19	10.439	1447	1454	1455	rBV2	66892	90256	1.89%	0.319%
20	10.586	1474	1479	1480	rBV3	42344	60024	1.25%	0.212%
21	10.657	1488	1491	1495	rBV	68148	98102	2.05%	0.347%
22	10.692	1495	1497	1501	rVB2	55981	50070	1.05%	0.177%
23	10.880	1525	1529	1532	rBV	52171	53562	1.12%	0.189%
24	10.986	1543	1547	1549	rBV	530648	471390	9.85%	1.667%
25	11.410	1614	1619	1624	rBV7	29346	56663	1.18%	0.200%
26	11.510	1630	1636	1638	rBV2	644579	990559	20.71%	3.504%
27	11.545	1638	1642	1648	rVV	1008047	1878287	39.26%	6.644%
28	11.592	1648	1650	1660	rVV2	115230	226462	4.73%	0.801%
29	11.680	1662	1665	1668	rVV3	121171	171307	3.58%	0.606%
30	11.716	1668	1671	1676	rVB4	74673	95417	1.99%	0.338%
31	11.869	1693	1697	1702	rBV7	34697	77485	1.62%	0.274%
32	12.033	1722	1725	1727	rBV	45840	48057	1.00%	0.170%
33	12.192	1749	1752	1754	rBV	222795	235924	4.93%	0.835%
34	12.233	1754	1759	1767	rVV3	182024	439695	9.19%	1.555%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072717\
 Data File : BF097119.D
 Acq On : 27 Jul 2017 13:43
 Operator : SJ/JU
 Sample : I4415-01RE
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-02-072417RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.339	1769	1777	1786	rVV	2561126	4783733	100.00%	16.922%
36	12.416	1786	1790	1793	rVB	232395	243891	5.10%	0.863%
37	12.574	1813	1817	1820	rBV	1226634	1233371	25.78%	4.363%
38	12.745	1844	1846	1851	rVB6	49957	59803	1.25%	0.212%
39	13.039	1893	1896	1899	rBV3	69054	83838	1.75%	0.297%
40	13.133	1910	1912	1920	rBV3	146627	233328	4.88%	0.825%
41	13.486	1969	1972	1977	rVB2	264616	298242	6.23%	1.055%
42	13.610	1989	1993	1996	rBV	708195	721011	15.07%	2.550%
43	13.804	2023	2026	2029	rBV	117669	136621	2.86%	0.483%
44	14.257	2100	2103	2106	rVB	189732	191900	4.01%	0.679%
45	14.968	2221	2224	2226	rVB	258342	254107	5.31%	0.899%
46	18.804	2873	2876	2880	rBV4	68840	90005	1.88%	0.318%


Sum of corrected areas: 28270135

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF072717\
Data File : BF097119.D
Acq On : 27 Jul 2017 13:43
Operator : SJ/JU
Sample : I4415-01RE
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-02-072417RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

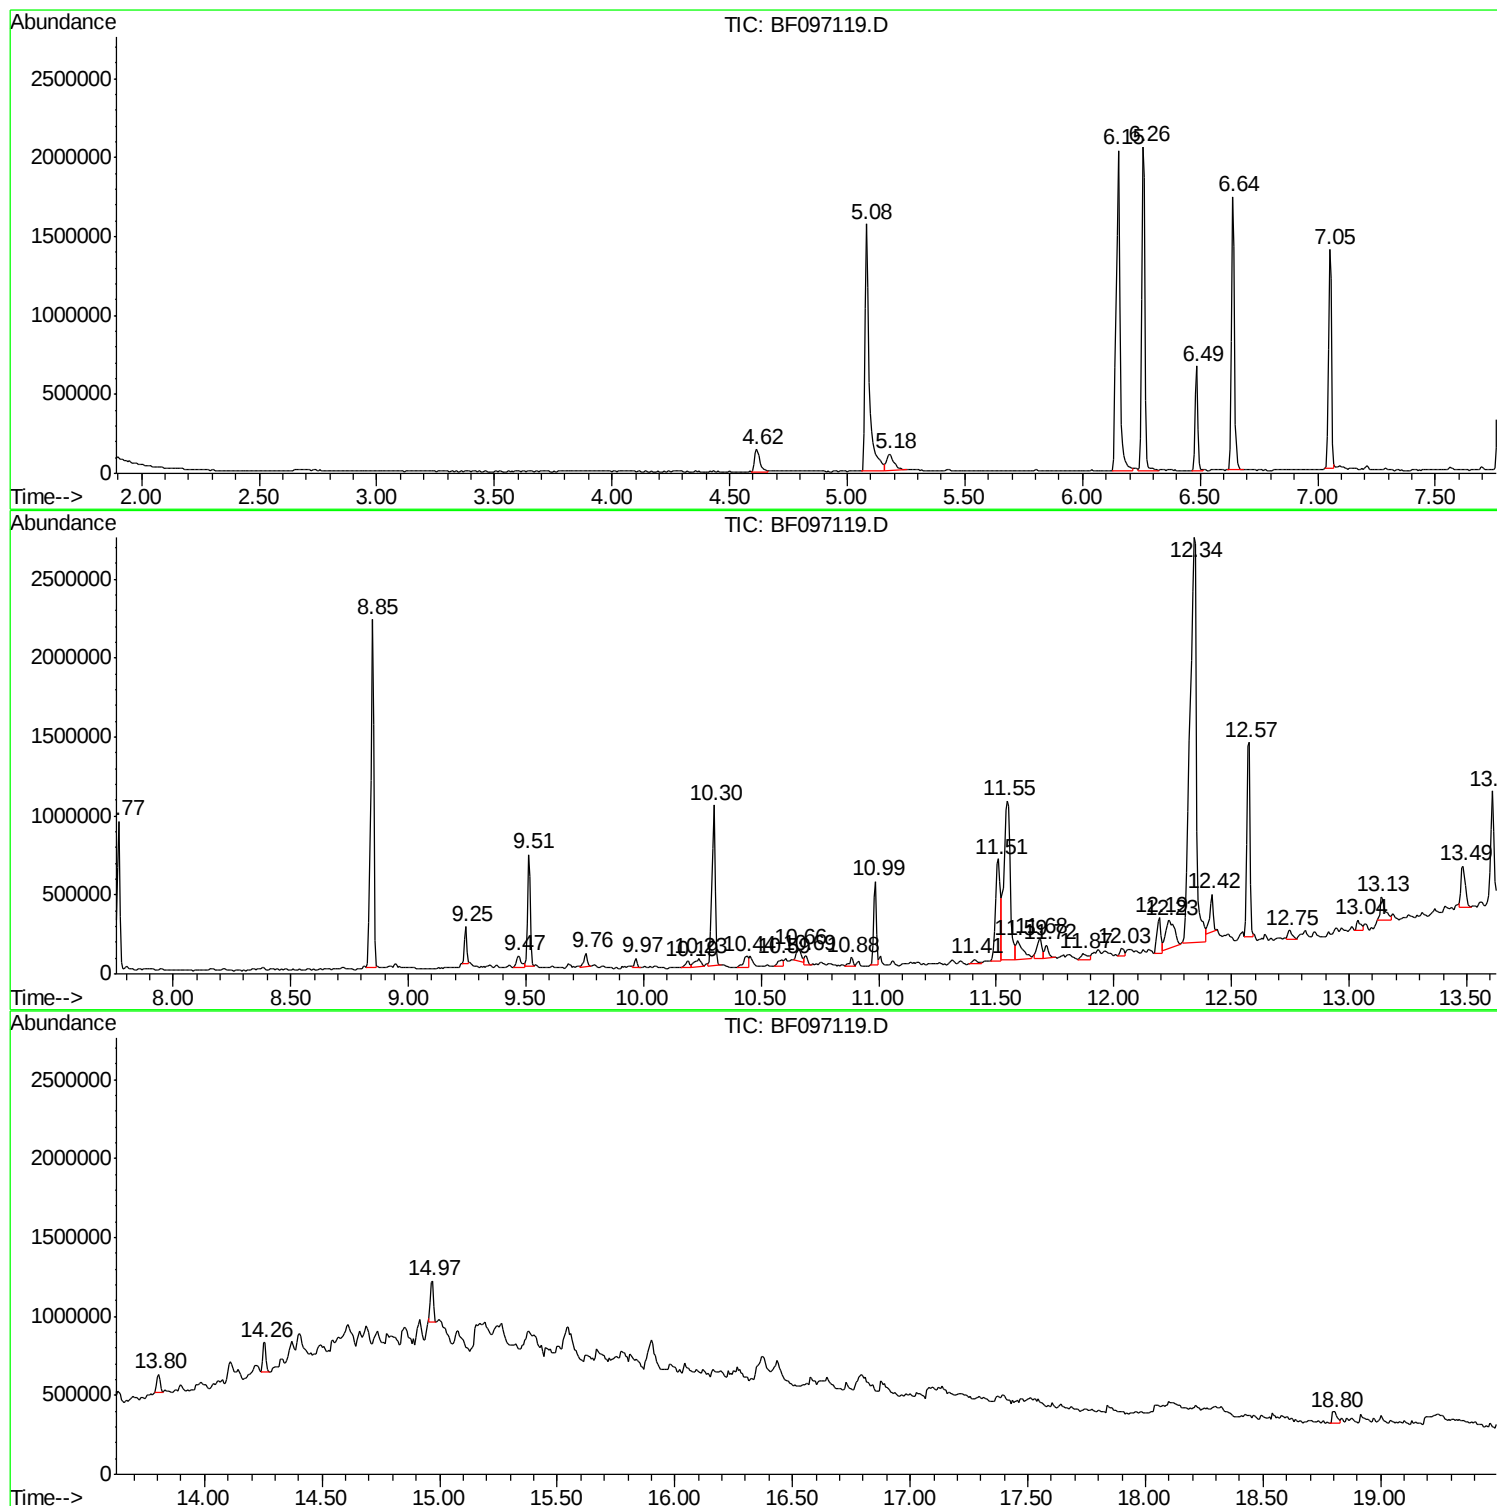

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF072717\
Data_File : BF097119.D
Acq_On : 27 Jul 2017 13:433
Operator : SJ/JUU
Sample : I4415-01REE
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SU-02-072417RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
