


Data Path : Z:\HPCHEM1\BNA F\Data\BF072717\
 Data File : BF097117.D
 Acq On : 27 Jul 2017 12:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 25 14:11:51 2017

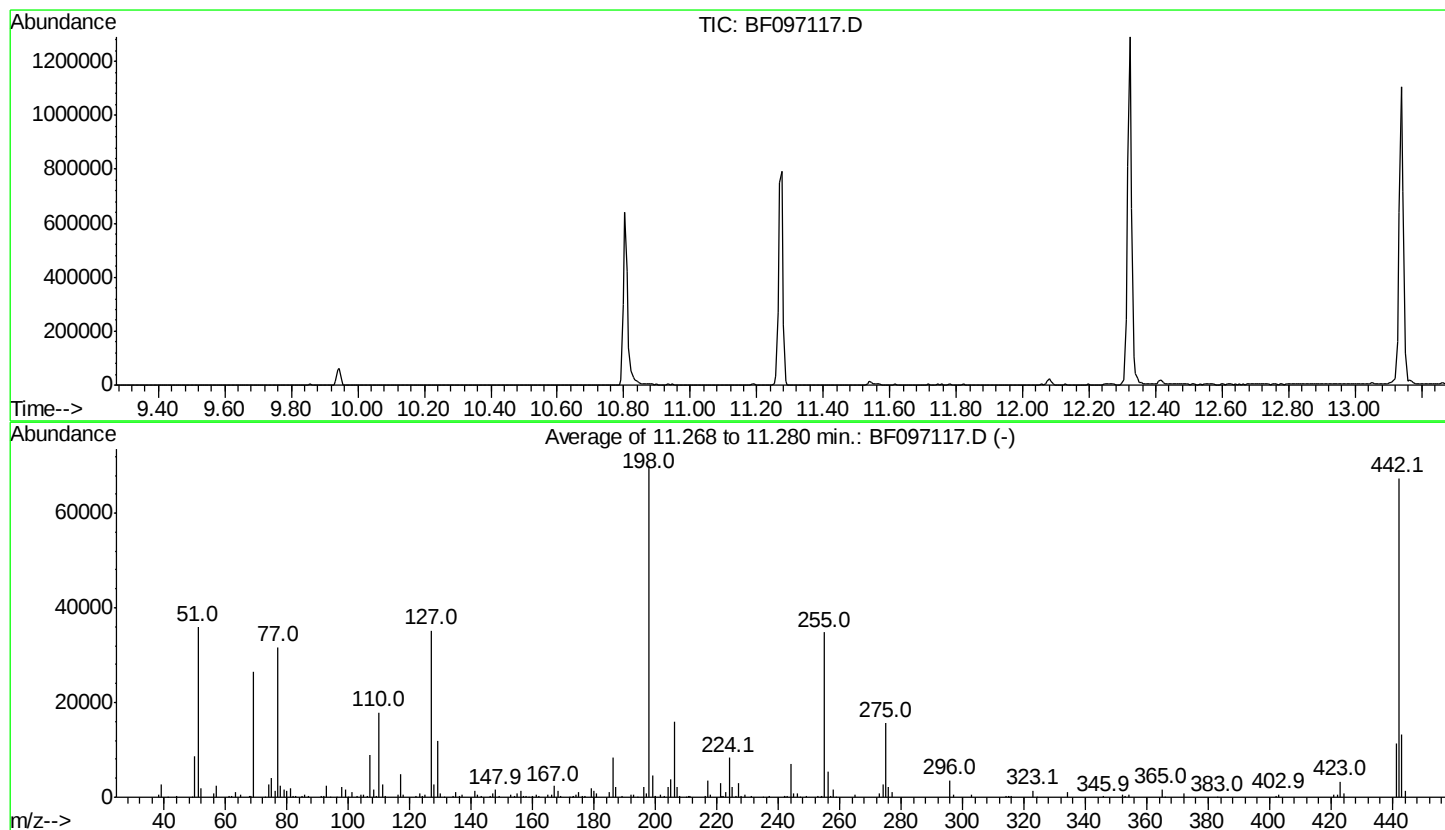

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	36069	PASS
68	69	0.00	2	0.8	210	PASS
69	198	0.00	100	38.0	26631	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	35199	PASS
197	198	0.00	2	1.0	729	PASS
198	198	100	100	100.0	70040	PASS
199	198	5	9	6.5	4545	PASS
275	198	10	60	22.4	15697	PASS
365	198	1	100	2.4	1700	PASS
441	442	0.01	24	16.8	11297	PASS
442	198	50	100	96.3	67421	PASS
443	442	15	24	19.5	13176	PASS