
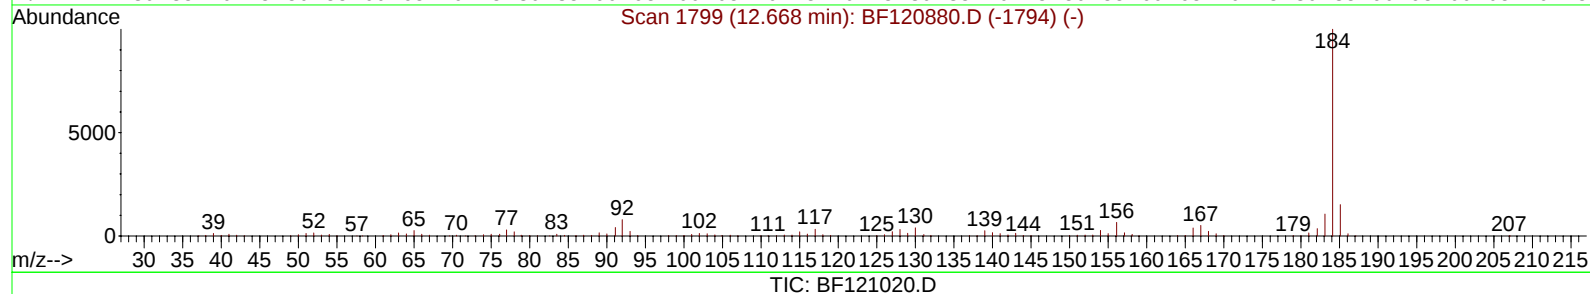
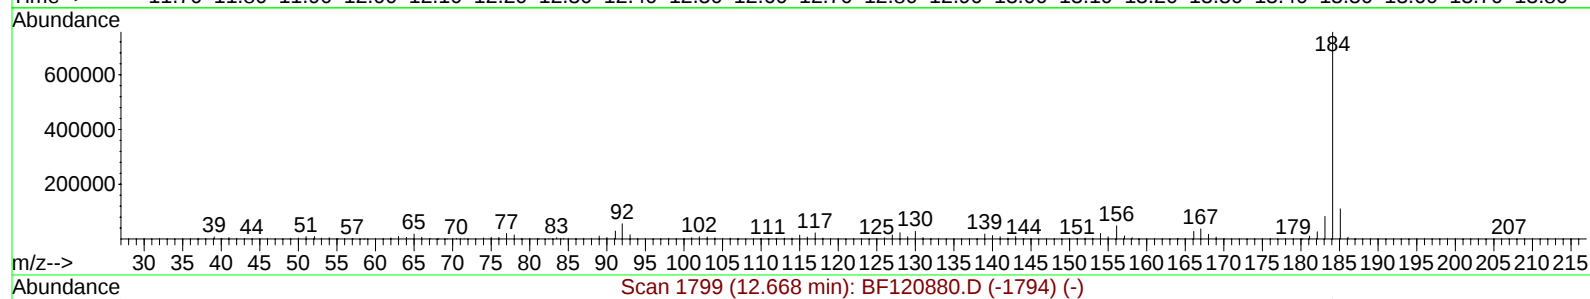


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072720\
 Data File : BF121020.D
 Acq On : 27 Jul 2020 8:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 18:41:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

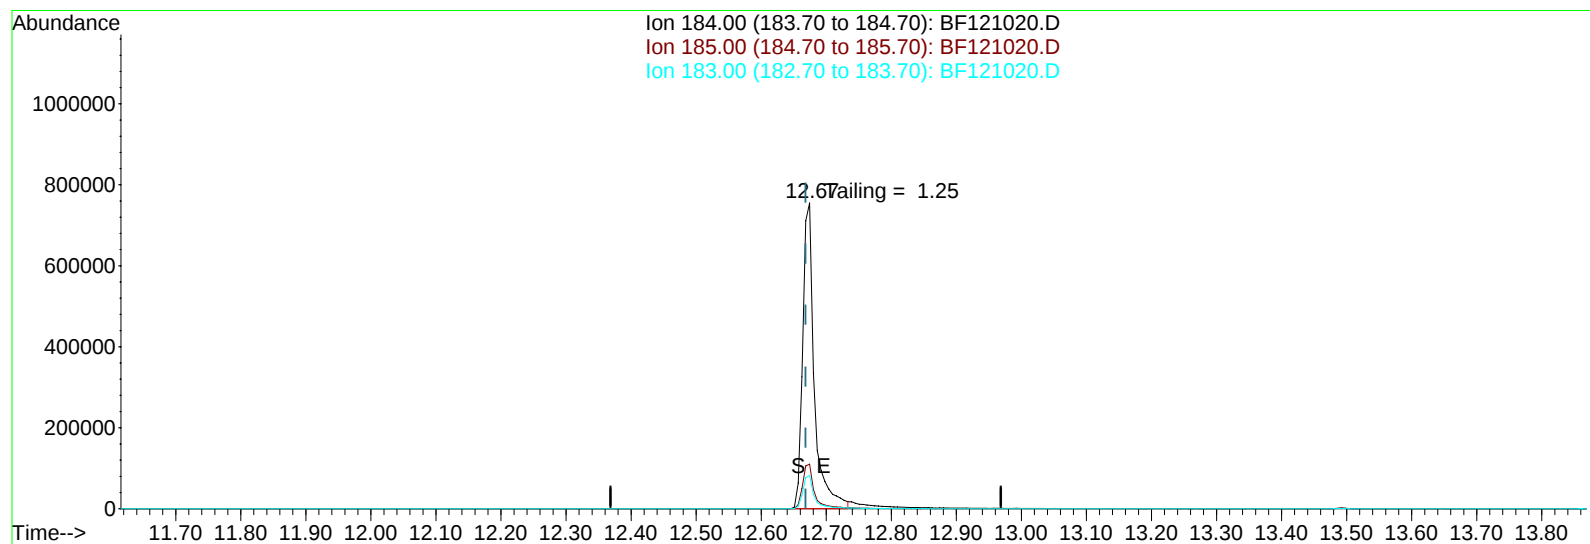

(77) Benzidine




12.674min (+0.006) 142690.80ng

response 994173

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.60
183.00	10.60	10.96
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072720\
Data File : BF121020.D
Acq On : 27 Jul 2020 8:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 18:41:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

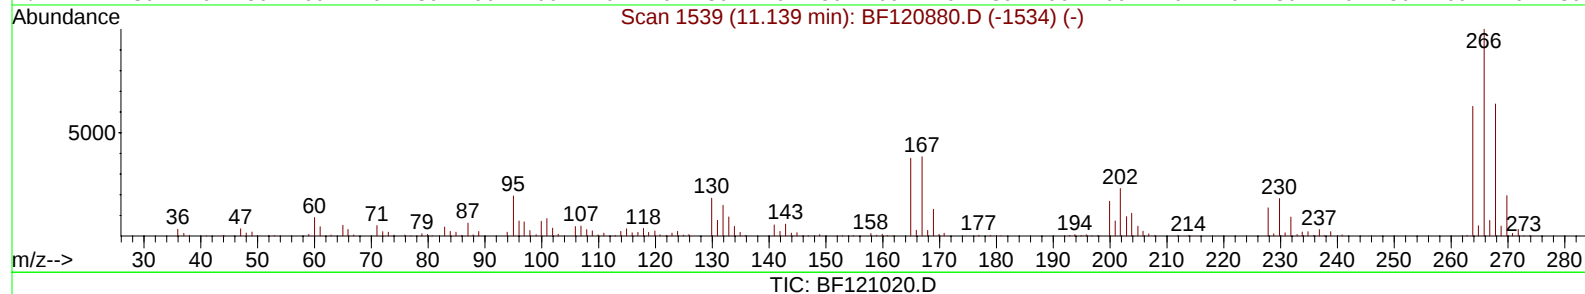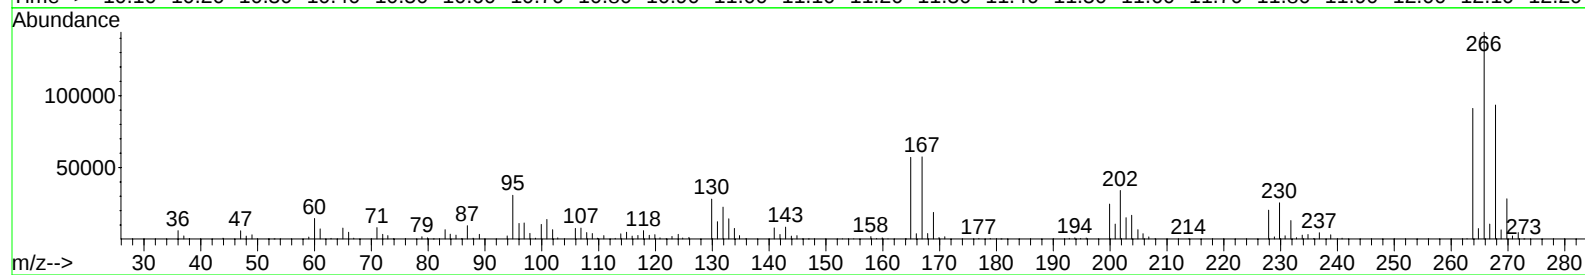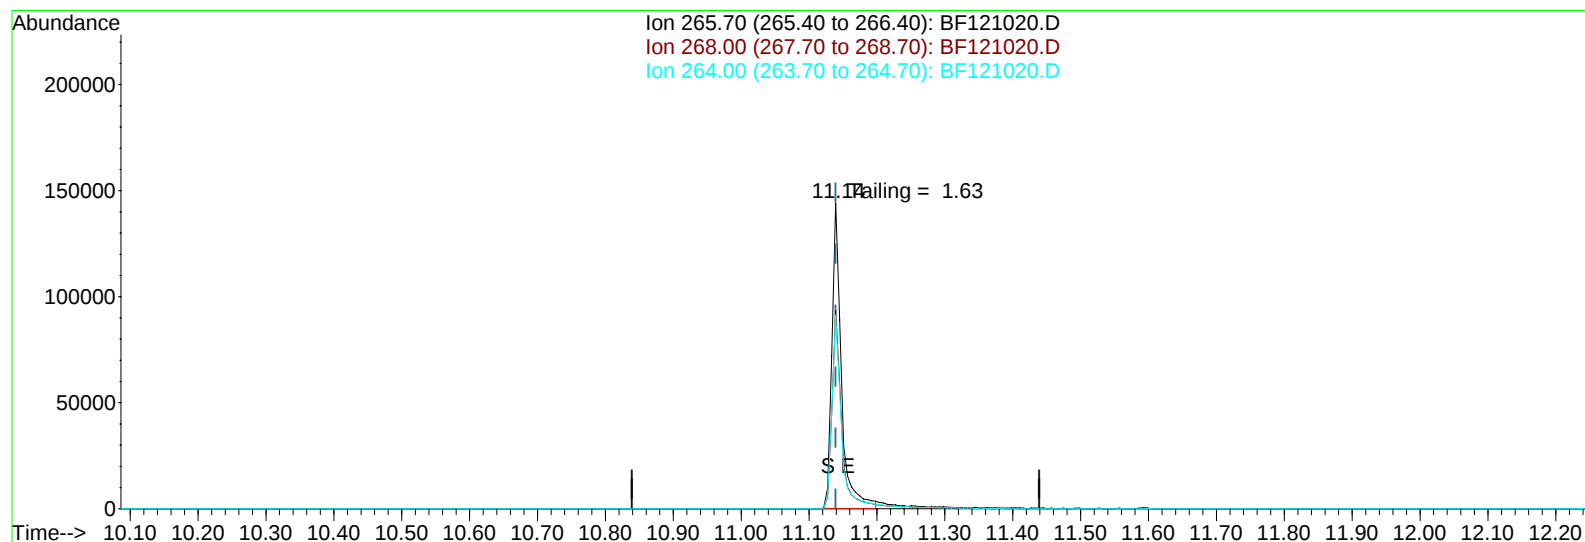

(70) Pentachlorophenol (C)

11.139min (+0.000) 76919.59ng

response 146683

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.86
264.00	62.70	63.24
0.00	0.00	0.00