
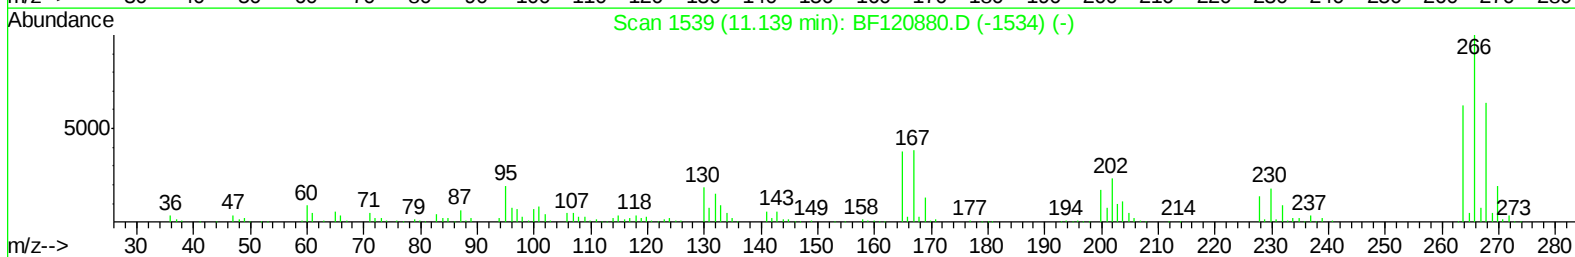
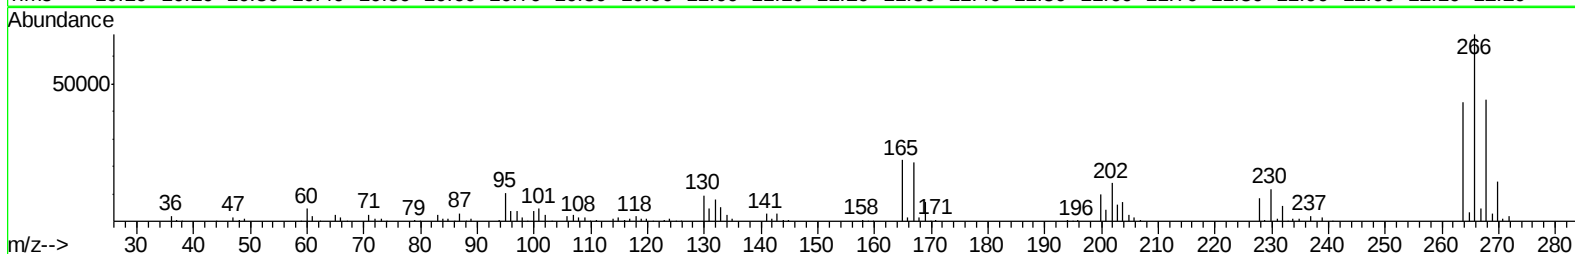


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072720\
Data File : BF121033.D
Acq On : 27 Jul 2020 15:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 01:48:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

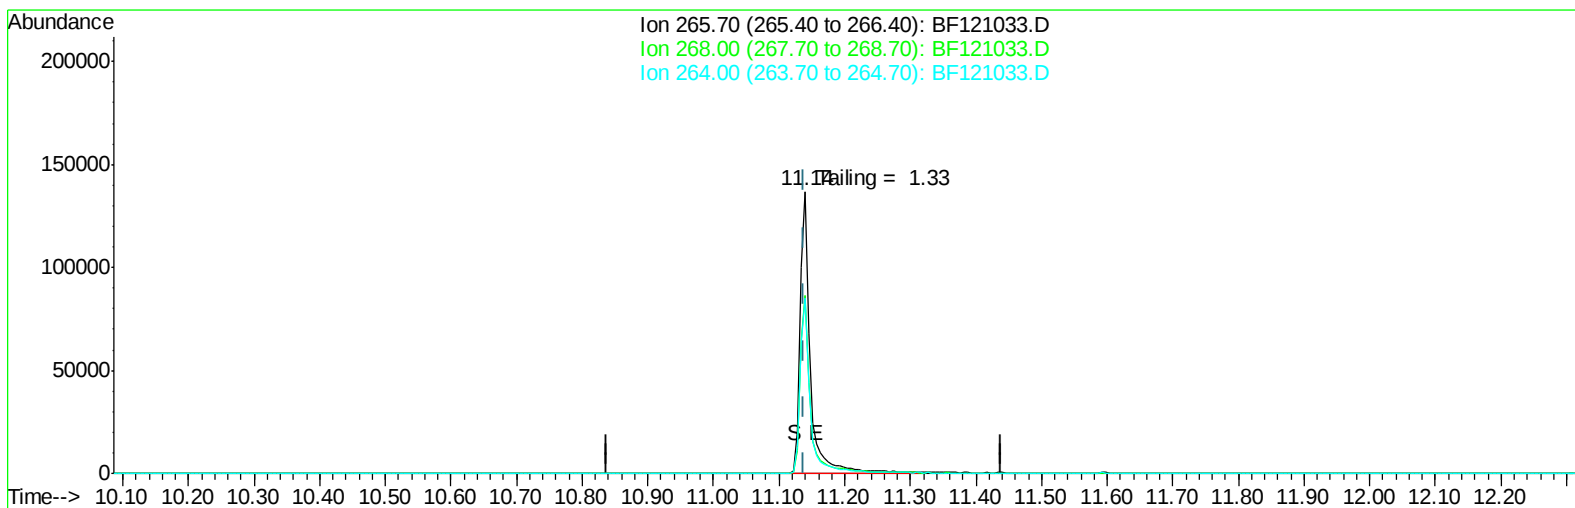

TIC: BF121033.D

(70) Pentachlorophenol (C)




11.139min (+0.000) 163924.32ng

response 150636

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.20
264.00	62.70	62.37
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072720\
Data File : BF121033.D
Acq On : 27 Jul 2020 15:36
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 01:48:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

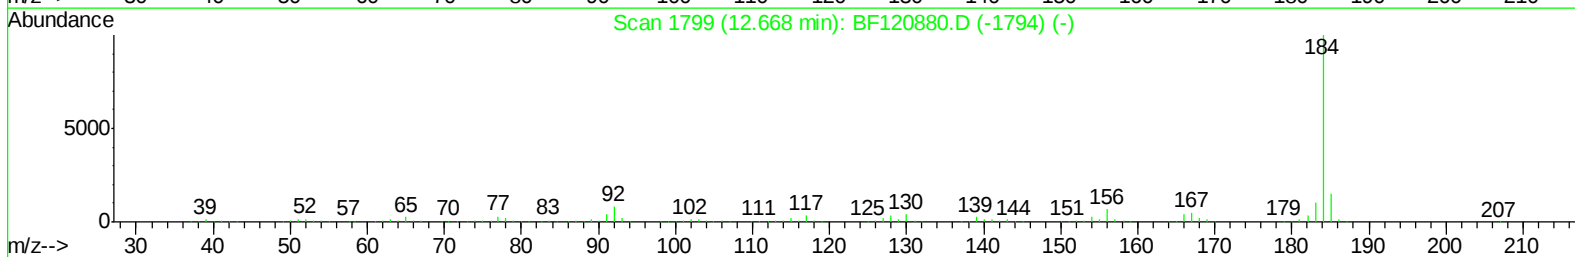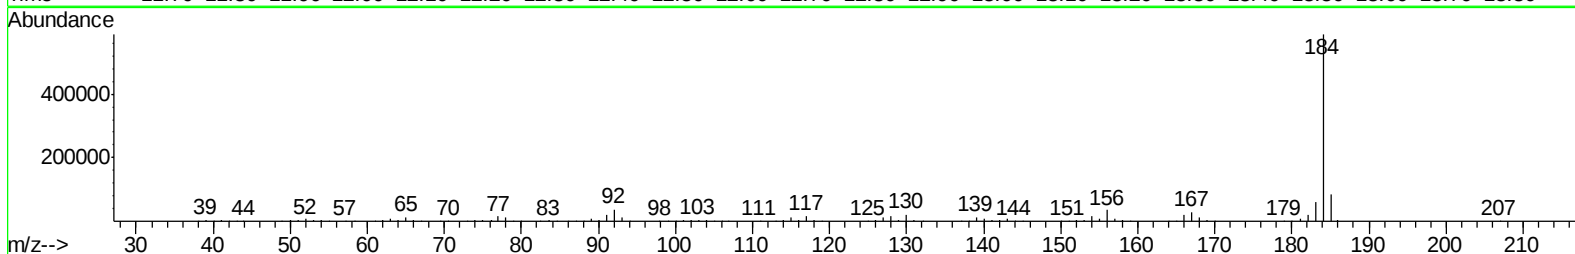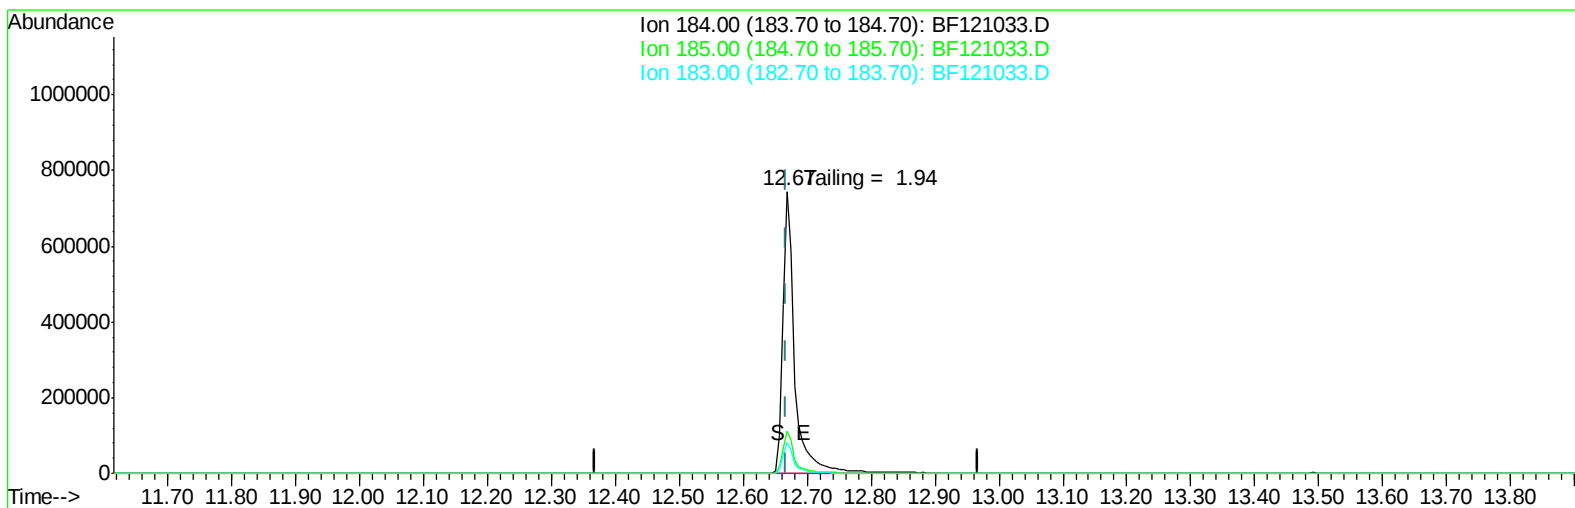

TIC: BF121033.D

(77) Benzidine

12.669min (+0.000) 329283.95ng

response 952321

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.87
183.00	10.60	11.02
0.00	0.00	0.00